

# Spirit<sup>IT</sup> Flow-X

## High accuracy flow computers



Certified flow calculations  
Flow and batch calculations  
Worksheet functions

**Measurement made easy**

—  
Flow-X/P with  
Flow-X/M module

## Introduction

Welcome to the exciting world of Spirit<sup>IT</sup> Flow-X! This document describes the spreadsheet functions for the Spirit<sup>IT</sup> Flow-X series and background information on related standards and calculation methods used in the industry for quality and quantity measurement of hydrocarbon and other type of fluids.

There are three reference manuals:

- Volume I – This Installation manual, with the installation instructions.
- Volume II – The Operation and Configuration manual. This manual consists of a general part and one of the following application-specific parts:
  - IIA - Operation and configuration
  - IIB - Gas Metric application
  - IIC - Liquid Metric application
  - IID - Gas US customary units application
  - IIE - Liquid US customary units application
- Volume III - The manuals for solutions that exceed our standard applications. This volume consists of 1 part:
  - IIIB - Function referencere

## For more information

All publications of Spirit<sup>IT</sup> Flow-X are available for free download from:



| Search for:  |                |
|--|----------------|
| Spirit <sup>IT</sup> Flow-X instruction manual               | IM/FlowX-EN    |
| Spirit <sup>IT</sup> Flow-X configuration manual             | CM/FlowX-EN    |
| Spirit <sup>IT</sup> Flow-X gas metric application manual    | CM/FlowX/GM-EN |
| Spirit <sup>IT</sup> Flow-X liquid metric application manual | CM/FlowX/LM-EN |
| Spirit <sup>IT</sup> Flow-X gas USC application manual       | CM/FlowX/GU-EN |
| Spirit <sup>IT</sup> Flow-X liquid USC application manual    | CM/FlowX/LU-EN |
| Spirit <sup>IT</sup> Flow-X function reference manual        | CM/FlowX/RF-EN |

## Contents

|          |  |          |
|----------|--|----------|
| <b>1</b> | <b>Introduction.....</b>                                 | <b>4</b> |
|          | Flow-X function library .....                            | 4        |
|          | API Petroleum Measurement Tables .....                   | 4        |
| <b>2</b> | <b>Spirit<sup>IT</sup> Gas and liquid functions.....</b> | <b>8</b> |
|          | fxAGA3_C .....   | 8        |
|          | fxAGA5_C .....   | 12       |
|          | fxAGA8_C .....   | 13       |
|          | fxAGA8_M .....   | 14       |
|          | fxAGA8_Gross .....                                       | 15       |
|          | fxAGA10_M .....  | 16       |
|          | fxAGA10ex_M .....  | 17       |
|          | fxAPI_Dens15C_1952 .....                                 | 19       |
|          | fxAPI_Dens15C_1980 .....                                 | 21       |
|          | fxAPI_Dens15C_NGL_LPG .....                              | 24       |
|          | fxAPI_Dens20C_NGL_LPG .....                              | 27       |
|          | fxAPI_Gravity60F_1952 .....                              | 30       |
|          | fxAPI_Gravity60F_1980 .....                              | 32       |
|          | fxAPI_MPMS_11_2_1 .....                                  | 35       |
|          | fxAPI_MPMS_11_2_1M .....                                 | 36       |
|          | fxAPI_MPMS_11_2_2 .....                                  | 37       |
|          | fxAPI_MPMS_11_2_2M .....                                 | 38       |
|          | fxAPI_MPMS_11_3_2_1 .....                                | 39       |
|          | fxAPI_MPMS_11_3_3_2 .....                                | 40       |
|          | fxAPI_RD60F_1980 .....                                   | 41       |
|          | fxAPI_SG60F_1952 .....                                   | 44       |
|          | fxAPI_RD60F_NGL_LPG .....                                | 46       |
|          | fxAPI_Table5_1952 .....                                  | 49       |
|          | fxAPI_Table5_1980 .....                                  | 50       |
|          | fxAPI_Table5_2004 .....                                  | 51       |
|          | fxAPI_Table6_1952 .....                                  | 52       |
|          | fxAPI_Table6_1980 .....                                  | 53       |
|          | fxAPI_Table6_2004 .....                                  | 54       |
|          | fxAPI_Table23_1952 .....                                 | 55       |
|          | fxAPI_Table23_1980 .....                                 | 56       |
|          | fxAPI_Table23_2004 .....                                 | 57       |
|          | fxAPI_Table23E .....                                     | 59       |
|          | fxAPI_Table24_1952 .....                                 | 60       |
|          | fxAPI_Table24_1980 .....                                 | 61       |
|          | fxAPI_Table24_2004 .....                                 | 63       |
|          | fxAPI_Table24E .....                                     | 64       |
|          | fxAPI_Table53_1952 .....                                 | 65       |
|          | fxAPI_Table53_1980 .....                                 | 66       |
|          | fxAPI_Table53_2004 .....                                 | 67       |
|          | fxAPI_Table53E .....                                     | 68       |
|          | fxAPI_Table54_1952 .....                                 | 69       |
|          | fxAPI_Table54_1980 .....                                 | 70       |
|          | fxAPI_Table54_2004 .....                                 | 71       |
|          | fxAPI_Table54E .....                                     | 72       |
|          | fxAPI_Table59_2004 .....                                 | 73       |
|          | fxAPI_Table59E .....                                     | 74       |
|          | fxAPI_Table60_2004 .....                                 | 75       |
|          | fxAPI_Table60E .....                                     | 76       |
|          | fxASTM_D1550_RD60 .....                                  | 77       |
|          | fxASTM_D1550_Ctl .....                                   | 79       |

|                                  |     |
|----------------------------------|-----|
| fxASTM_D4311M_09_C .....         | 80  |
| fxASTM_D4311M_09_M .....         | 81  |
| fxConvertUnit .....              | 82  |
| fxEthylene_IUPAC_C .....         | 83  |
| fxEthylene_IUPAC_M .....         | 84  |
| fxEthylene_NIST1045 .....        | 85  |
| fxGasViscosity_2004 .....        | 86  |
| fxGERG2008_Gas .....             | 87  |
| fxGERG2008_Flash .....           | 88  |
| fxGOST30319 .....                | 89  |
| fxGOST30319_AGA8 .....           | 90  |
| fxGOST30319_SGERG91 .....        | 91  |
| fxGPA_TP15 .....                 | 92  |
| fxGPA2172_C .....                | 93  |
| fxGPA2172_M .....                | 95  |
| fxIAPWS_IF97_C .....             | 97  |
| fxIAPWS_IF97_M .....             | 99  |
| fxInterpolationCurve .....       | 101 |
| fxISO5167_ISA1932Nozzle .....    | 102 |
| fxISO5167_LongRadiusNozzle ..... | 104 |
| fxISO5167_Orifice .....          | 106 |
| fxISO5167_Venturi .....          | 110 |
| fxISO5167_VenturiNozzle .....    | 112 |
| fxISO6976_1983_M .....           | 114 |
| fxISO6976_1995_M .....           | 115 |
| fxISO6976ex_1995_M .....         | 116 |
| fxISO6976_2016_M .....           | 118 |
| fxISO6976ex_2016_M .....         | 118 |
| fxMR113 .....                    | 121 |
| fxNX19_1962 .....                | 122 |
| fxNX19_M .....                   | 123 |
| fxOIML_R22_1975 .....            | 124 |
| fxSarasota_C .....               | 125 |
| fxSarasota_M .....               | 126 |
| fxSGERG_C .....                  | 127 |
| fxSGERG_M .....                  | 129 |
| fxSolartron_Gas_C .....          | 130 |
| fxSolartron_Gas_M .....          | 132 |
| fxSolartron_Liquid_C .....       | 134 |
| fxSolartron_Liquid_M .....       | 136 |
| fxSolartron_SG .....             | 138 |
| fxUGC_C .....                    | 139 |
| fxUGC_M .....                    | 140 |
| fxVCone_C .....                  | 141 |
| fxVCone_M .....                  | 143 |

|          |   |            |
|----------|---|------------|
| <b>3</b> | <b>Flow-X flow computer functions .....</b> | <b>146</b> |
|          | fx2CellSelection .....                      | 146        |
|          | fx3CellSelection .....                      | 147        |
|          | fxBatchFWA .....                            | 149        |
|          | fxBatchHistData .....                       | 150        |
|          | fxBatchLatch .....                          | 151        |
|          | fxBatchMax .....                            | 152        |
|          | fxBatchMin .....                            | 153        |
|          | fxBatchTotal .....                          | 154        |
|          | fxBatchTWA .....                            | 155        |

|                                    |            |
|------------------------------------|------------|
| fxBatchWatch .....                 | 156        |
| fxDeviationAlarm .....             | 157        |
| fxGenerateReport .....             | 158        |
| fxIndex .....                      | 159        |
| fxKeypadFallback .....             | 160        |
| fxKeypadFallbackArray .....        | 161        |
| fxLatch .....                      | 162        |
| fxLimitAlarm .....                 | 163        |
| fxName .....                       | 164        |
| fxPeriodFWA .....                  | 165        |
| fxPeriodLatch .....                | 166        |
| fxPeriodMax .....                  | 167        |
| fxPeriodMin .....                  | 168        |
| fxPeriodTotal .....                | 169        |
| fxPeriodTWA .....                  | 170        |
| fxPeriodWatch .....                | 171        |
| fxPID .....                        | 172        |
| fxROCArm .....                     | 175        |
| fxSetOnChange .....                | 176        |
| fxSetOnCondition .....             | 177        |
| fxSetOnEvent .....                 | 178        |
| fxSetIndexOnChange .....           | 179        |
| fxSetIndexOnCondition .....        | 180        |
| fxSetIndexOnEvent .....            | 181        |
| fxStatusAlarm .....                | 182        |
| fxTag .....                        | 183        |
| fxTimer .....                      | 184        |
| fxTotalizerDelta .....             | 185        |
| fxTotalizerRate .....              | 186        |
| fxWatchUpdate .....                | 187        |
| <b>4 Flow-X IO Functions .....</b> | <b>189</b> |
| fxAnalogInput .....                | 189        |
| fxAnalogOutput .....               | 190        |
| fxSetAnalogOutput .....            | 191        |
| fxDigitalInput .....               | 192        |
| fxDigitalOutput .....              | 193        |
| fxSetDigitalOutput .....           | 194        |
| fxFrequencyOutput .....            | 195        |
| fxSetFrequencyOutput .....         | 196        |
| fxDoubleChronometry .....          | 197        |
| fxPulseInput .....                 | 199        |
| fxResetPulseInputErrors .....      | 201        |
| xPulseOutput .....                 | 202        |
| fxSetPulseOutput .....             | 203        |
| fxPT100Input .....                 | 204        |
| fxRTDInput .....                   | 205        |
| fxPT100Table .....                 | 206        |
| fxTimePeriodInput .....            | 207        |
| <b>5 Reference .....</b>           | <b>208</b> |
| Unit Types .....                   | 208        |
| Terminology .....                  | 214        |
| Standard composition .....         | 215        |
| <b>6 Revisions .....</b>           | <b>216</b> |

# 1 Introduction

## Flow-X function library

The Spirit<sup>IT</sup> Flow-X series of flow computer uses Microsoft Excel as its configuration environment. Each Flow-X application consists of a single Excel workbook that contains one or more worksheets.

Flow-X functions are configured as regular Excel functions. By using the output of one function as an input (argument) in another function a complete calculation scheme can be made. Functions can be defined on multiple sheets in order to organize the application.

## API Petroleum Measurement Tables

### History

The first version of the API Petroleum Measurement Tables was published in **1952**. In those days measurement readings were taken manually and the tables were used to convert the observed density or gravity at the observed temperature to the value at the reference temperature. So the table values were the actual standard.

The 1952 Tables consists of 58 tables containing all kind of correction and conversion factors used in the measurement of hydrocarbon liquids. Each table deals with a particular conversion of units, correction of density, or correction of volume. The 1952 tables that have to do with the conversion of density and volume are: 5, 6, 23, 24, 53 and 54.

Table 5, 6, 23 and 24 convert density or volume to or from to a reference temperature of 60°F, while tables 53 and 54 refer to 15°C.

In **1980** a complete new set of tables was published together with computer routines to allow electronic devices to automatically calculate the volume conversion factors and API gravity / (relative) density at the reference temperature. Back then most electronic devices were not capable of performing double-precision floating point calculations, so the standard prescribed all kind of rounding and truncating rules to make sure that the calculations would always provide the same result. For the 1980 version the calculation procedures are the standard rather than the table values.

In the 1980 version, which is also referred to as **API-2540**, the tables are divided into 3 product groups and a letter designation was used to distinguish between the sub-tables. "A" was used for crude oil, "B" for refined products and "C" for special applications. The 1980 tables, however, did not cover the LPGs and NGLs density ranges and the 1952 Tables were left valid for these products. Furthermore, the lubricating oil tables (designated as "D") were not complete at the time of the printing in 1980 and were released two years later. As opposed to the A, B and C tables no implementation procedures were defined for the D tables.

In 1988 the Institute of Petroleum released its Paper No. 3 with tables 59 and 60 that are based on a reference temperature of 20°C.

This resulted in the following Petroleum Measurement Tables dealing with the conversion of volume and density to and from a reference temperature.

| Number | Title  |
|--------|--|
| 5      | API Gravity Reduction to 60°F                                      |
| 6      | Reduction of Volume to 60°F Against API Gravity at 60°F            |
| 23     | Reduction of Observed Specific Gravity to Specific Gravity 60/60°F |
| 24     | Reduction of Volume to 60o F Against Specific Gravity 60/60°F      |
| 53     | Reduction of Observed Density to Density at 15°C                   |
| 54     | Reduction of Volume to 15°C Against Density at 15°C                |
| 59     | Reduction of Observed Density to Density at 20°C                   |
| 60     | Reduction of Volume to 20°C Against Density at 20°C                |

In **2004** the API MPMS 11.1 1980 tables were superseded by a new set of tables primarily for the following reasons:

- API 11.1:2004 includes the correction for both temperature and pressure in one and the same algorithm
- Taken into account the progress in electronics (and for other reasons) the complex truncating and rounding rules were abandoned. Instead the calculation procedures use double-precision floating point math. The input and output values are still rounded in order to obtain consistent results.
- The convergence methods for the correction of observed density to base density have been improved.
- On-line density measurement by densitometers became common practice, requiring the pressure and temperature correction to be incorporated in one and the same procedure
- The tables are extended in both temperature and density to cover lower temperatures and higher densities.
- The previous standard used a significant digit format which resulted in 4 or 5 decimal places depending on whether the observed temperature was above or below the reference temperature. The new standard prescribes 5 decimal places if or both cases.
- The IP paper No. 3 tables were added to accommodate conversion to 20°C.

Tables for lubricating oils including the implementation procedures are now part of the standard.

### Volume correction for pressure

The API MPMS 11.1:1980 Tables only cover the correction for temperature. The correction for pressure was published in API MPMS standards 11.2.1 and 11.2.2.

The correction for pressure is to the atmospheric pressure or, for products within the lower density range, to the equilibrium vapor pressure.

To calculate the equilibrium vapor pressure an Addendum was added to API MPMS 11.2.2. This addendum is also known as **GPA TP-15** (1988). In September 2007 the addendum was replaced by a new API standard 11.2.5 and at the same time GPA TP-15 (1988) was updated with a new 2007 revision.

## NGL and LPG tables

For NGL and LPG products volume correction tables 24E and 23E (at 60 °F) were published in **GPA TP-25** (1988), so the letter 'E' was used to distinguish the tables from the related API MPMS A, B, C and D tables.

GPA TP-25 has been superseded by **GPA TP-27** / API MPMS 11.2.4 (2007), which includes tables 53E, 54E, 59E and 60E to convert to 15°C and 20°C as well. All text from TP-25 is included without technical change, so TP-25 is still viable for conversion to and from 60 °F.

## Overview of hydrocarbon liquid conversion standards

- ASTM-IP Petroleum Measurement Tables, Historical Edition, 1952
- API MPMS Chapter 11.1□ - 1980\* (Temperature VCFs for Generalized Crude Oils, Refined Products, and Lubricating Oils): Historical; Published in 14 separate volumes

Also known as

- API Standard 2540 (API-2540)
- ASTM D1250
- IP 200
- In 1982 chapters XIII and XIV were published containing tables 5D, 6D, 53D and 54D for lubricating oils.
- API MPMS Chapter 11.1□ - 2004 (Temperature & Pressure VCFs for Generalized Crude Oils, Refined Products and Lube Oils)
- API MPMS Chapter 11.2.1- 1984 (Compressibility Factors for Hydrocarbons: 0-90°API): Historical: now incorporated into Chapter 11.1-2004
- API MPMS Chapter 11.2.1M- 1984 (Compressibility Factors for Hydrocarbons: 638-1074 kg/m<sup>3</sup>): Historical: now incorporated into Chapter 11.1-2004
- API MPMS Chapter 11.2.2 - 1984 (Compressibility Factors for Hydrocarbons: 0.350-0.637 Relative Density and –50°F to 140°F)
- API MPMS Chapter 11.2.2M - 1986 (Compressibility Factors for Hydrocarbons: 350-637 kg/m<sup>3</sup> Density (15°C) and –46°C to 60°C)

## Overview of the functions

The following table lists the volume conversion functions for hydrocarbon liquids as provided by the Flow-X series of flow computer.

| Function   | Temperature correction                         | Pressure correction | Input               | Output              |
|--|--|---------------------|---------------------|---------------------|
| <b>ASTM-IP Petroleum Measurement Tables 1952 - American Edition</b>                      |  |                     |                     |                     |
| API_Table23 (1952)   | Table 23 - Specific Gravity Reduction to 60 °F |                     | SG (T)              | SG (60°F)           |
| API_Table24 (1952)   | Table 24 - Volume Reduction to 60 °F           |                     | SG (60°F)           | Ctl                 |
| <b>Crude Oils, Refined Products and Lubricating Oils (API MPMS 11.1:1980 / API-2540)</b> |  |                     |                     |                     |
| API_Table5 (1980)  | API 11.1:1980 Tables 5A, 5B and 5D             | API 11.2.1:1984     | °API (T, P)         | °API (60°F, Pe)     |
| API_Table6 (1980)  | API 11.1:1980 Tables 6A, 6B and 6D             | API 11.2.1:1984     | °API (60°F, Pe)     | °API (T, P)         |
| API_Table23 (1980)   | API 11.1:1980 Tables 23A and 23B               | API 11.2.1:1984     | RD (T, P)           | RD (60°F, Pe)       |
| API_Table24 (1980)   | API 11.1:1980 Tables 24A and 24B               | API 11.2.1:1984     | RD (60°F, Pe)       | RD (T, P)           |
| API_Table53 (1980)   | API 11.1:1980 Tables 53A, 53B and 53D          | API 11.2.1M:1984    | Density (T, P)      | Density (15°C, Pe)  |
| API_Table54 (1980)   | API 11.1:1980 Tables 54A, 54B and 54D          | API 11.2.1M:1984    | Density (15°C, Pe)  | Density (T, P)      |
| <b>Crude Oils, Refined Products and Lubricating Oils (API MPMS 11.1:2004)</b>            |  |                     |                     |                     |
| API_Table5 (2004)  | API 11.1:2004                                  | API 11.1:2004       | °API (T, P)         | °API (60°F, 0 psig) |
| API_Table6 (2004)  | API 11.1:2004                                  | API 11.1:2004       | °API (60°F, 0 psig) | °API (T, P)         |

- API MPMS Chapter 11.2.2A - 1984 (Addendum to Correlation of Vapor Pressure Correction for NGL): Superseded by Chapter 11.2.5
- API Publication/GPA TP-25/ASTM Publication (Temperature Correction for the volume of Light Hydrocarbons – Tables 24E and 23E: Superseded by API MPMS Chapter 11.2.4 GPA TP-25 was published in 1998 and replaced the 1952 tables 23, 24 for Light Hydrocarbon Liquids and GPA Technical Publication TP-16, which were previously used for volumetric measurement of LPG.
- API MPMS Chapter 11.2.4 - 2007 / GPA TP-27 / ASTM Publication (Temperature Correction for the Volume of NGL and LPG – Tables 23E, 24E, 53E, 54E, 59E, 60E): Supersedes GPA TP-25
- API MPMS Chapter 11.2.5 - 2007 / GPA TP-15 / ASTM Publication (A Simplified Vapor Pressure Correlation for Commercial NGLs): Supersedes Addendum to Chapter 11.2.2 (11.2.2A)
- IP No. 3 - 1988 (Energy Institute (formerly Institute of Petroleum), Petroleum Measurement Paper No 3 Computer Implementation Procedures for Correcting Densities and Volumes to 20 C. Superseded by IP No.3 - 1997
- IP No. 3 - 1997 (Energy Institute (formerly Institute of Petroleum), Petroleum Measurement Paper No 3 Computer Implementation Procedures for Correcting Densities and Volumes to 20 C. Supersedes IP No.3 - 1988
- ISO 91-1 - 1982 Petroleum measurement tables Part 1: Tables based on reference temperatures of 15 °C and 60 °F. Superseded by ISO 91-1 1992.
- ISO 91-1 - 1992 Petroleum measurement tables Part 1: Tables based on reference temperatures of 15 °C and 60 °F. Supersedes ISO 91-1 1982.
- ISO 91-2 - 1991 Petroleum measurement tables Part 2: Tables based on reference temperatures of 20 °C
- OIML R 63 - 1994 Petroleum measurement tables

| Function                        | Temperature correction        | Pressure correction                                 | Input                                 | Output                   |
|---------------------------------|-------------------------------|---|---------------------------------------|--------------------------|
| API_Table23 (2004)              | API 11.1:2004                 | API 11.1:2004                                       | RD (T, P)                             | RD (60°F, 0 psig)        |
| API_Table24 (2004)              | API 11.1:2004                 | API 11.1:2004                                       | RD (60°F, 0 psig)                     | RD (T, P)                |
| API_Table53 (2004)              | API 11.1:2004                 | API 11.1:2004                                       | Density (T, P)                        | Density (15°C, 0 bar(g)) |
| API_Table54 (2004)              | API 11.1:2004                 | API 11.1:2004                                       | Density (15°C, 0 bar(g))              | Density (T, P)           |
| API_Table59 (2004)              | API 11.1:2004                 | API 11.1:2004                                       | Density (T, P)                        | Density (20°C, 0 bar(g)) |
| API_Table60 (2004)              | API 11.1:2004                 | API 11.1:2004                                       | Density (20°C, 0 bar(g))              | Density (T, P)           |
| API_Table6C (2004)              | API 11.1:2004                 | Not applicable                                      | Thermal expansion coefficient at 60°F | Ctl                      |
| <b>NGL and LPG (API 11.2.4)</b> |                               |   |                                       |                          |
| API_Table23E                    | API 11.2.4: 2007<br>Table 23E | API 11.2.2:1986<br>GPA TP-15:1988<br>GPA TP-15:2007 | RD (T, P)                             | RD (60°F, Pe)            |
| API_Table24E                    | API 11.2.4: 2007<br>Table 24E | API 11.2.2:1986<br>GPA TP-15                        | RD (60°F, Pe)                         | RD (T, P)                |
| API_Table53E                    | API 11.2.4: 2007<br>Table 53E | API 11.2.2:1986<br>GPA TP-15                        | Density (T, P)                        | Density (15°C, Pe)       |
| API_Table54E                    | API 11.2.4: 2007<br>Table 53E | API 11.2.2:1986<br>GPA TP-15                        | Density (15°C, Pe)                    | Density (T, P)           |
| API_Table59E                    | API 11.2.4: 2007<br>Table 59E | API 11.2.2M:1986<br>GPA TP-15                       | Density (T, P)                        | Density (20°C, Pe)       |
| API_Table60E                    | API 11.2.4: 2007<br>Table 60E | API 11.2.2M:1986<br>GPA TP-15                       | Density (20°C, Pe)                    | Density (T, P)           |

### Hydrometer Correction

The API MPMS 11.1 1980 Standard (API-2540) assumes that the API gravity or relative density is observed with a glass hydrometer. Therefore a correction may be applied for the change of volume of the glass hydrometer with temperature.

The hydrometer correction applies for tables 5A, 5B, 23A, 23B, 53A and 53B.

The 2004 standard does not include a correction for a glass hydrometer.

### API-2540 Boundaries

API MPMS 11.1:1980 (API 2540) is based on published data that lie within the so-called 'Data' range. The other table values were obtained from extrapolation and lie within the 'Extrapolated' range. It is recommended not to use API-2540 outside the 'Data' and 'Extrapolated' ranges.

For the lubricating oil tables no difference is made between data that is table values that are based on published data and table values that are determined by extrapolation.

| Range              | API Gravity<br>[°API] | Relative Density<br>[-] | Density<br>[kg/m <sup>3</sup> ] | Temperature<br>[°F]                | Temperature<br>[°C] |
|--------------------|-----------------------|-------------------------|---------------------------------|------------------------------------|---------------------|
| Data Range         | 0 .. 40               | 1.0760 .. 0.8250        | 1075.0 .. 824.0                 | 0 .. 250                           | -18..120            |
|                    | 40 .. 50              | 0.8250 .. 0.7795        | 824.0 .. 778.5                  | 0 .. 200                           | -18..90             |
|                    | 50 .. 55              | 0.7795 .. 0.7585        | 778.5 .. 758.0                  | 0 .. 150                           | -18..60             |
| Extrapolated Range | 0 .. 40               | 1.0760 .. 0.8250        | 1075.0 .. 824.0                 | 250 .. 300                         | 120..150            |
|                    | 40 .. 50              | 0.8250 .. 0.7795        | 824.0 .. 778.5                  | 200 .. 250                         | 90..125             |
|                    | 50 .. 55              | 0.7795 .. 0.7585        | 778.5 .. 758.0                  | 150 .. 200                         | 60..95              |
|                    | 55 .. 100             | 0.7585 .. 0.6110        | 758.0 .. 610.5                  | 0 .. 200                           | -18..95             |
| Applies for:       | Table 5A              | Table 23A               | Table 53A                       | Table 5A                           | Table 53A           |
|                    | Table 6A              | Table 24A               | Table 54A                       | Table 6A<br>Table 23A<br>Table 24A | Table 54A           |

| Range              | API Gravity<br>[°API] | Relative Density<br>[-] | Density<br>[kg/m <sup>3</sup> ] | Temperature<br>[°F]                | Temperature<br>[°C] |
|--------------------|-----------------------|-------------------------|---------------------------------|------------------------------------|---------------------|
| Data Range         | 0 .. 40               | 1.0760 .. 0.8250        | 1075.0 .. 824.0                 | 0 .. 250                           | -18..120            |
|                    | 40 .. 50              | 0.8250 .. 0.7795        | 824.0 .. 778.5                  | 0 .. 200                           | -18..90             |
|                    | 50 .. 85              | 0.7795 .. 0.6535        | 778.5 .. 653.0                  | 0 .. 150                           | -18..60             |
| Extrapolated Range | 0 .. 40               | 1.0760 .. 0.8250        | 1075.0 .. 824.0                 | 250 .. 300                         | 120..150            |
|                    | 40 .. 50              | 0.8250 .. 0.7795        | 824.0 .. 778.5                  | 200 .. 250                         | 90..125             |
|                    | 50 .. 85              | 0.7795 .. 0.6535        | 778.5 .. 653.0                  | 150 .. 200                         | 60..95              |
| Applies for:       | Table 5B              | Table 23B               | Table 53B                       | Table 5B                           | Table 53B           |
|                    | Table 6B              | Table 24B               | Table 54B                       | Table 6B<br>Table 23B<br>Table 24B | Table 54B           |

| Range        | API Gravity<br>[°API] | Relative Density<br>[-] | Density<br>[kg/m <sup>3</sup> ] | Temperature<br>[°F]                  | Temperature<br>[°C] |
|--------------|-----------------------|-------------------------|---------------------------------|--------------------------------------|---------------------|
| Data Range   | -10..45               | 0.8..1.165              | 800..1164                       | 0 .. 300                             | -20..+150           |
| Applies for: | Table 5D              | Table 23D*              | Table 53D                       | Table 5D                             | Table 53D           |
|              | Table 6D              | Table 24D*              | Table 54D                       | Table 6D<br>Table 23D*<br>Table 24D* | Table 54D           |

\* Values derived from Table 5D/6D

### API-2540 - Rounding and truncating rules

For each table API Standard 2540 specifies an explicit 'Calculation Procedure' that includes the rounding and truncating of all the input, intermediate and output values. The 'Calculation Procedure' is considered to be the standard rather than the table values or a set of equations. The function provides the option to either apply the full API rounding and truncating requirements or to perform the calculation procedure without any rounding and truncating being applied.

For tables 6A, 6B, 24A, 24B and 54A and 54B the standard makes a distinction between computational and table values for the calculated VCF. The table values are always rounded to 4 decimal places, Whereas the computational values has 4 decimal places when the VFC >=1 and 5 decimal places when the VCF < 1.

When API rounding is enabled the convergence limit is set to the limit value as specified in the standard. When the API rounding is disabled the convergence limit is set to 0.00001 kg/m<sup>3</sup> to obtain highest precision.

#### API-11.1:2004 Limits

| Range            | Density                                  | Temperature | Pressure        |
|------------------|--|-------------|-----------------|
| Crude Oil        | 610.6..1163.5 kg/m <sup>3</sup> @ 60°F   | -58..302 °F | 0..1500 psig    |
|                  | 100..-10 API @ 60°F                      | -50..150 °C | 0..103.4 bar(g) |
|                  | 0.61120..1.16464 RD @ 60°F               |             |                 |
|                  | 611.16..1163.79 kg/m <sup>3</sup> @ 15°C |             |                 |
|                  | 606.12..1161.15 kg/m <sup>3</sup> @ 20°C |             |                 |
| Refined products | 610.6..1163.5 kg/m <sup>3</sup> @ 60°F   | -58..302 °F | 0..1500 psig    |
|                  | 100..-10 API @ 60°F                      | -50..150 °C | 0..103.4 bar(g) |
|                  | 0.61120..1.16464 RD @ 60°F               |             |                 |
|                  | 611.16..1163.86 kg/m <sup>3</sup> @ 15°C |             |                 |
|                  | 606.12..1160.62 kg/m <sup>3</sup> @ 20°C |             |                 |
| Lubricating oils | 800.9..1163.5 kg/m <sup>3</sup> @ 60°F   | -58..302 °F | 0..1500 psig    |
|                  | 45..-10 API @ 60°F                       | -50..150 °C | 0..103.4 bar(g) |
|                  | 0.80168..1.1646 RD @ 60°F                |             |                 |
|                  | 801.25..1163.85 kg/m <sup>3</sup> @ 15°C |             |                 |
|                  | 798.11..1160.71 kg/m <sup>3</sup> @ 20°C |             |                 |

### API constants in US customary units

For the tables in US customary units the following constants apply (both for the 1980 and the 2004 tables):

| Product          | API Table | K0        | K1      | K2          |
|------------------|-----------|-----------|---------|-------------|
| Crude oil        | A         | 341.0957  | 0.0     | 0.0         |
| Gasoline         | B         | 192.4571  | 0.2438  | 0.0         |
| Transition area  | B         | 1489.0670 | 0.0     | -0.00186840 |
| Jet fuels        | B         | 330.3010  | 0.0     | 0.0         |
| Fuel oils        | B         | 103.8720  | 0.2701  | 0.0         |
| Lubricating oils | D         | 0.0       | 0.34878 | 0.0         |

### API constants in metric units

For the tables in metric units the following constants apply (both for the 1980 and the 2004 tables):

| Product          | API Table | K0        | K1     | K2          |
|------------------|-----------|-----------|--------|-------------|
| Crude oil        | A         | 613.9723  | 0.0    | 0.0         |
| Gasoline         | B         | 346.4228  | 0.4388 | 0.0         |
| Transition area  | B         | 2680.3206 | 0.0    | -0.00336312 |
| Jet fuels        | B         | 594.5418  | 0.0    | 0.0         |
| Fuel oils        | B         | 186.9696  | 0.4862 | 0.0         |
| Lubricating oils | D         | 0.0       | 0.6278 | 0.0         |

## 2 Spirit<sup>IT</sup> Gas and liquid functions

This chapter lists all available Spirit<sup>IT</sup> functions for gas and liquid calculations in alphabetical order. These functions are both available in the Flow-X flow computer software and in the Flow-Xpert offline calculation software.

### fxAGA3\_C

#### Description

The function calculates the mass flow rate for Orifice pressure differential flow devices according to the AGA-3 standard for orifice meters with flange taps.

#### Compliance

- AGA Report No. 3 - Orifice Metering Measurement of fluid flow by means of pressure differential devices, 1992
- API Manual of Petroleum Measurement Standards, Chapter 14 Natural Gas Fluids Measurement, Section 3 - Concentric Square-edged Orifice Meters 1992.
- Orifice Metering of Natural Gas and Other Related Hydrocarbon Fluids – Concentric, Square-edged Orifice Meters, Part 1: General Equations and Uncertainty Guidelines, fourth edition 2012.

#### Function inputs

| Function inputs               | Remark   | EU           | SW tag   | Range      | Default |
|-------------------------------|--|--------------|----------|------------|---------|
| Name                          | Optional tag name, tag description and tag group   |              |          |            |         |
| Differential Pressure         | Differential pressure over the primary flow device measured at the up- and downstream pressure tapings, which need to be in the positions as specified in the standard   | inH2O @ 60°F |          | 0..1000    | 0       |
| Pressure                      | Down- or upstream pressure value of the fluid at metering conditions   | psia         |          | 0..30000   | 0       |
| Temperature                   | Down- or upstream temperature of the fluid at metering conditions  | °F           |          | -400..2000 | 0       |
| Density                       | Down or upstream density of the fluid at metering conditions   | lbm/ft3      |          | 0..200     | 0       |
| Dynamic Viscosity             | Dynamic viscosity of the fluid   | lbm/ft.s     | DYNVIS   | 0..10      | 6.9e-6  |
| Isentropic Exponent           | Also referred to as $\kappa$ (kappa). For an ideal gas this coefficient is equal to the ratio of the specific heat capacity at constant pressure to the specific heat at constant volume. This ratio is commonly used when the real value is unknown.  | -            | KAPPA    | 0..10      | 1.3     |
| Pipe Diameter                 | Internal diameter of the pipe at reference temperature   | inches       | PIPEDIAM | 0..100     | 0       |
| Pipe Expansion factor         | The thermal expansion coefficient of the pipe material   | 1/°F         | PIPEEXP  | 0..1       | 6.2e-6  |
| Pipe Reference temperature    | The reference temperature that corresponds to the 'Pipe diameter' input value  | °F           | PIPEREFT | -400..2000 | 68      |
| Orifice Diameter              | Orifice diameter at reference temperature  | inches       | ORIFDIAM | 0..100     | 0       |
| Orifice Expansion factor      | The thermal expansion coefficient of the orifice material<br>Typical values are:   | 1/°F         | ORIFEXP  | 0..1       | 9.25e-6 |
| Orifice Reference Temperature | The reference temperature that corresponds to the 'Orifice diameter' input value   | °F           | ORIFREFT | -400..2000 | 68      |
| Pressure Location             | 1: Upstream tapping<br>Input 'Pressure' represents the pressure at the upstream pressure tapping ( $p_1$ ).<br>Since the absolute pressure is usually measured at the upstream tapping this is the most common setting.<br>2: Downstream tapping<br>Input 'Pressure' represents the pressure at the downstream tapping ( $p_2$ ).  | -            | PRESLOC  |            | 1       |
| Temperature Location          | 1: Upstream tapping<br>Input 'Temperature' represents the upstream temperature ( $t_1$ ).<br>2: Downstream tapping<br>Input 'Temperature' represents the temperature at the downstream tapping ( $t_2$ ).<br>3: Recovered pressure<br>Input 'Temperature' represents the downstream temperature at a location where the pressure has fully recovered ( $t_3$ ).<br>Since temperature measurement is usually downstream of the flow device this is the most common setting. | -            | TEMPLOC  |            | 3       |
| Temperature Correction        | 1: Use $(1-\kappa)/\kappa$<br>Isentropic expansion using $(1-\kappa)/\kappa$ as the temperature referral exponent<br>2: Use temperature exponent<br>Isentropic expansion using input 'Temperature Exponent' as the temperature referral exponent [-]   | -            | TEMPCOR  |            | 1       |
| Temperature Exponent          | To correct the temperature from down- to upstream conditions (or vice versa) the formula $(\kappa-1)/\kappa$ (isentropic expansion) will be used when the input value is set to 0, else the input value will be  |              | TEMPEXP  |            | 0       |



| Function inputs   | Remark   | EU | SW tag  | Range    | Default |
|-------------------|--|----|---------|----------|---------|
|                   | used.<br>For more details refer to section 'Temperature correction'.   |    |         |          |         |
| Density Location  | This parameter specifies if and how the density should be corrected from downstream to upstream conditions.<br>1: Upstream tapping<br>Input 'Density' represents the density at the upstream pressure tapping ( $p_1$ ).<br>2: Downstream tapping<br>Input 'Density' represents the density at the downstream tapping ( $p_2$ ).<br>3: Recovered pressure<br>Input 'Density' represents the density downstream at a location Where the pressure has fully recovered ( $p_3$ ). | -  | DENSLOC |          | 0       |
| Density Exponent. | This factor is used when density correction is enabled. The formula $1/\kappa$ will be used when the input value is set to 0, else the input value will be used.<br>For more details refer to section function 'ISO5167- Orifice' 'Density correction'.  | -  | DENSEXP |          | 0       |
| Fluid             | The type of fluid being measured<br>1: Gas<br>2: Liquid<br>For liquid the expansion factor is set to 1, i.e. the fluid is considered to be incompressible.   | -  | FLUID   |          | 0       |
| Drain hole        | When input is > 0 then an additional correction on the orifice diameter will be applied to account for the drain hole, as explained further on.  | in | DRAIN   | 0.. 100  | 0       |
| Fpwl              | Local Gravitational Correction Factor for Deadweight Calibrators used to calibrate differential and static pressure Instruments. Directly applied on the calculated mass flow rate within each iteration.  | -  | FPWL    | 0.9..1.1 | 1       |
| Year Of Edition   | 1: Edition 1992<br>2: Edition 2012   |    |         |          | 1       |

## Function outputs

| Function outputs                  | Remark  | EU      | SW tag  | Alarm                      | Fallback |
|-----------------------------------|---|---------|---------|----------------------------|----------|
| Status                            | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence  |         | STS     | FIOOR<br>CALCERR<br>NOVONV |          |
| Mass flow rate                    | The calculated mass flow rate   | klbm/hr | MASSR   |                            | 0        |
| Beta ratio                        | Orifice to pipe diameter ratio at upstream temperature  | -       | BETA    |                            | 0        |
| Orifice diameter                  | At the upstream temperature   | inches  | ORIFUP  |                            | 0        |
| Pipe diameter                     | At the upstream temperature   | inches  | PIPEUP  |                            | 0        |
| Upstream pressure                 | Pressure at upstream tapping ( $p_1$ )  | psia    | PRESUP  |                            | 0        |
| Pressure at downstream tapping    | Pressure at downstream tapping ( $p_2$ )  | psia    | PRESDN  |                            | 0        |
| Recovered downstream pressure     | Fully recovered downstream pressure ( $p_3$ )   | psia    | PRESREC |                            | 0        |
| Upstream temperature              | Temperature at upstream tapping ( $t_1$ )   | °F      | TEMPUP  |                            | 0        |
| Temperature at downstream tapping | Temperature at downstream tapping ( $t_2$ )   | °F      | TEMPDN  |                            | 0        |
| Downstream Temperature            | 'Fully recovered' downstream temperature ( $t_3$ )  | °F      | TEMPREC |                            | 0        |
| Upstream density                  | Density at upstream tapping ( $\rho_1$ )  | lbm/ft3 | DENSUP  |                            | 0        |
| Density at downstream tapping     | Pressure at downstream tapping ( $\rho_2$ )   | lbm/ft3 | DENSDN  |                            | 0        |
| Downstream density                | 'Fully recovered' downstream density ( $\rho_3$ )   | lbm/ft3 | DENSREV |                            | 0        |
| Reynolds number                   | The <u>pipe</u> Reynolds number, i.e. the Reynolds number upstream of the orifice and not the one within the device throat itself)  | -       | REYN    |                            | 0        |
| Discharge coefficient             |   | -       | DISCF   |                            | 0        |
| Expansion Factor                  |   | -       | EXPFAC  |                            | 0        |
| Velocity of Approach              |   | -       | VOA     |                            | 0        |
| Pressure out of range             | 0: Pressure is in valid range<br>1: Pressure is out of valid range  | -       | PRESOOR | PRESOOR                    | 0        |
| Reynolds out of range             | 0: Reynolds number is in valid range<br>1: Reynolds number is out of valid range  | -       | REYNOOR | REYNOOR                    | 0        |
| Diameter out of range             | 0: Device and pipe diameter and Beta ratio in valid range<br>1: Device diameter, pipe diameter and/or Beta ratio out of valid range | -       | DIAMOOR | DIAMOOR                    | 0        |

## Calculations

The calculations are in accordance with the standard.

## Pressure correction

The relation between the pressure at the upstream tapping  $p_1$  and the pressure at the downstream tapping ( $p_2$ ) is as following:

$$p_2 = p_1 - \frac{\Delta p \cdot K_{units}}{1000}$$

The relation between the pressure at the upstream tapping and the downstream tapping is as following:

$$p_3 = p_1 - p_{LOSS}$$

$$p_{LOSS} = \frac{(1 - \alpha \cdot \beta^2)}{(1 + \alpha \cdot \beta^2)} \cdot \Delta p \cdot K_{units}$$

$$\alpha = C \cdot E$$

$$E = \frac{1}{\sqrt{(1 - \beta^4)}}$$

Where:

|                    |  |              |
|--------------------|--|--------------|
| p <sub>1</sub>     | Pressure at upstream tapping   | psia         |
| p <sub>2</sub>     | Pressure at downstream tapping   | psia         |
| p <sub>3</sub>     | Fully recovered downstream pressure  | psia         |
| Δp                 | Differential pressure  | inH2O @ 60°F |
| p <sub>LOSS</sub>  | Pressure loss over the meter   | psi          |
| C                  | Discharge coefficient as calculated by the standard  | -            |
| α                  | Flow coefficient   | -            |
| β                  | Diameter ratio at the upstream pressure and temperature  | -            |
| E                  | Velocity of approach factor  | -            |
| K <sub>units</sub> | Unit conversion factor to convert a value expressed in 'inH2O @60°F' to the corresponding expressed in 'psi' (conversion as specified in section 'Unit Types') | -            |

### Temperature correction

When input 'Temperature correction' is set to 1, then an isentropic expansion based on the isentropic coefficient is applied:

$$t_1 = (t_2 + 459.67) \cdot \left( \frac{p_2}{p_1} \right)^{\frac{1-\kappa}{\kappa}} - 459.67$$

$$t_1 = (t_3 + 459.67) \cdot \left( \frac{p_3}{p_1} \right)^{\frac{1-\kappa}{\kappa}} - 459.67$$

When input 'Temperature correction' is set to 2, then an isentropic expansion based on input 'Temperature exponent' is applied:

$$t_1 = (t_2 + 459.67) \cdot \left( \frac{p_2}{p_1} \right)^{K_{TE}} - 459.67$$

$$t_1 = (t_3 + 459.67) \cdot \left( \frac{p_3}{p_1} \right)^{K_{TE}} - 459.67$$

Where:

|                |  |      |
|----------------|--|------|
| t <sub>1</sub> | Upstream temperature                                   | °F   |
| t <sub>2</sub> | Temperature at the downstream tapping                  | °F   |
| t <sub>3</sub> | Temperature at the fully recovered downstream pressure | °F   |
| p <sub>1</sub> | Upstream pressure                                      | psia |

|                 |                                     |      |
|-----------------|-------------------------------------|------|
| p <sub>2</sub>  | Pressure at the downstream tapping  | psia |
| p <sub>3</sub>  | Fully recovered downstream pressure | psia |
| κ               | Isentropic exponent                 | -    |
| K <sub>TE</sub> | Temperature exponent                | -    |

**Density correction**

When input 'Density exponent' = 0, then the following isentropic corrections are applied (depending on the type of Density Correction)

$$\rho_1 = \rho_2 \cdot \left( \frac{p_1}{p_2} \right)^{\frac{1}{\kappa}} \qquad \rho_1 = \rho_3 \cdot \left( \frac{p_1}{p_3} \right)^{\frac{1}{\kappa}}$$

Else the value of input 'Density Exponent' is used

$$\rho_1 = \rho_2 \cdot \left( \frac{p_1}{p_2} \right)^{K_{DE}} \qquad \rho_1 = \rho_3 \cdot \left( \frac{p_1}{p_3} \right)^{K_{DE}}$$

Where:

|          |  |         |
|----------|--|---------|
| $\rho_1$ | Upstream density                                   | lbm/ft3 |
| $\rho_2$ | Density at the downstream tapping                  | lbm/ft3 |
| $\rho_3$ | Density at the fully recovered downstream pressure | lbm/ft3 |
| $p_1$    | Upstream pressure                                  | psia    |
| $p_2$    | Pressure at the downstream tapping                 | psia    |
| $p_3$    | Fully recovered downstream pressure                | psia    |
| $\kappa$ | Isentropic exponent                                | -       |
| $K_{DE}$ | Density exponent                                   | -       |

## fxAGA5\_C

### Description

The AGA 5 standard defines methods to calculate the mass and volume based calorific values at 60°F and 14.73 psia for a natural gas based on known molar fractions of the non-hydrocarbon gas components.

### Compliance

- A.G.A. Transmission Measurement Committee Report No. 5 (Fuel gas Energy Metering) 1981
- A.G.A. Transmission Measurement Committee Report No. 5 (Fuel gas Energy Metering) 1996 (Reprinted 1999)

### Function inputs

| Function inputs  | Remark  | EU             | SW tag | Range | Default |
|------------------|---|----------------|--------|-------|---------|
| Name             | Optional tag name, tag description and tag group  |                |        |       |         |
| Composition      | Standard composition as defined in section 'Standard gas composition.<br>Only the following components are considered by the calculation:<br>N2 Nitrogen<br>CO2 Carbon dioxide<br>H2O Water<br>H2S Hydrogen sulfide<br>H2 Hydrogen<br>CO Carbon monoxide<br>O2 Oxygen<br>He Helium<br>Sum of these fractions may not exceed 1 | molar fraction | COMP   | 0..1  | 0       |
| Specific Gravity | Molar Mass Ratio, i.e. ratio of the molar mass of the gas and of the molar mass of air (specified in AGA-5 as 28.9644 kg/kmol (lbm/lbmol))  | -              | SG     | 0..1  | 0       |

### Function outputs

| Function outputs       | Remark  | EU      | SW tag  | Alarm            | Fallback |
|------------------------|---|---------|---------|------------------|----------|
| Status                 | 0: Normal<br>1: Input argument out of range<br>2: Calculation error |         | STS     | FIOOR<br>CALCERR |          |
| Calorific value mass   | Mass based calorific value  | Btu/lbm | CV_MASS |                  | 0        |
| Calorific value volume | Volume calorific value at 60°F and 14.73 psia                       | Btu/scf | CV_VOL  |                  | 0        |

### Calculations

The Energy to Mass ratio is calculated according to Section III of the standard, which contains the calculation procedure for the gas mass to energy conversion. The equations based on the 'by volume' fractional values are used (and not the equations based on the 'by weight' values).

The Energy to Volume ratio is calculated according to Section II of the standard, which contains the calculation procedure for the gas volume to energy conversion.

## fxAGA8\_C

### Description

The compressibility and density of a gas are calculated from the composition, temperature and pressure in accordance with the 'Detail Characterization' method outlined in the AGA-8 standard, with the input and output values in **US Customary** units.

### Compliance

- AGA Report No. 8, Second edition November 1992 - 2nd printing July 1994
- API MPMS 14.2, Second edition November 1992 - 2nd printing July 1994
- ISO 12213 Natural gas — Calculation of compression factor — Part 2: Calculation using molar-composition analysis, 1997

### Boundaries

The AGA-8 calculation has defined uncertainty bounds for gas mixtures that lie within the 'Normal range'. Also an 'Expanded range' of gas mixtures is defined for which the AGA-8 calculation has a higher uncertainty. Using the AGA-8 calculation for gas mixtures that lie outside the 'Expanded range' is not recommended.

### Function inputs

| Function inputs  | Remark   | EU      | SW tag     | Range      | Default |
|------------------|--|---------|------------|------------|---------|
| Name             | Optional tag name, tag description and tag group   |         |            |            |         |
| Pressure         | Pressure value   | psia    |            | 0..40000   | 1.01325 |
| Temperature      | Temperature value  | °F      |            | -250..+800 | 0       |
| Composition      | Standard composition as defined in section 'Standard gas composition'.   | mol/mol | COMP       | 0..1       | 0       |
| neo-Pentane mode | Determines what to do when component neo-Pentane is larger than zero<br>1: Add to i-Pentane<br>2: Add to n-Pentane<br>3: Neglect | -       | NEOC5_MODE |            | 1       |

### Function outputs

| Function outputs       | Remark  | EU        | SW tag  | Alarm                                 | Fallback |
|------------------------|---|-----------|---------|---------------------------------------|----------|
| Status                 | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence<br>4: Mole fractions do not add up to 1.0 +/- 0.0001   |           | STS     | FIOOR<br>CALCERR<br>NOCONV<br>COMPERR |          |
| Compressibility factor |   | -         | Z       |                                       | 1        |
| Mass Density           |   | lb/ft3    | MASDENS |                                       | 0        |
| Mole Density           |   | lbmol/ft3 | MOLDENS |                                       | 0        |
| Molar Mass             |   | lb/lbmol  | MOLMASS |                                       | 0        |
| Range                  | 0: In Normal Range<br>All inputs are within the 'Normal Range'<br>1: In Extended Range<br>One or more inputs within the 'Extended Range', but none of the inputs outside the Extended range (outputs values have higher uncertainty)<br>2: Out of Range<br>One or more inputs outside the 'Extended Range' (using the AGA8 calculation is not recommended in this case) |           | RANGE   | 00R                                   | 0        |

### Calculations

The calculations are as documented in the standard.

| Input value                        | Normal Range   | Expanded Range | EU   |
|------------------------------------|----------------|----------------|------|
| Pressure                           | 0 .. 20000     | 0 .. 20000     | psia |
| Temperature                        | -200 .. +400   | -200 .. +400   | °F   |
| Mole fraction of Methane           | 0.45 .. 1.00   | 0.00 .. 1.00   | -    |
| Mole fraction of Ethane            | 0.00 .. 0.10   | 0.00 .. 1.00   | -    |
| Mole fraction of Propane           | 0.00 .. 0.04   | 0.00 .. 0.12   | -    |
| Mole fraction of Butanes           | 0.00 .. 0.01   | 0.00 .. 0.06   | -    |
| Mole fraction of Pentanes          | 0.00 .. 0.003  | 0.00 .. 0.04   | -    |
| Mole fraction of Hexanes Plus      | 0.00 .. 0.002  | *              | -    |
| Mole fraction of Carbon monoxide   | 0.00 .. 0.03   | 0.00 .. 0.03   | -    |
| Mole fraction of Carbon dioxide    | 0.00 .. 0.30   | 0.00 .. 1.00   | -    |
| Mole fraction of Nitrogen          | 0.00 .. 0.50   | 0.00 .. 1.00   | -    |
| Mole fraction of Helium            | 0.00 .. 0.002  | 0.00 .. 0.03   | -    |
| Mole fraction of Argon             | 0.00 .. 0.00   | 0.00 .. 0.01   | -    |
| Mole fraction of Oxygen            | 0.00 .. 0.00   | 0.00 .. 0.21   | -    |
| Mole fraction of Hydrogen Sulphide | 0.00 .. 0.0002 | 0.00 .. 1.00   | -    |
| Mole fraction of Hydrogen          | 0.00 .. 0.10   | 0.00 .. 1.00   | -    |
| Mole fraction of Water             | 0.00 .. 0.0005 | *              | -    |

\* For these components the dew point temperature is the upper limit. Limit check is ignored for reason of simplicity.

## fxAGA8\_M

### Description

The compressibility and density of a gas are calculated from its composition, temperature and pressure in accordance with the 'Detail Characterization' method outlined in the AGA8 standard, with the input and output values in **metric** units.

### Compliance

- AGA Report No. 8, Second edition November 1992 - 2nd printing July 1994
- API MPMS 14.2, Second edition November 1992 - 2nd printing July 1994

- ISO 12213 Natural gas — Calculation of compression factor — Part 2: Calculation using molar-composition analysis, 1997
- AGA Report No. 8, Third edition April 2017

### Boundaries

The AGA-8 calculation has defined uncertainty bounds for gas mixtures that lie within the 'Normal range'. Also an 'Expanded range' of gas mixtures is defined for which the AGA-8 calculation has a higher uncertainty. Using the AGA-8 calculation for gas mixtures that lie outside the 'Expanded range' is not recommended.

### Function inputs

| Function inputs  | Remark   | EU      | SW tag     | Range      | Default |
|------------------|--|---------|------------|------------|---------|
| Name             | Optional tag name, tag description and tag group   |         |            |            |         |
| Pressure         | Pressure value   | bar(a)  |            | 0..2800    | 1.01325 |
| Temperature      | Temperature value  | °C      |            | -150..+450 | 0       |
| Composition      | Standard composition as defined in section 'Standard gas composition.  | mol/mol | COMP       | 0..1       | 0       |
| neo-Pentane mode | Determines what to do when component neo-Pentane is larger than zero<br>1: Add to i-Pentane<br>2: Add to n-Pentane<br>3: Neglect | -       | NEOC5_MODE |            | 1       |
| Year Of Edition  | 1: Edition 1994<br>2: Edition 2017   |         |            |            | 1       |

### Function outputs

| Function outputs       | Remark   | EU      | SW tag  | Alarm                                 | Fallback |
|------------------------|--|---------|---------|---------------------------------------|----------|
| Status                 | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence<br>4: Mole fractions do not add up to 1.0 +/- 0.0001  |         | STS     | FLOOR<br>CALCERR<br>NOCONV<br>COMPERR |          |
| Compressibility factor |  | -       | Z       |                                       | 1        |
| Mass Density           |  | kg/m3   | MASDENS |                                       | 0        |
| Mole Density           |  | kmol/m3 | MOLDENS |                                       | 0        |
| Molar Mass             |  | kg/kmol | MOLMASS |                                       | 0        |
| Range                  | 0: In Normal Range<br>All inputs are within the 'Normal Range'<br>1: In Extended Range<br>One or more inputs within the 'Extended Range, but none of the inputs outside the Extended rang (outputs values have higher uncertainty)<br>2: Out of Range<br>One or more inputs outside the 'Extended Range' (using the AGA8 calculation is not recommended in this case |         | RANGE   | OOR                                   | 0        |

### Calculations

The calculations are as documented in the standard.

## fxAGA8\_Gross

### Description

This function calculates the compressibility factor in accordance with the AGA-8 Gross Characterization Method. Although the AGA-8 Gross Method is based on the Standard GERG Virial Equation Of State (SGERG) there are slight differences in the results.

Two different methods are specified by the standard. Method 1 takes the Pressure, Temperature, Specific Gravity (Relative Density), Carbon Dioxide content and Gross Heating Value (GHV) as inputs. Method 2 takes the same inputs except for the Nitrogen content instead of GHV.

### Compliance

AGA 8, Second edition November 1992 - 2nd printing July 1994

- AGA Report No. 8, Second edition November 1992 - 2nd printing July 1994
- API MPMS 14.2, Second edition November 1992 - 2nd printing July 1994

### Function inputs

| Function inputs           | Remark  | EU      | Range       | Default |
|---------------------------|---|---------|-------------|---------|
| Name                      | Optional tag name, tag description and tag group  |         |             |         |
| Temperature               | Observed temperature  | °F      | -250..+800  | 60      |
| Pressure                  | Observed pressure   | psia    | 0..40000    |         |
| Relative density          | Relative density at the corresponding reference temperature and pressure  | -       | 0..2        | 0       |
| RD reference temperature  | Reference temperature for relative density  | °F      | -250 ..+800 | 60      |
| RD reference pressure     | Reference pressure for relative density   | psia    | 0..40000    | 14.73   |
| Gross heating value       | Gross heating value at the corresponding reference temperature and pressure   | Btu/ft3 | 0..2500     | 0       |
| GHV reference temperature | Reference temperature for gross heating value   | °F      | -250 ..+800 | 60      |
| GHV reference pressure    | Reference pressure for gross heating value  | psia    | 0..40000    | 14.73   |
| Nitrogen                  | Nitrogen (N2) fraction  | mol/mol | 0..1        | 0       |
| Carbon dioxide            | Carbon dioxide (CO2) fraction   | mol/mol | 0..1        | 0       |
| Method                    | Gross Characterization Method:<br>1: GHV, Relative Density, CO2<br>2: Relative Density, CO2, N2<br>Note: For Method 1 input 'Nitrogen' is not used, while for Method 2 inputs 'Gross heating value', 'GHV reference temperature' and 'GHV reference pressure' are not used. | -       |             | 0       |

### Function outputs

| Function outputs       | Remark   | EU        | SW tag | Alarm                      | Fallback |
|------------------------|--|-----------|--------|----------------------------|----------|
| Status                 | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence   |           | STS    | FIOOR<br>CALCERR<br>NOCONV |          |
| Compressibility factor |  | -         |        |                            | 1        |
| Molar mass             |  | lb/ lbmol |        |                            | 0        |
| Density                | Density at observed pressure and temperature   | lb/ft3    |        |                            | 0        |
| Range                  | 0: In Normal Range<br>All components are within the range that is recommended by the standard<br>1: Out of Range<br>One or more inputs are outside the recommended range |           | RANGE  |                            | 0        |

### Calculations

The calculations are in accordance with the standard.

### Boundaries

The AGA8 standard recommends using the Gross Characterization Method only when input conditions lie within the following range. For conditions outside this range the standard recommends to use the Detailed Characterization Method.

| Input value         | Normal Range  | EU      |
|---------------------|---------------|---------|
| Temperature         | 32..130       | °F      |
| Pressure            | 0 .. 1200     | psia    |
| Gross heating value | 475 .. 1210   | Btu/ft3 |
| Relative density    | 0.554 .. 0.87 | -       |
| Carbon dioxide      | 0.00 .. 0.30  | mol/mol |
| Nitrogen            | 0.00 .. 0.50  | mol/mol |

## fxAGA10\_M

### Description

The function calculates the speed of sound of a gas at the specified conditions of temperature and pressure using the formulae presented in the American Gas Association Report No 10.

### Compliance

AGA Report No. 10 - Speed of Sound in Natural Gas and Other Related Hydrocarbon Gases, January 2003

### Boundaries

The AGA-10 calculation has defined uncertainty bounds for gas mixtures that lie within the 'Normal range'. Also an 'Expanded range' of gas mixtures is defined for which the AGA-10 calculation has a higher uncertainty. Using the AGA-10 calculation for gas mixtures that lie outside the 'Expanded range' is not recommended.

The AGA-10 standard specifies the same limits as the AGA-8 standard. Refer to the fxAGA8 function for details on the actual limit values used by this function to set output 'Range'.

### Function inputs

| Function inputs  | Remark   | EU      | SW tag     | Range      | Default |
|------------------|--|---------|------------|------------|---------|
| Name             | Optional tag name, tag description and tag group   |         |            |            |         |
| Pressure         | Observed pressure  | bar(a)  |            | 0..2000    |         |
| Temperature      | Observed temperature   | °C      |            | -200..+400 |         |
| Composition      | Standard composition as defined in section 'Standard gas composition.'   | mol/mol | COMP       | 0..1       |         |
| neo-Pentane mode | Determines what to do when component neo-Pentane is larger than zero<br>1: Add to i-Pentane<br>2: Add to n-Pentane<br>3: Neglect | -       | NEOC5_MODE |            | 1       |

### Function outputs

| Function outputs | Remark  | EU  | SW tag | Alarm                                 | Fallback |
|------------------|---|-----|--------|---------------------------------------|----------|
| Status           | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence<br>4: Mole fractions do not add up to 1.0 +/- 0.0001   |     | STS    | FLOOR<br>CALCERR<br>NOCONV<br>COMPOOR |          |
| Speed of sound   |   | m/s | SOS    |                                       | 0        |
| Range            | 0: In Normal Range<br>All inputs are within the 'Normal Range'<br>1: In Extended Range<br>One or more inputs within the 'Extended Range', but none of the inputs outside the Extended rang (outputs values have higher uncertainty)<br>2: Out of Range<br>One or more inputs outside the 'Extended Range' (using the AGA10 calculation is not recommended in this case) |     | RANGE  | OOOR                                  | 0        |

### Calculations

Calculations are as documented in the standard.



## fxAGA10ex\_M

### Description

The extended AGA 10 function provides an extensive set of gas properties at the specified conditions of temperature and pressure using the formulae presented in the American Gas Association Report No 10.

### Compliance

AGA Report No. 10 - Speed of Sound in Natural Gas and Other Related Hydrocarbon Gases, January 2003

### Boundaries

The AGA-10 calculation has defined uncertainty bounds for gas mixtures that lie within the 'Normal range'. Also an 'Expanded range' of gas mixtures is defined for which the AGA-10 calculation has a higher uncertainty. Using the AGA-10 calculation for gas mixtures that lie outside the 'Expanded range' is not recommended.

The AGA-10 standard specifies the same limits as the AGA-8 standard. Refer to the fxAGA8 function for details on the actual limit values used by this function to set output 'Range'.

### Function inputs

| Function inputs  | Remark   | EU      | SW tag     | Range      | Default |
|------------------|--|---------|------------|------------|---------|
| Name             | Optional tag name, tag description and tag group   |         |            |            |         |
| Pressure         | Observed pressure  | bar(a)  |            | 0..2000    |         |
| Temperature      | Observed temperature   | °C      |            | -200..+400 |         |
| Composition      | Standard composition as defined in section 'Standard gas composition'.   | mol/mol | COMP       | 0..1       |         |
| neo-Pentane mode | Determines what to do when component neo-Pentane is larger than zero<br>1: Add to i-Pentane<br>2: Add to n-Pentane<br>3: Neglect | -       | NEOC5_MODE |            | 1       |

### Function outputs

| Function outputs                            | Remark  | EU                 | SW tag    | Alam                                  | Fall back |
|---|---|--------------------|-----------|---------------------------------------|-----------|
| Status                                      | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence<br>4: Mole fractions do not add up to 1.0 +/- 0.0001   |                    | STS       | FLOOR<br>CALCERR<br>NOCONV<br>COMPOOR |           |
| Molecular weight                            |   | kg/kmol            | MOLMASS   |                                       |           |
| Molar density at base conditions            |   | mol/m <sup>3</sup> | MOLDENSB  |                                       |           |
| Molar density at flowing conditions         |   | mol/m <sup>3</sup> | MOLDENSF  |                                       |           |
| Mass density at base conditions             |   | kg/m <sup>3</sup>  | MASSDENSB |                                       |           |
| Mass density at flowing conditions          |   | kg/m <sup>3</sup>  | MASSDENSF |                                       |           |
| Ideal gas relative density                  |   | -                  | IRD       |                                       |           |
| Real gas relative density                   |   | -                  | RRD       |                                       |           |
| Velocity of sound                           |   | m/s                | SOS       |                                       |           |
| Compressibility at base conditions          |   | -                  | ZB        |                                       |           |
| Compressibility at flowing conditions       |   | -                  | ZF        |                                       |           |
| Supercompressibility                        |   | -                  | FPV       |                                       |           |
| Ideal gas specific enthalpy                 |   | kJ/kg              | MASSHO    |                                       |           |
| Real gas specific enthalpy                  |   | kJ/kg              | MASSH     |                                       |           |
| Real gas specific entropy                   |   | kJ/kg/K            | MASSS     |                                       |           |
| Ideal gas isobaric heat capacity            |   | kJ/kg/K            | MASSCPO   |                                       |           |
| Real gas isobaric heat capacity             |   | kJ/kg/K            | MASSCP    |                                       |           |
| Real gas isochoric heat capacity            |   | kJ/kg/K            | MASSCV    |                                       |           |
| Ideal gas isobaric heat capacity            |   | kJ/kmol/K          | MOLCPO    |                                       |           |
| Real gas isobaric heat capacity             |   | kJ/kmol/K          | MOLCP     |                                       |           |
| Real gas isochoric heat capacity            |   | kJ/kmol/K          | MOLCV     |                                       |           |
| Ratio of specific heats                     |   | -                  | CPCV      |                                       |           |
| Isentropic exponent                         |   | -                  | KAPPA     |                                       |           |
| Critical flow factor                        |   | -                  | CRITC     |                                       |           |
| Ideal gas specific enthalpy                 |   | kJ/kmol            | MOLHO     |                                       |           |
| Real gas specific enthalpy                  |   | kJ/kmol            | MOLH      |                                       |           |
| Isentropic perfect gas critical flow factor |   | -                  | CI        |                                       |           |
| Isentropic real gas critical flow factor    |   | -                  | CRI       |                                       |           |
| Range                                       | 0: In Normal Range<br>All inputs are within the 'Normal Range'<br>1: In Extended Range<br>One or more inputs within the 'Extended Range', but none of the inputs outside the Extended rang (outputs values have higher uncertainty)<br>2: Out of Range<br>One or more inputs outside the 'Extended Range' (using the AGA10 calculation is not |                    | RANGE     |                                       | 0         |
|   |   |                    |           | OOR                                   |           |

| Function outputs          | Remark | EU | SW tag | Alam | Fall back |
|---------------------------|--------|----|--------|------|-----------|
| recommended in this case) |        |    |        |      |           |

Calculations

Calculations are as documented in the standard.

## fxAPI\_Dens15C\_1952

### Description

#### Density (T, P) <--> Density (15°C, equilibrium pressure)

This function converts a density value at the observed temperature and pressure to the density at 15°C and the equilibrium pressure (typically 0 barg) or vice versa. The temperature conversion is according to ASTM-IP Petroleum Measurements Tables 1952 (Also known as API-1952 tables) Table 54.

Note: this function is a combination of the API 1952 Tables and API 11.2.1M. For the calculation from observed to standard conditions an iterative calculation is required. The rounding and truncating of input and intermediate values is implemented such that the example calculations as specified in both standards are exactly reproduced.

### Compliance

- ASTM-IP Petroleum Measurement Tables, Metric Edition, Metric Units of Measurement, 1952
- API MPMS 11.2.1M - Compressibility Factors for Hydrocarbons: 638 - 1074 Kilograms per Cubic Meter Range - First Edition, August 1984

### Function inputs

| Function inputs      | Remark  | EU     | SW tag     | Range     | Default |
|----------------------|---|--------|------------|-----------|---------|
| Name                 | Optional tag name, tag description and tag group  |        |            |           |         |
| Observed Density     | Depending on the conversion method this is the Density either at the observed temperature and observed pressure or at 15 °C and the equilibrium pressure  | kg/m3  |            | 0..1300   | 0       |
| Observed temperature |   | °C     |            | -100..200 | 15      |
| Observed pressure    |   | bar(g) |            | -1..150   | 0       |
| API 11.2.1 rounding  | 0: Disabled<br>The calculation of the compressibility factor F is performed with full precision<br>1: Enabled<br>API-MPMS 11.2.1 rounding and truncating rules are applied. The compressibility factor F is rounded to 3 decimal places as specified in the standard. | -      | API1121RND |           | 0       |
| Equilibrium pressure | The equilibrium pressure is considered to be 0 bar(g) for liquids which have an equilibrium pressure less than atmospheric pressure (in compliance with API MPMS 12.2 par. 12.2.5.4).   | bar(g) | EQUIPRES   | 0..150    | 0       |
| Conversion method    | 1: From observed to standard conditions<br>2: From standard to observed conditions  |        | CONVERSION |           | 1       |

### Function outputs

| Function outputs      | Remark   | EU    | SW tag | Alarm                      | Fallback |
|-----------------------|--|-------|--------|----------------------------|----------|
| Status                | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence   | -     | STS    | FLOOR<br>CALCERR<br>NOCONV | 1        |
| Output Density        | Depending on the conversion method this is the Density either at 15 °C and the equilibrium pressure or at the observed temperature and observed pressure | kg/m3 | DENS   |                            | 0        |
| CTL                   | Volume correction factor for temperature.  | -     | CTL    |                            | 1        |
| CPL                   | Volume correction factor for pressure<br>Value will be rounded according to input 'API 11.2.1 rounding'  | -     | CPL    |                            | 1        |
| CTPL                  | Combined volume correction factor<br>CTPL = CTL * CPL  | -     | CTPL   |                            | 1        |
| F                     | Compressibility factor   | 1/bar | F      |                            | 0        |
| CTL calc out of range | With respect to the standard used for the calculation of CTL the combination of input values is:<br>0: In Range<br>1: Out of Range                       |       |        | CTL0OR                     | 0        |
| CPL calc out of range | With respect to the standard used for the calculation of CPL the combination of input values is:<br>0: In Range<br>1: Out of Range                       |       |        | CPLOOR                     | 0        |

### Calculations

The calculations depend on the conversion method.

**Conversion method 1:** from observed to standard conditions.

The function performs the following iterative algorithm to calculate the Density at standard conditions:

- 1 At the start of the iteration the initial value for Density at [15 °C, equilibrium pressure] is set to the Observed Density. The initial CPL value is set to 1.
- 2 The CTL value is determined from the Density at [15 °C, equilibrium pressure] according to API 1952 Table 54.
- 3 The Density at [15 °C, equilibrium pressure] is calculated from the Observed Density, the new CTL value and the CPL value from the previous iteration.
- 4 The compressibility factor is calculated according to API MPMS 11.2.1M from the density at [15 °C, equilibrium pressure] and the 'Observed temperature'. If API 11.2.1M rounding is enabled then the density and temperature are rounded and the calculations are performed in accordance with the rounding and truncating rules of the standard.
- 5 The CPL value is calculated from the compressibility factor and the 'Observed pressure' and 'Equilibrium pressure' input values.
- 6 The Density at [15 °C, equilibrium pressure] is calculated by dividing the Observed Density by the CTL and the new CPL value.
- 7 Steps 2 through 6 are repeated taking the Density value from step 6 as the start value for the next iteration until the absolute difference between two consecutive Density values is 0.0001.

**Conversion method 2:** from standard to observed conditions.

The function performs straightforward calculations to determine the Density at observed conditions:

- 1 The CTL value is calculated according to API 1952 Table 54
- 2 The compressibility factor is calculated according to API MPMS 11.2.1M from the input density and temperature'. If API 11.2.1M rounding is enabled then the input density and temperature are rounded and the calculations are performed in accordance with the rounding and truncating rules of the standard.
- 3 The CPL value is calculated from the compressibility factor and the 'Observed pressure' and 'Equilibrium pressure' input values.
- 4 The output Density (at observed temperature and pressure) is calculated from the input Density and the CTL and the CPL values.

## fxAPI\_Dens15C\_1980

### Description

#### Density (T, P) <--> Density (15°C, equilibrium pressure)

This function converts a density value at the observed temperature and pressure to the density value at 15°C and the equilibrium pressure (typically 0 bar(g)) or vice versa.

The temperature conversion is according to API-2540, Tables 53A/54A (Generalized Crude Oils) and 53B/54B (Refined Oil Products) and API MPMS 11.1 Chapter XIV Table 53D/54D: 1984 (Lubricating Oils), while the volume correction for pressure according to API MPMS 11.2.1M.

An iterative calculation needs to be applied to convert the observed density to the value at base conditions.

Note: this function is a combination of API2540 and API 11.2.1M. For the calculation from observed to standard conditions an iterative calculation is required. The rounding and truncating of input and intermediate values is implemented such that the example calculations as specified in both standards are exactly reproduced.

### Compliance

- API MPMS 11.1 Volume X (API Standard 2540) - Table 53A - Generalized Crude Oils, Correction of Observed Density to Density at 15°C - First Edition, August 1980
- API MPMS 11.1 Volume X (API Standard 2540) - Table 54A - Generalized Crude Oils, Correction of Volume to 15°C against Density at 15°C- First Edition, August 1980
- API MPMS 11.1 Volume X (API Standard 2540) - Table 53B - Generalized Products, Correction of Observed Density to Density at 15°C - First Edition, August 1980
- API MPMS 11.1 Volume X (API Standard 2540) - Table 54B - Generalized Products, Correction of Volume to 15°C against Density at 15°F - First Edition, August 1980
- API MPMS 11.1 Volume XIV - Table 53D - Generalized Lubricating Oils, Correction of Observed Density to Density at 15°C - January 1982
- API MPMS 11.1 Volume XIV - Table 54D - Generalized Lubricating Oils, Correction of Volume to 15°C against Density at 15°F - January 1982
- API MPMS 11.2.1M - Compressibility Factors for Hydrocarbons: 638 - 1074 Kilograms per Cubic Meter Range - First Edition, August 1984

### Function inputs

| Function inputs      | Remark   | EU     | SW tag     | Range     | Default |
|----------------------|--|--------|------------|-----------|---------|
| Name                 | Optional tag name, tag description and tag group   |        |            |           |         |
| Input density        | Meaning depends on the input 'Conversion method'.<br>'Conversion method' = 1<br>Density at the observed temperature and pressure<br>'Conversion method' = 2<br>Density at 15 °C and the equilibrium pressure.  | kg/m3  |            | 0..1300   | 0       |
| Observed temperature |  | °C     |            | -100..200 | 15      |
| Observed pressure    |  | bar(g) |            | -1..150   | 0       |
| Product              | 1: A - Crude Oil<br>2: B - Auto select<br>Selection based on density at 15 °C<br>3: B - Gasoline<br>4: B - Transition Area<br>5: B - Jet Fuels<br>6: B - Fuel Oil<br>7: D - Lubricating Oil  |        | PRDTYP     |           | 1       |
| API 2540 rounding    | 0: Disabled<br>The calculations are performed with full precision and the final CTL value is rounded as specified by input 'CTL decimal places'<br>1: Enabled for computational value<br>API-2540 rounding and truncating rules are applied and, in case of conversion method 2 (standard to observed), the <b>computational</b> value for CTL as specified in Table 54 is used, meaning that the CTL value has:<br>4 decimal places if CTL >=1<br>5 decimal places if CTL < 1.<br>2: Enabled for table value<br>API-2540 rounding and truncating rules are applied and, in case of conversion method 2 (standard to observed), the <b>table</b> value for CTL as specified in Table 54 meaning that the CTL value has 4 decimal places in all cases<br>3: Enabled with 5 decimal places<br>API-2540 rounding and truncating rules are applied, and, in case of conversion method 2 (standard to observed), the CTL value has 5 decimal places in all cases.<br><br>Note: although not strictly in accordance with the standard, this option is more commonly used than option 'Enabled for computational value'<br>Note: for conversion type 1 'From observed to standard conditions' the CTL factor is rounded to 6 decimal places when input 'API 2540 rounding' > 0, as in accordance with table 53. |        | API2540RND | -         | 0       |

| Function inputs       | Remark  | EU     | SW tag     | Range  | Default |
|-----------------------|---|--------|------------|--------|---------|
| Hydrometer correction | Only applies for conversion method<br>'1: From observed to standard conditions'<br>0: Disabled<br>1: Enabled  | -      | HYDROCOR   |        | 0       |
| API 11.2.1M rounding  | 0: Disabled<br>The calculation of the compressibility factor F is performed with full precision.<br>1: Enabled<br>API-MPMS 11.2.1M rounding and truncating rules are applied. The compressibility factor F is rounded to 3 decimal places as specified in the standard. | -      | API1121RND |        | 0       |
| Equilibrium pressure  | The equilibrium pressure is considered to be 0 bar(g) for liquids which have an equilibrium pressure less than atmospheric pressure (in compliance with API MPMS 12.2 par. 12.2.5.4)  | bar(g) | EQUIPRES   | 0..150 | 0       |
| Conversion method     | 1: From observed to standard conditions<br>2: From standard to observed conditions  |        | CONVERSION |        | 1       |

### Function outputs

| Function outputs      | Remark  | EU    | SW tag | Alarm                      | Fallback |
|-----------------------|---|-------|--------|----------------------------|----------|
| Status                | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence  | -     | STS    | FLOOR<br>CALCERR<br>NOCONV | 1        |
| Output density        | Meaning depends on the input 'Conversion method'.<br>'Conversion method' = 1<br>Density at 15 °C and the equilibrium pressure.<br>'Conversion method' = 2<br>Density at the observed temperature and pressure           | kg/m3 | DENS   |                            | 0        |
| CTL                   | Volume correction factor for temperature.<br>Value will be rounded according to input 'API2540 rounding'  | -     | CTL    |                            | 1        |
| CPL                   | Volume correction factor for pressure<br>Value will be rounded according to input 'API 11.2.1M rounding'  | -     | CPL    |                            | 1        |
| CTPL                  | Combined volume correction factor<br>CTPL = CTL * CPL   | -     | CTPL   |                            | 1        |
| K0                    | Actual value of constant K0 used for CTL calculation  | -     | K0     |                            | 0        |
| K1                    | Actual value of constant K1 used for CTL calculation  | -     | K1     |                            | 0        |
| K2                    | Actual value of constant K2 used for CTL calculation  | -     | K2     |                            | 0        |
| Alpha                 | Thermal expansion factor  | 1/°C  | ALPHA  |                            | 0        |
| F                     | Compressibility factor  | 1/bar | F      |                            | 0        |
| Product               | When input 'Product' is 'B - Auto select', then the output is set to the actual selected product of tables 53B/54B (enumerative value as defined for input 'Product'), else the output is set equal to input 'Product'. | -     | PRDCUR |                            | 0        |
| CTL calc out of range | With respect to the standard used for the calculation of CTL the combination of input values is:<br>0: In Range<br>1: Out of Range  |       |        | CTLOOR                     | 0        |
| CPL calc out of range | With respect to the standard used for the calculation of CPL the combination of input values is:<br>0: In Range<br>1: Out of Range  |       |        | CPLOOR                     | 0        |

### Calculations

The calculations depend on the conversion method.

#### Conversion method 1: from observed to standard conditions.

The function performs the following iterative algorithm to calculate the density at reference conditions:

- 1 First the inputs are rounded in accordance with the API2540 standard, provided that API2540 rounding is enabled.
- 2 The hydrometer correction on the input density is applied, provided that this correction is enabled
- 3 At the start of the iteration the density at [15 °C, equilibrium pressure] is set equal to the observed density and the initial CPL value is set to 1.
- 4 When the type of product is set to 'B – Auto select' (automatic selection of the refined product range) the K0, K1 and K2 factors are determined based on the density at [15 °C, equilibrium pressure]. The Transition area is only taken in consideration in the 2<sup>nd</sup> iteration loop, as specified in the standard.

- 5 The Alpha factor is calculated according from the density at [15 °C, equilibrium pressure] and the K0, K1 and K2 factor. If API2540 rounding is enabled, then the intermediate results are rounded or truncated as specified API-2540 Table 53.
- 6 The CTL value is calculated according to API-2540 Table 53 from the Alpha factor and the differential temperature (= observed temperature – 15°C). If API2540 rounding is enabled, then the intermediate results are rounded or truncated as specified API-2540 Table 53.
- 7 Depending on the type of API2540 rounding the calculated CTL value is rounded to 6 decimal places or not rounded at all.
- 8 The density at [15 °C, equilibrium pressure] is calculated by dividing the observed density by the new CTL value and the CPL value from the previous iteration.
- 9 The compressibility factor is calculated according to API MPMS 11.2.1M from the density at [15 °C, equilibrium pressure] and the 'Observed temperature'. If API 11.2.1M rounding is enabled then the density and temperature are rounded and

the calculations are performed in accordance with the rounding and truncating rules of the standard.

- 10 The CPL value is calculated from the compressibility factor and the 'Observed pressure' and 'Equilibrium pressure' input values.
- 11 The density at [15°C, equilibrium pressure] is calculated by dividing the observed density by CTL and the new CPL value.
- 12 If API2540 rounding is enabled then the density at [15°C, equilibrium pressure] value is rounded to 3 decimal places as specified in the standard.
- 13 Steps 4 through 12 are repeated taking the density value from step 12 as the starting value until the absolute difference between two consecutive density values is either 0.05 (or 0.07 for the transition area) or 0.000001, depending of API2540 rounding being enabled or not.
- 14 For refined products the entire iteration loop is repeated if the density at [15°C, equilibrium pressure] appears to be in a different product region than the observed input density. This is required because a different product region means different K0, K1 and K2 factors.
- 15 When API2540 rounding is enabled, the final density at [15°C, equilibrium pressure] is rounded to 1 decimal place.

**Conversion method 2:** from standard to observed conditions.

The function performs straightforward calculations to determine the density at observed conditions:

- 1 First the inputs are rounded in accordance with the API2540 standard, provided that API2540 rounding is enabled.
- 2 When the type of product is set to 'B – Auto select' (automatic selection of the refined product range) the K0, K1 and K2 factors are determined based on the input density
- 3 The Alpha factor is calculated according from the input density and the K0, K1 and K2 factor. If API2540 rounding is enabled, then the intermediate results are rounded or truncated as specified API-2540 Table 54.
- 4 The CTL value is calculated according to API-2540 Table 54 from the Alpha factor and the differential temperature (= observed temperature – 15°C If API2540 rounding is enabled, then the intermediate results are rounded or truncated as specified API-2540 Table 54.
- 5 Depending on the type of API2540 rounding the calculated CTL value is rounded to 4 or 5 decimal places or not rounded at all.
- 6 The compressibility factor is calculated according to API MPMS 11.2.1M from the input density and temperature'. If API 11.2.1M rounding is enabled then the input density and temperature are rounded and the calculations are performed in accordance with the rounding and truncating rules of the standard.
- 7 The CPL value is calculated from the compressibility factor and the 'Observed pressure' and 'Equilibrium pressure' input values.
- 8 The density at [15°C, equilibrium pressure] is calculated by multiplying the input density by the CTL and the CPL values.

## fxAPI\_Dens15C\_NGL\_LPG

### Description

#### Density (T, P) <--> Density (15°C, Pe)

This function converts the density value at the observed temperature and pressure to the density value at 15°C and the equilibrium pressure or vice versa.

The temperature correction is according to API MPMS 11.2.4:2007 (GPA TP-27), while the pressure correction is according to API MPMS 11.2.2M:1984.

The calculation of the equilibrium pressure is according to GPA TP-15 (API MPMS 11.2.2 Addendum:1994).

### Compliance

- API MPMS 11.2.4: Temperature Correction for the Volume of NGL and LPG Tables 23E, 24E, 53E, 54E, 59E & 60E, September 2007
- GPA TP-27: Temperature Correction for the Volume of NGL and LPG Tables 23E, 24E, 53E, 54E, 59E & 60E, September 2007
- API MPMS Chapter 11.2.2M - 1986 (Compressibility Factors for Hydrocarbons: 350-637 kg/m<sup>3</sup> Density (15°C) and -46°C to 60°C)
- API MPMS 11.2.5: A Simplified Vapor Pressure Correlation for Commercial NGLs, September 2007
- GPA TP-15: A Simplified Vapor Pressure Correlation for Commercial NGLs, September 2007 (also covers GPA TP-15 1988)
- API MPMS 11.2.2 Addendum : Compressibility Factors for Hydrocarbons: Correlation of Vapor Pressure for Commercial Natural Gas Liquids (same as GPA TP-15:1988)

### Function inputs

| Name                       | Remark  | EU     | SW tag     | Range     | Default |
|----------------------------|---|--------|------------|-----------|---------|
| Name                       | Optional tag name, tag description and tag group  |        |            |           |         |
| Input density              | Depending on the conversion method this represents the density either at the observed temperature and pressure or at 15 °C and the equilibrium pressure   | -      |            | 0..750    | 0       |
| Observed temperature       | Temperature at which the density is observed  | °C     |            | -100..150 | 15      |
| Observed pressure          | Pressure at which the density is observed   | bar(a) |            | -1..200   | 0       |
| API 11.2.4 rounding        | 0: Disabled<br>The calculations are performed with full precision and the output values are not rounded<br>1: Enabled<br>The related values are rounded as defined in the standard  |        | API1124RND |           | 0       |
| API 11.2.2M rounding       | 0: Disabled<br>The calculations are performed with full precision and the output values are not rounded<br>1: Enabled<br>The related values are rounded as defined in the standard  |        | API1122RND |           | 0       |
| Equilibrium pressure mode  | 1: Use Input<br>The value of input 'Equilibrium pressure value' is used for the calculation of CPL<br>2: GPA TP-15<br>The equilibrium pressure is calculated in accordance with GPA TP-15   |        | EQUIPMODE  |           | 2       |
| Equilibrium pressure value | Only used when input 'Equilibrium pressure mode' is set to 'Use input'. The value will be used for the calculation of the CPL   | bar(a) | EQUIPINP   |           | 0       |
| GPA TP-15 rounding         | Only used when 'Equilibrium pressure mode is set to 'GPA TP-15'<br>0: Disabled<br>Full precision (no rounding and truncating applied)<br>1: Enabled<br>Rounding as defined in ' GPA TP15:1988 / API MPMS 11.2.2 Addendum':1994  | -      | TP15RND    |           | 0       |
| P100 Correlation           | Only used when 'Equilibrium pressure mode is set to 'GPA TP-15'<br>0: Disabled<br>The standard correlation is commonly used for pure products such as propane, butane and natural gasoline. It only requires the relative density and the temperature to calculate the vapor pressure<br>1: Enabled<br>The improved correlation requires the vapor pressure at 100°F (37.8 °C). This method is better suited for varied NGL mixes Where different product mixes could have the same specific gravity but different equilibrium pressures. | -      | P100CORR   |           | 0       |
| Vapor pressure at 100°F    | Only used when 'Equilibrium pressure mode is set to 'GPA TP-15' and the P100 correlation is enabled.  | bar(a) | EQUIP100F  | 0..200    | 0       |
| Conversion method          | 1: From observed to standard conditions<br>2: From standard to observed conditions  |        | CONVMETH   |           | 1       |

### Function outputs

| Name | Remark | EU | SW tag | Alarm | Fallback |
|------|--------|----|--------|-------|----------|
|------|--------|----|--------|-------|----------|



| Name                   | Remark   | EU     | SW tag   | Alarm                      | Fallback |
|------------------------|--|--------|----------|----------------------------|----------|
| Status                 | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence   | -      | STS      | FLOOR<br>CALCERR<br>NOCONV | 1        |
| Output density         | Depending on the conversion method this represents the density either at 15 °C and the equilibrium pressure or the observed temperature and pressure   | kg/m3  | DENS     |                            | 0        |
| CTL                    | Volume correction factor for temperature.<br>Value will be rounded according to input 'API 11.2.4 rounding'  | -      | CTL      |                            | 1        |
| CPL                    | Volume correction factor for pressure<br>Value will be rounded according to input 'API 11.2.2M rounding'   | -      | CPL      |                            | 1        |
| CTPL                   | Combined volume correction factor<br>CTPL = CTL * CPL  | -      | CTPL     |                            | 1        |
| F                      | Compressibility factor<br>The output value will be either rounded or not depending input 'API rounding'  | 1/bar  | F        |                            | 0        |
| Equilibrium pressure   | The equilibrium pressure calculated by GPA TP-15<br>Will be set to 0 when equilibrium pressure is below atmospheric pressure   | bar(a) | EQUIPCUR |                            | 0        |
| CTL calc out of range  | With respect to the API 11.2.4 standard the combination of input values is:<br>0: In Range<br>1: Out of Range<br>The following range checks apply:<br>Conversion method 1: observed -> standard<br>$0.21 \leq RD \leq 0.74$<br>with $RD = \text{Input density} / 999.016/\text{CPL}$<br>$-46 \leq T \leq 93 \text{ }^{\circ}\text{C}$<br>Table 23E reference fluid ranges<br>Conversion method 1: standard -> observed<br>$351.7 \leq \text{Input density} \leq 687.8 \text{ kg/m}^3$<br>$-46 \leq T \leq 93 \text{ }^{\circ}\text{C}$<br>Table 23E reference fluid ranges |        |          | CTL00R                     | 0        |
| CPL calc out of range  | With respect to API 11.2.2M the combination of input values is:<br>0: In Range<br>1: Out of Range<br>The following range checks apply:<br>$350 \leq \text{Density } 15 \text{ }^{\circ}\text{C} \leq 637 \text{ kg/m}^3$<br>$-46 \text{ }^{\circ}\text{C} \leq T \leq 60 \text{ }^{\circ}\text{C}$   |        |          | CPLOOR                     | 0        |
| GPA TP-15 out of range | Only set when the GPA TP-15 calculation is enabled<br>With respect to the GPA TP-15 standard the combination of input values is:<br>0: In Range<br>1: Out of Range<br>The following range checks apply:<br>For lower range:<br>$0.350 \leq RD60 < 0.425$<br>$-50 \text{ to } (695.51 * RD60 - 155.51) \text{ }^{\circ}\text{F}$<br>Higher range:<br>$0.425 \leq RD60 \leq 0.676$<br>$-50 \text{ to } 140 \text{ }^{\circ}\text{F}$<br>with RD60 being the relative density at 60°F   | -      |          | TP150OR                    | 0        |

## Calculations

The calculations depend on the conversion method.

### Conversion method 1: from observed to standard conditions.

The function performs the following iterative algorithm to calculate the density at 15 °C and the equilibrium pressure.

- When API 11.2.4 rounding is enabled, the input density and temperature values are rounded in accordance with the standard
- At the start of the iteration the density at [15 °C, equilibrium pressure] is set equal to the observed density and the CPL value is set to 1.
- First the density corrected for pressure is calculated by dividing the observed density by the CPL value.
- The relative density corrected for pressure is calculated from the density corrected for pressure
- The relative density at [60 °F, equilibrium pressure] is calculated from the relative density corrected for pressure and the observed temperature according to Table 23E
- The relative density at [15 °C, equilibrium pressure] is calculated from the relative density at [60 °F, equilibrium pressure] converted to 15 °C according to Table 24E
- The density at [15 °C, equilibrium pressure] is calculated from the relative density at [15 °C, equilibrium pressure]
- The CTL value is calculated by dividing the density corrected for pressure by the density at [15 °C, equilibrium pressure]
- Depending on the value of input 'Equilibrium pressure mode', either value of input 'Equilibrium pressure value' is used or the equilibrium pressure (vapor pressure) is calculated according to GPA TP-15. Whether the GPA TP-15 rounding and truncation rules are applied is dictated by input 'GPA-TP15 rounding'
- The compressibility factor F is calculated according to API MPMS 11.2.2M from the density at [15 °C, equilibrium pressure] and the 'Observed temperature', with, depending on

input API 11.2.2M, rounding and truncation according to the standard.

- 11 The CPL value is calculated from the compressibility factor, the equilibrium pressure and the 'Observed pressure' input value.
- 12 The new value for density at [15°C, equilibrium pressure] is calculated by dividing the observed density by the CTL and CPL values.
- 13 Steps 3 though 12 are repeated taking the density value from step 12 as the starting value until the absolute difference between two consecutive density values is less than the convergence limit.  
To avoid convergence problems different convergence limits are applied, depending on whether API 11.2.2M and/or GPA TP-15 rounding is applied:  
If API 11.2.2M rounding is enabled -> Limit = 0.05 kg/m<sup>3</sup>  
else if GPA TP-15 rounding is enabled -> Limit = 0.005 kg/m<sup>3</sup>  
else -> Limit = 0.00001 kg/m<sup>3</sup>
- 14 If API 11.2.4 rounding is enabled, then the density at [15°C, equilibrium pressure] is rounded to 0.1

**Conversion method 2:** from standard to observed conditions.

The function performs straightforward calculations to determine the density at observed conditions:

- 1 When API 11.2.4 rounding is enabled, the input density and temperature values are rounded in accordance with the standard
- 2 The CTL value and the relative density at [60 °F, equilibrium pressure] are calculated according to API MPMS 11.2.4 (GPA TP-27) Table 60E from the density at [15 °C, equilibrium pressure] and the 'Observed temperature'.
- 3 Depending on the value of input 'Equilibrium pressure mode', either value of input 'Equilibrium pressure value' is used or the equilibrium pressure (vapor pressure) is calculated according to GPA TP-15.
- 4 The compressibility factor is calculated according to API MPMS 11.2.2M from the density at [15 °C, equilibrium pressure] and the 'Observed temperature'.
- 5 The CPL value is calculated from the compressibility factor, the equilibrium pressure and the 'Observed pressure' input value.
- 6 If API 11.2.4 rounding is enabled, then the CTL value is rounded at [60°F, equilibrium pressure] is rounded to 0.00001
- 7 The density at the observed conditions is calculated by multiplying the density at [15 °C, equilibrium pressure] by the CTL value and the CPL value.

## fxAPI\_Dens20C\_NGL\_LPG

### Description

#### Density (T, P) <--> Density (20°C, Pe)

This function converts the density value at the observed temperature and pressure to the density value at 20°C and the equilibrium pressure or vice versa.

The temperature correction is according to API MPMS 11.2.4:2007 (GPA TP-27), while the pressure correction is according to API MPMS 11.2.2M:1984.

The calculation of the equilibrium pressure is according to GPA TP-15 (API MPMS 11.2.2 Addendum:1994).

### Compliance

- API MPMS 11.2.4: Temperature Correction for the Volume of NGL and LPG Tables 23E, 24E, 53E, 54E, 59E & 60E, September 2007
- GPA TP-27: Temperature Correction for the Volume of NGL & LPG Tables 23E, 24E, 53E, 54E, 59E & 60E, September 2007
- API MPMS Chapter 11.2.2M - 1986 (Compressibility Factors for Hydrocarbons: 350-637 kg/m<sup>3</sup> Density (15°C) and -46°C to 60°C)
- API MPMS 11.2.5: A Simplified Vapor Pressure Correlation for Commercial NGLs, September 2007
- GPA TP-15: A Simplified Vapor Pressure Correlation for Commercial NGLs, September 2007 (also covers GPA TP-15 1988)
- API MPMS 11.2.2 Addendum : Compressibility Factors for Hydrocarbons: Correlation of Vapor Pressure for Commercial Natural Gas Liquids (same as GPA TP-15:1988)

### Function inputs

| Name                       | Remark   | EU                | SW tag     | Range     | Default |
|----------------------------|--|-------------------|------------|-----------|---------|
| Name                       | Optional tag name, tag description and tag group   |                   |            |           |         |
| Input density              | Depending on the conversion method this represents the density either at the observed temperature and pressure or at 20 °C and the equilibrium pressure  | kg/m <sup>3</sup> |            | 0..750    | 0       |
| Observed temperature       | Temperature at which the density is observed   | °C                |            | -100..150 | 20      |
| Observed pressure          | Pressure at which the density is observed  | bar(a)            |            | -1..200   | 0       |
| API 11.2.4 rounding        | 0: Disabled<br>The calculations are performed with full precision and the output values are not rounded<br>1: Enabled<br>The related values are rounded as defined in the standard   |                   | API1124RND |           | 0       |
| API 11.2.2M rounding       | 0: Disabled<br>The calculations are performed with full precision and the output values are not rounded<br>1: Enabled<br>The related values are rounded as defined in the standard   |                   | API1122RND |           | 0       |
| Equilibrium pressure mode  | 1: Use Input<br>The value of input 'Equilibrium pressure value' is used for the calculation of CPL<br>2: GPA TP-15<br>The equilibrium pressure is calculated in accordance with GPA TP-15  |                   | EQUIPMODE  |           | 2       |
| Equilibrium pressure value | Only used when input 'Equilibrium pressure mode' is set to 0.<br>The value will be used for the calculation of the CPL   | bar(a)            | EQUIPINP   |           | 0       |
| GPA TP-15 rounding         | 0: Disabled<br>Full precision (no rounding and truncating applied)<br>1: Enabled<br>Rounding as defined in ' GPA TP15:1988 / API MPMS 11.2.2 Addendum':1994  | -                 | TP15RND    |           | 0       |
| P100 Correlation           | 0: Disabled<br>The standard correlation is commonly used for pure products such as propane, butane and natural gasoline. It only requires the relative density and the temperature to calculate the vapor pressure<br>1: Enabled<br>The improved correlation requires the vapor pressure at 100°F (37.8 °C). This method is better suited for varied NGL mixes Where different product mixes could have the same specific gravity but different equilibrium pressures. | -                 | P100CORR   |           | 0       |
| Vapor pressure at 100°F    |  | bar(a)            | EQUIP100F  | 0..200    | 0       |
| Conversion method          | 1: From observed to standard conditions<br>2: From standard to observed conditions   |                   | CONVMETH   |           | 1       |

### Function outputs

| Name   | Remark  | EU | SW tag | Alarm         | Fallback |
|--------|---|----|--------|---------------|----------|
| Status | 0: Normal<br>1: Input argument out of range<br>Outputs will be set to fallback values<br>2: Calculation error | -  | STS    | FLOOR<br>CALC | 1        |

| Name                   | Remark   | EU     | SW tag   | Alarm   | Fallback |
|------------------------|--|--------|----------|---------|----------|
|                        | Outputs will be set to fallback values<br>3: No convergence within 15 iterations<br>Outputs will be set to values of last iteration  |        |          | NOCONV  |          |
| Output density         | Depending on the conversion method this represents the density either at 20 °C and the equilibrium pressure or the observed temperature and pressure   | kg/m3  | DENS     |         | 0        |
| CTL                    | Volume correction factor for temperature.<br>Value will be rounded according to input 'API 11.2.4 rounding'  | -      | CTL      |         | 1        |
| CPL                    | Volume correction factor for pressure<br>Value will be rounded according to input 'API 11.2.2M rounding'   | -      | CPL      |         | 1        |
| CTPL                   | Combined volume correction factor<br>CTPL = CTL * CPL  | -      | CTPL     |         | 1        |
| F                      | Compressibility factor<br>The output value will be either rounded or not depending input 'API rounding'  | 1/bar  | F        |         | 0        |
| Equilibrium pressure   | The equilibrium pressure calculated by GPA TP-15<br>Will be set to 0 when equilibrium pressure is below atmospheric pressure   | bar(a) | EQUIPCUR |         | 0        |
| CTL calc out of range  | With respect to the API 11.2.4 standard the combination of input values is:<br>0: In Range<br>1: Out of Range<br>The following range checks apply:<br>Conversion method 1: observed -> standard<br>0.21 <= RD <= 0.74<br>with RD = Input density / 999.016/CPL<br>-46 <= T <= 93 °C<br>Table 23E reference fluid ranges<br>Conversion method 1: standard -> observed<br>331.7 <= Input density <= 683.6 kg/m3<br>-46 <= T <= 93 °C<br>Table 23E reference fluid ranges |        |          | CTLOOR  | 0        |
| CPL calc out of range  | With respect to API 11.2.2M the combination of input values is:<br>0: In Range<br>1: Out of Range<br>The following range checks apply:<br>350 <= Density 15 °C <= 637 kg/m3<br>-46 °C <= T <= 60 °C  |        |          | CPLOOR  | 0        |
| GPA TP-15 out of range | Only set when the GPA TP-15 calculation is enabled<br>With respect to the GPA TP-15 standard the combination of input values is:<br>0: In Range<br>1: Out of Range<br>The following range checks apply:<br>For lower range:<br>0.350 <= RD60 < 0.425<br>-50 to (695.51*RD60 - 155.51) °F<br>Higher range:<br>0.425 <= RD60 <= 0.676<br>-50 to 140 °F<br>with RD60 being the relative density at 60°F   | -      |          | TP15OOR | 0        |

## Calculations

The calculations depend on the conversion method.

**Conversion method 1:** from observed to standard conditions.

The function performs the following iterative algorithm to calculate the density at 20 °C and the equilibrium pressure.

- When API 11.2.4 rounding is enabled, the input density and temperature values are rounded in accordance with the standard
- At the start of the iteration the density at [20 °C, equilibrium pressure] is set equal to the observed density and the CPL value is set to 1.
- First the density corrected for pressure is calculated by dividing the observed density by the CPL value.
- The relative density corrected for pressure is calculated from the density corrected for pressure
- The relative density at [60 °F, equilibrium pressure] is calculated from the relative density corrected for pressure and the observed temperature according to Table 23E

- The relative density at [20 °C, equilibrium pressure] is calculated from the relative density at [60 °F, equilibrium pressure] converted to 20 °C according to Table 24E
- The density at [20 °C, equilibrium pressure] is calculated from the relative density at [20 °C, equilibrium pressure]
- The CTL value is calculated by dividing the density corrected for pressure by the density at [20 °C, equilibrium pressure]
- Depending on the value of input 'Equilibrium pressure mode', either value of input 'Equilibrium pressure value' is used or the equilibrium pressure (vapor pressure) is calculated according to GPA TP-15. Whether the GPA TP-15 rounding and truncation rules are applied is dictated by input 'GPA-TP15 rounding'
- API 11.2.2M requires the density at [15 °C, equilibrium pressure]. For this purpose the relative density at [15 °C, equilibrium pressure] is calculated according to Table 24E from the relative density at [60 °F, equilibrium pressure] and at 15 °C. This relative density value is then converted to the density at [15 °C, equilibrium pressure].

- 11 The compressibility factor F is calculated according to API MPMS 11.2.2M from the density at [15 °C, equilibrium pressure] and the 'Observed temperature', with, depending on input API 11.2.2M, rounding and truncation according to the standard.
- 12 The CPL value is calculated from the compressibility factor, the equilibrium pressure and the 'Observed pressure' input value.
- 13 The new value for density at [20°C, equilibrium pressure] is calculated by dividing the observed density by the CTL and CPL values.
- 14 Steps 2 though 6 are repeated taking the density value from step 6 as the starting value until the absolute difference between two consecutive density values is less than the convergence limit.  
To avoid convergence problems different convergence limits are applied, depending on whether API 11.2.2M and/or GPA TP-15 rounding is applied:  
If API 11.2.2M rounding is enabled -> Limit = 0.05 kg/m<sup>3</sup>  
else if GPA TP-15 rounding is enabled -> Limit = 0.005 kg/m<sup>3</sup>  
else -> Limit = 0.00001 kg/m<sup>3</sup>  
If API 11.2.4 rounding is enabled, then the density at [20°C, equilibrium pressure] is rounded to 0.1

**Conversion method 2:** from standard to observed conditions.

The function performs straightforward calculations to determine the density at observed conditions:

- 1 When API 11.2.4 rounding is enabled, the input density and temperature values are rounded in accordance with the standard
- 2 The CTL value and the relative density at [60 °F, equilibrium pressure] are calculated according to API MPMS 11.2.4 (GPA TP-27) Table 54 from the density at [20 °C, equilibrium pressure] and the 'Observed temperature'.
- 3 Depending on the value of input 'Equilibrium pressure mode', either value of input 'Equilibrium pressure value' is used or the equilibrium pressure (vapor pressure) is calculated according to GPA TP-15.
- 4 API 11.2.2M requires the density at [15 °C, equilibrium pressure]. For this purpose the relative density at [15 °C, equilibrium pressure] is calculated according to Table 24E from the relative density at [60 °F, equilibrium pressure] and at 15 °C. This relative density value is then converted to the density at [15 °C, equilibrium pressure].
- 5 The compressibility factor is calculated according to API MPMS 11.2.2M from the density at [15 °C, equilibrium pressure] and the 'Observed temperature'.
- 6 The CPL value is calculated from the compressibility factor, the equilibrium pressure and the 'Observed pressure' input value.
- 7 If API 11.2.4 rounding is enabled, then the CTL value is rounded at [60°F, equilibrium pressure] is rounded to 0.00001
- 8 The density at the observed conditions is calculated by multiplying the input density by the CTL value and the CPL value.

## fxAPI\_Gravity60F\_1952

### Description

**°API (T, P) <--> °API (60°F, equilibrium pressure)**

This function calculates the API gravity value at the observed temperature and pressure to the API gravity value at 60°F and the equilibrium pressure (typically 0 psig) or vice versa.

The volume correction for temperature is according to 1952 API Table 5 and 6, while the volume correction for pressure is according to API MPMS 11.2.1.

Note: this function is a combination of the API 1952 Tables and API 11.2.1. For the calculation from observed to standard conditions an iterative calculation is required. The rounding and truncating of input and intermediate values is implemented such that the example calculations as specified in both standards are exactly reproduced.

### Compliance

- ASTM-IP Petroleum Measurement Tables, American Edition, United States Units of Measurement, 1952
- API MPMS 11.2.1 - Compressibility Factors for Hydrocarbons: 0 - 90°API Gravity Range - First Edition, August 1984

### Function inputs

| Function inputs      | Remark  | EU   | SW tag     | Range     | Default |
|----------------------|---|------|------------|-----------|---------|
| Name                 | Optional tag name, tag description and tag group  |      |            |           |         |
| Input API gravity    | Depending of the conversion method this represents the API gravity at either the observed temperature and pressure or at 60 °F and the equilibrium pressure   | °API |            | -20..120  | 0       |
| Observed temperature | Temperature at which the API gravity is observed  | °F   |            | -100..400 | 60      |
| Observed pressure    | Pressure at which the API gravity is observed   | psig |            | -10..2000 | 0       |
| API 11.2.1 rounding  | 0: Disabled<br>The calculation of the compressibility factor F is performed with full precision<br>1: Enabled<br>API-MPMS 11.2.1 rounding and truncating rules are applied. The compressibility factor F is rounded to 3 decimal places as specified in the standard. | -    | API1121RND |           | 0       |
| Equilibrium pressure | The equilibrium pressure is considered to be 0 psig for liquids which have an equilibrium pressure less than atmospheric pressure (in compliance with API MPMS 12.2 par. 12.2.5.4)  | psig | EQUIPRES   | 0..2000   | 0       |
| Conversion method    | 1: From observed to standard conditions<br>2: From standard to observed conditions  |      | CONVERSION |           | 1       |

### Function outputs

| Function outputs      | Remark  | EU    | SW tag | Alarm                   | Fallback |
|-----------------------|---|-------|--------|-------------------------|----------|
| Status                | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence  | -     | STS    | FLOOR<br>CALC<br>NOCONV | 1        |
| Output API gravity    | Depending of the conversion method this represents the API gravity at either at 60 °F and the equilibrium pressure or the observed temperature and pressure | °API  | API    |                         | 0        |
| CTL                   | Volume correction factor for temperature.   | -     | CTL    |                         | 1        |
| CPL                   | Volume correction factor for pressure<br>Value will be rounded according to input 'API 11.2.1 rounding'   | -     | CPL    |                         | 1        |
| CTPL                  | Combined volume correction factor<br>CTPL = CTL * CPL   | -     | CTPL   |                         | 1        |
| F                     | Compressibility factor  | 1/psi | F      |                         | 0        |
| CTL calc out of range | With respect to the standard used for the calculation of CTL the combination of input values is:<br>0: In Range<br>1: Out of Range                          |       |        | CTLOOR                  | 0        |
| CPL calc out of range | With respect to the standard used for the calculation of CPL the combination of input values is:<br>0: In Range<br>1: Out of Range                          |       |        | CPLOOR                  | 0        |

## Calculations

The calculations depend on the conversion method.

**Conversion method 1:** from observed to standard conditions.

The function performs the following iterative algorithm to calculate the API Gravity at standard conditions:

- 1 At the start of the iteration the initial value for API Gravity at [60 °F, equilibrium pressure] is set to the Observed API Gravity. The initial CPL value is set to 1.
- 2 The CTL value is determined from the API Gravity at [60 °F, equilibrium pressure] according to API 1952 Table 6.
- 3 The API Gravity at [60 °F, equilibrium pressure] is calculated from the Observed API gravity, the new CTL value and the CPL value from the previous iteration.
- 4 Because API 11.2.1 requires the API gravity value at 60 °F, the API gravity at [60 °F, equilibrium pressure] is calculated from the API gravity at [60 °F, equilibrium pressure].
- 5 The compressibility factor is calculated according to API MPMS 11.2.1 from the API gravity at [60 °F, equilibrium pressure] and the 'Observed temperature'. If API 11.2.1 rounding is enabled then the API gravity and temperature are rounded and the calculations are performed in accordance with the rounding and truncating rules of the standard.
- 6 The CPL value is calculated from the compressibility factor and the 'Observed pressure' and 'Equilibrium pressure' input values.
- 7 The API Gravity at [60°F, equilibrium pressure] is calculated by dividing the Observed API Gravity by the CTL and the new CPL value.
- 8 Steps 2 through 7 are repeated taking the API gravity value from step 7 as the start value for the next iteration until the absolute difference between two consecutive API gravity values is 0.01.

**Conversion method 2:** from standard to observed conditions.

The function performs straightforward calculations to determine the API Gravity at observed conditions:

- 1 The CTL value is calculated according to API 1952 Table 6
- 2 Because API 11.2.1 requires the API gravity value at 60 °F, the API gravity at 60 °F is calculated from the 'Input API Gravity'.
- 3 The compressibility factor is calculated according to API MPMS 11.2.1 from the API gravity and the 'Observed temperature'. If API 11.2.1 rounding is enabled then the input density and temperature are rounded and the calculations are performed in accordance with the rounding and truncating rules of the standard.
- 4 The CPL value is calculated from the compressibility factor and the 'Observed pressure' and 'Equilibrium pressure' input values.
- 5 The output API Gravity (at observed temperature and pressure) is calculated from the input API Gravity and the CTL and the CPL values.

## fxAPI\_Gravity60F\_1980

### Description

**°API (T, P) <--> °API (60°F, equilibrium pressure)**

This function calculates the API gravity value at the observed temperature and pressure to the API gravity value at 60°F and the equilibrium pressure (typically 0 psig) or vice versa. The volume correction for temperature is according to API-2540, Tables 5/6A (Generalized Crude Oils) and 5/6B (Refined Oil Products) and API MPMS 11.1 Chapter XIII Table 5D: 1984 (Lubricating Oils), while the volume correction for pressure according to API MPMS 11.2.1.

Note: this function is a combination of API2540 and API 11.2.1. For the calculation from observed to standard conditions an iterative calculation is required. The rounding and truncating of input and intermediate values is implemented such that the example calculations as specified in both standards are exactly reproduced.

### Compliance

- API MPMS 11.1 Volume X (API Standard 2540) - Table 5A - Generalized Crude Oils, Correction of Observed API Gravity to API Gravity at 60°F - First Edition, August 1980
- API MPMS 11.1 Volume X (API Standard 2540) - Table 5B - Generalized Products, Correction of Observed API Gravity to API Gravity at 60°F- First Edition, August 1980
- API MPMS 11.1 Volume XIII - Table 5D - Generalized Lubricating Oils, Correction of Observed API Gravity to API Gravity at 60°F - January 1982
- API MPMS 11.1 Volume X (API Standard 2540) - Table 6A - Generalized Crude Oils, Correction of Volume to 60°F against API Gravity at 60°F - First Edition, August 1980
- API MPMS 11.1 Volume X (API Standard 2540) - Table 6B - Generalized Products, Correction of Volume to 60°F against API Gravity at 60°F - First Edition, August 1980
- API MPMS 11.1 Volume XIII - Table 6D - Generalized Lubricating Oils, Correction of Volume to 60°F against API Gravity at 60°F F - January 1982
- API MPMS 11.2.1 - Compressibility Factors for Hydrocarbons: 0 - 90°API Gravity Range - First Edition, August 1984

### Function inputs

| Function inputs       | Remark  | EU   | SW tag     | Range     | Default |
|-----------------------|---|------|------------|-----------|---------|
| Name                  | Optional tag name, tag description and tag group  |      |            |           |         |
| Input API gravity     | Depending of the conversion method this represents the API gravity at either the observed temperature and pressure or at 60 °F and the equilibrium pressure   | °API |            | -20..120  | 0       |
| Observed temperature  | Temperature at which the API gravity is observed  | °F   |            | -50..400  | 60      |
| Observed pressure     | Pressure at which the API gravity is observed   | psig |            | -10..2000 | 0       |
| Product               | 1: A - Crude Oil<br>2: B - Auto select<br>Selection based on °API at 60 °F<br>3: B - Gasoline<br>4: B - Transition Area<br>5: B - Jet Fuels<br>6: B - Fuel Oil<br>7: D - Lubricating Oil  |      | PRDTYP     | -         | 1       |
| API-2540 rounding     | 0: Disabled<br>The calculations are performed with full precision and the final CTL value is rounded as specified by input 'CTL decimal places'<br>1: Enabled for computational value<br>API-2540 rounding and truncating rules are applied and, in case of conversion method 2 (standard to observed), the computational value for CTL as specified in Table 6 is used, meaning that the CTL value has:<br>4 decimal places if CTL >=1<br>5 decimal places if CTL < 1.<br>2: Enabled for table value<br>API-2540 rounding and truncating rules are applied and, in case of conversion method 2 (standard to observed), the table value for CTL as specified in Table 6 meaning that the CTL value has 4 decimal places in all cases<br>3: Enabled with 5 decimal places<br>API-2540 rounding and truncating rules are applied, and, in case of conversion method 2 (standard to observed), the CTL value has 5 decimal places in all cases.<br>Note: although not strictly in accordance with the standard, this option is more commonly used than option 'Enabled for computational value'<br>Note: for conversion type 1 'From observed to standard conditions' the CTL factor is rounded to 6 decimal places when input 'API 2540 rounding' > 0, as in accordance with table 5. |      | API2540RND | -         | 0       |
| Hydrometer correction | Only applies for conversion method '1: From observed to standard conditions'<br>0: Disabled<br>1: Enabled   | -    | HYDROCOR   |           | 0       |



| Function inputs      | Remark  | EU   | SW tag     | Range   | Default |
|----------------------|---|------|------------|---------|---------|
| API 11.2.1 rounding  | 0: Disabled<br>The calculation of the compressibility factor F is performed with full precision<br>1: Enabled<br>API-MPMS 11.2.1 rounding and truncating rules are applied. The compressibility factor F is rounded to 3 decimal places as specified in the standard. | -    | API1121RND |         | 0       |
| Equilibrium pressure | The equilibrium pressure is considered to be 0 psig for liquids which have an equilibrium pressure less than atmospheric pressure (in compliance with API MPMS 12.2 par. 12.2.5.4)  | psig | EQUIPRES   | 0..2000 | 0       |
| Conversion method    | 1: From observed to standard conditions<br>2: From standard to observed conditions  |      | CONVERSION |         | 1       |

## Function outputs

| Function outputs      | Remark   | EU    | SW tag | Alarm                   | Fallback |
|-----------------------|--|-------|--------|-------------------------|----------|
| Status                | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence   | -     | STS    | FLOOR<br>CALC<br>NOCONV | 1        |
| Output API gravity    | Depending of the conversion method this represents the API gravity at either at 60 °F and the equilibrium pressure or the observed temperature and pressure  | °API  | API    |                         | 0        |
| CTL                   | Volume correction factor for temperature.<br>Value will be rounded according to input 'API2540 rounding'   | -     | CTL    |                         | 1        |
| CPL                   | Volume correction factor for pressure<br>Value will be rounded according to input 'API 11.2.1 rounding'  | -     | CPL    |                         | 1        |
| CTPL                  | Combined volume correction factor<br>CTPL = CTL * CPL  | -     | CTPL   |                         | 1        |
| K0                    | Actual value of constant K0 used for CTL calculation   | -     | K0     |                         | 0        |
| K1                    | Actual value of constant K1 used for CTL calculation   | -     | K1     |                         | 0        |
| K2                    | Actual value of constant K2 used for CTL calculation   | -     | K2     |                         | 0        |
| Alpha                 | Thermal expansion factor   | 1/°F  | ALPHA  |                         | 0        |
| F                     | Compressibility factor   | 1/psi | F      |                         | 0        |
| Product               | When input 'Product' is 'B - Auto select', then the output is set to the actual selected product of table 5B / 6B (enumerative value as defined for input 'Product'), else the output is set equal to input 'Product'. | -     | PRDCUR |                         | 0        |
| CTL calc out of range | With respect to the standard used for the calculation of CTL the combination of input values is:<br>0: In Range<br>1: Out of Range   |       |        | CTLOOR                  | 0        |
| CPL calc out of range | With respect to the standard used for the calculation of CPL the combination of input values is:<br>0: In Range<br>1: Out of Range   |       |        | CPLOOR                  | 0        |

## Calculations

The calculations depend on the conversion method.

**Conversion method 1:** from observed to standard conditions.

The function performs the following iterative algorithm to calculate the API gravity at standard conditions:

- 1 First the inputs are rounded in accordance with the API2540 standard, provided that API2540 rounding is enabled.
- 2 The observed density [kg/m<sup>3</sup>] is calculated from the observed API gravity
- 3 The hydrometer correction on the observed density is applied, provided that this correction is enabled
- 4 At the start of the iteration the initial value for density and API gravity at [60 °F, equilibrium pressure] is set to respectively the observed density and the observed API gravity. The initial CPL value is set to 1.
- 5 When the type of product is set to 'B – Auto select' (automatic selection of the refined product range) the K0, K1 and K2 factors are determined based on the API gravity at [60 °F, equilibrium pressure]. The Transition area is only taken in consideration in the 2nd iteration loop, as specified in the standard.
- 6 The Alpha factor is calculated according from the density at [60 °C, equilibrium pressure] and the K0, K1 and K2 factor. If

API2540 rounding is enabled, then the intermediate results are rounded or truncated as specified API-2540 Table 5.

- 7 The CTL value is calculated according to API-2540 Table 5 from the Alpha factor and the differential temperature (= observed temperature – 60°F). If API2540 rounding is enabled, then the intermediate results are rounded or truncated as specified API-2540 Table 5.
- 8 Depending on the type of API2540 rounding the calculated CTL value is rounded to 6 decimal places or not rounded at all.
- 9 The density at [60 °F, equilibrium pressure] is calculated by dividing the observed density by the new CTL value and the CPL value from the previous iteration.
- 10 The API gravity at [60 °F, equilibrium pressure] is calculated from the density at [60 °F, equilibrium pressure]
- 11 The compressibility factor is calculated according to API MPMS 11.2.1 from the API gravity at [60 °F, equilibrium pressure] and the 'Observed temperature'. If API 11.2.1 rounding is enabled then the API gravity and temperature are rounded and the calculations are performed in accordance with the rounding and truncating rules of the standard.
- 12 The CPL value is calculated from the compressibility factor and the 'Observed pressure' and 'Equilibrium pressure' input values.

- 13 The density at [60°F, equilibrium pressure] is calculated by dividing the observed density by CTL and the new CPL value.
- 14 If API2540 rounding is enabled then the density at [60°F, equilibrium pressure] value is rounded to 3 decimal places as specified in the standard.
- 15 The API gravity at [60 °F, equilibrium pressure] is calculated from the density at [60 °F, equilibrium pressure]
- 16 If API2540 rounding is enabled then the API gravity at [60°F, equilibrium pressure] value is rounded to 1 decimal place as specified in the standard.
- 17 Steps 5 through 16 are repeated taking the density value from step 14 as the start value for the next iteration until the absolute difference between two consecutive density values is either 0.05 (or 0.07 for the transition area) or 0.000001, depending of API2540 rounding being enabled or not.
- 18 For refined products the entire iteration loop is repeated if the API gravity at [60°F, equilibrium pressure] appears to be in a different product region than the observed API gravity. This is required because a different product region means different K0, K1 and K2 factors.

**Conversion method 2:** from standard to observed conditions.

The function performs straightforward calculations to determine the API gravity at observed conditions:

- 1 First the inputs are rounded in accordance with the API2540 standard, provided that API2540 rounding is enabled.
- 2 The density at [60°F, equilibrium pressure] is calculated from the input API gravity
- 3 When the type of product is set to 'B – Auto select' (automatic selection of the refined product range) the K0, K1 and K2 factors are determined based on the input API gravity
- 4 The Alpha factor is calculated according from the density at [60°F, equilibrium pressure] and the K0, K1 and K2 factor. If API2540 rounding is enabled, then the intermediate results are rounded or truncated as specified API-2540 Table 6.
- 5 The CTL value is calculated according to API-2540 Table 6 from the Alpha factor and the differential temperature (= observed temperature – 60°F). If API2540 rounding is enabled, then the intermediate results are rounded or truncated as specified API-2540 Table 6.
- 6 Depending on the type of API2540 rounding the calculated CTL value is rounded to 4 or 5 decimal places or not rounded at all.
- 7 The compressibility factor is calculated according to API MPMS 11.2.1 from the input density and temperature'. If API 11.2.1 rounding is enabled then the input density and temperature are rounded and the calculations are performed in accordance with the rounding and truncating rules of the standard.
- 8 The CPL value is calculated from the compressibility factor and the 'Observed pressure' and 'Equilibrium pressure' input values.
- 9 The API gravity at observed temperature and pressure is calculated from the input API gravity and the CTL and the CPL values.

## fxAPI\_MPMS\_11\_2\_1

### Description

The API MPMS 11.2.1 standard consists of a printed table that contains compressibility factors to correct hydrocarbon volumes under pressure to the corresponding volumes at the equilibrium pressure for the metered temperature.

The table contains compressibility factors related to meter temperature and API gravity at 60°F.

From the compressibility factor the volume correction for pressure is calculated according to API MPMS 12.2.

### Compliance

- API MPMS 11.2.1 - Compressibility Factors for Hydrocarbons: 0 - 90°API Gravity Range - First Edition, August 1984
- API MPMS 12.2 - Calculation of Liquid Petroleum Quantities Measured by Turbine or Displacement Meters

### Boundaries

API MPMS 11.2.1 defines the following limits on the input values:

- 0 to 90 °API
- 20 to +200 °F
- 0 to 1500 psig.

### API Rounding

The actual standard is the printed table. It also includes the 'Calculation Procedure' to obtain the table values based on the rounding and truncating of all input, intermediate and output values.

The function provides the option to either output the table value (including the full API rounding and truncating requirements) or to perform the calculation procedure without any rounding and truncating being applied.

### Function inputs

| Name                 | Remark   | EU   | SW tag   | Range     | Default |
|----------------------|--|------|----------|-----------|---------|
| Name                 | Optional tag name, tag description and tag group   |      |          |           |         |
| API60                | API gravity at 60°F  | °API |          | 0..120    | 0       |
| Observed Temperature |  | °F   |          | -50..400  | 60      |
| Observed Pressure    |  | psig |          | -10..2000 | 0       |
| Equilibrium Pressure | The equilibrium pressure is considered to be 0 psig for liquids which have an equilibrium pressure less than atmospheric pressure (in compliance with API MPMS 12.2 par. 12.2.5.4)   | psig | EQUIPRES | 0..2000   | 0       |
| API 11.2.1 rounding  | 0: Disabled<br>The calculation of the compressibility factor F is performed with full precision.<br>1: Enabled<br>API-MPMS 11.2.1 rounding and truncating rules are applied. The compressibility factor F is rounded to 3 decimal places as specified in the standard. |      | APIROUND | -         | 0       |

### Function outputs

| Name                     | Remark   | EU    | SW tag | Alarm           | Fallback |
|--------------------------|--|-------|--------|-----------------|----------|
| Status                   | 0: Normal<br>1: Input argument out of range<br>2: Calculation error  |       | STS    | FIOOR<br>CALERR | 1        |
| CPL                      | Volume correction factor for pressure<br>Note: to achieve compliance with API MPMS 12.2 the CPL value needs to be rounded to 4 decimal places. | -     | CPL    |                 | 1        |
| F                        | Compressibility factor<br>The output value will rounded according to input 'API 11.2.1 rounding'   | 1/psi | F      |                 | 0        |
| Calculation out of range | With respect to the standard the input values are:<br>0: In Range<br>1: Out of Range   | -     |        | OOR             | 0        |

### Calculations

The calculations are in either full or partial compliance with the standards, depending on whether API rounding is enabled or not and on the actual number of decimal places for the CPL value (API MPMS 12.2 defines 4 decimal places for the CPL value). The CPL value is calculated as follows (in compliance with API MPMS 12.2):

If  $P_e > 0$  then

$$CPL = \frac{1}{1 - F \cdot (P_o - P_e)}$$

### Else

$$CPL = \frac{1}{1 - F \cdot P_o}$$

With:

|     |                                       |       |
|-----|---------------------------------------|-------|
| CPL | Volume correction factor for pressure | -     |
| F   | Compressibility factor                | 1/psi |
| Po  | Observed pressure                     | psig  |
| Pe  | Equilibrium pressure                  | psig  |

## fxAPI\_MPMS\_11\_2\_1M

### Description

The API MPMS 11.2.1M standard consists of a printed table that contains compressibility factors to correct hydrocarbon volumes under pressure to the corresponding volumes at the equilibrium pressure for the metered temperature.

The table contains compressibility factors related to meter temperature and density at 15°C.

This metric standard corresponds with API MPMS 11.2.1 (the customary version)

### Data Limits

API MPMS 11.2.1M defines the following limits on the input values:

- 638 to 1074 kg/m<sup>3</sup>
- -30 to 90 °C
- 0 to 103 bar(g).

It is advised not to use the standard outside these limits.

### Compliance

- 11.2.1M - Compressibility Factors for Hydrocarbons: 638 - 1074 Kilograms per Cubic Meter Range - First Edition, August 1984
- API MPMS 12.2 - Calculation of Liquid Petroleum Quantities Measured by Turbine or Displacement Meters

### Function inputs

| Name                 | Remark  | EU                | SW tag   | Range     | Default |
|----------------------|---|-------------------|----------|-----------|---------|
| Name                 | Optional tag name, tag description and tag group  |                   |          |           |         |
| Density at 15°C      |   | kg/m <sup>3</sup> |          | 0..1300   | 0       |
| Observed temperature |   | °C                |          | -100..200 | 15      |
| Observed pressure    |   | bar(g)            |          | -1..150   | 0       |
| Equilibrium pressure | The equilibrium pressure is considered to be 0 bar(g) for liquids which have an equilibrium pressure less than atmospheric pressure (in compliance with API MPMS 12.2 par. 12.2.5.4)  | bar(g)            | EQUIPRES |           | 0       |
| API 11.2.1M rounding | 0: Disabled<br>The calculation of the compressibility factor F is performed with full precision<br>1: Enabled<br>API-MPMS 11.2.1M rounding and truncating rules are applied. The compressibility factor F is rounded in accordance with the standard. | -                 | APIROUND |           | 0       |

### Function outputs

| Name                     | Remark   | EU    | SW tag | Alarm         | Fallback |
|--------------------------|--|-------|--------|---------------|----------|
| Status                   | 0: Normal<br>1: Input argument out of range<br>2: Calculation error  |       | STS    | FIOOR<br>CALC | 1        |
| CPL                      | Volume correction factor for pressure<br>Note: to achieve compliance with API MPMS 12.2 the CPL value needs to be rounded to 4 decimal places. | -     | CPL    |               | 1        |
| F                        | Compressibility factor<br>The output value will be either rounded or not depending input 'API 11.2.1M rounding '                               | 1/bar | F      |               | 0        |
| Calculation out of range | With respect to the standard the input values are:<br>0: In Range<br>1: Out of Range   | -     |        | OOR           | 0        |

### Calculations

The calculations are in either full or partial compliance with the standards, depending on whether API rounding is enabled or not and on the actual number of decimal places for the CPL value (API MPMS 12.2 defines 4 decimal places for the CPL value). The CPL value is calculated as follows (in compliance with API MPMS 12.2):

If  $P_e > 0$  then

$$CPL = \frac{1}{1 - F \cdot (P_o - P_e)}$$

Else

$$CPL = \frac{1}{1 - F \cdot P_o}$$

With:

|                |                                       |        |
|----------------|---------------------------------------|--------|
| CPL            | Volume correction factor for pressure | -      |
| F              | Compressibility factor                | 1/bar  |
| P <sub>o</sub> | Observed pressure                     | bar(g) |
| P <sub>e</sub> | Equilibrium pressure                  | bar(g) |

## fxAPI\_MPMS\_11\_2\_2

### Description

The API MPMS 11.2.2 standard consists of a printed table that contains compressibility factors to correct hydrocarbon volumes under pressure to the corresponding volumes at the equilibrium pressure for the metered temperature.

The table contains compressibility factors related to meter temperature and the relative density at 60°F.

### Compliance

- 11.2.2 - Compressibility Factors for Hydrocarbons: 0.350 - 0.637 Relative Density (60°F/60°F) and -50°F to 140°F Metering Temperature - Second Edition, October 1986

### Boundaries

API MPMS 11.2.2 defines the following limits on the input values:

- 0.350 to 0.637 (relative density)
- 50 to 140 °F
- 0 to 2200 psig

### Pseudo-critical temperature check

The standard specifies that the observed temperature must be less than the **pseudo-critical** temperature

$$\text{Observed Temperature [Rankin]} < \text{Pseudo Critical Temperature} * 0.96$$

With:

$$\text{Pseudo Critical Temperature [Rankin]} = 621.418 - 822.686 * \text{RD60} + 1737.86 * \text{RD60}^2$$

$$\text{Observed Temperature [Rankin]} = \text{Observed Temperature [°F]} + 459.7;$$

### API Rounding

The actual standard is the printed table. Also included is a 'Calculation Procedure' that illustrates how to obtain the table values including all required rounding and truncating of the input, intermediate and output values.

The function provides the option to either output the table value (including all the full API rounding and truncating requirements) or to perform the calculation procedure without any rounding and truncating being applied.

### Function inputs

| Function inputs          | Remark   | EU   | SW tag   | Range     | Default |
|--------------------------|--|------|----------|-----------|---------|
| Name                     | Optional tag name, tag description and tag group   |      |          |           |         |
| Relative density at 60°F | Relative density at 60°F   | -    |          | 0..0.75   | 0       |
| Observed Temperature     |  | °F   |          | -100..300 | 60      |
| Observed Pressure        |  | psig |          | -10..2500 | 0       |
| Equilibrium Pressure     | The equilibrium pressure is considered to be 0 psig for liquids which have an equilibrium pressure less than atmospheric pressure (in compliance with API MPMS 12.2 par. 12.2.5.4)   | psig | EQUIPRES | 0..2500   | 0       |
| API 11.2.2 rounding      | 0: Disabled<br>The calculation of the compressibility factor F and CPL is performed with full precision.<br>1: Enabled<br>API-MPMS 11.2.2 rounding and truncating rules are applied.<br>The compressibility factor F is rounded to 8 decimal places with a maximum of 4 significant digits as specified in the standard.<br>The CPL value is rounded to 4 decimal places in compliance with the standard |      | APIROUND | -         | 0       |

### Function outputs

| Function outputs | Remark   | EU    | SW tag | Alarm            | Fallback |
|------------------|--|-------|--------|------------------|----------|
| Status           | 0: Normal<br>1: Input argument out of range<br>2: Calculation error  |       | STS    | FLOOR<br>CALCERR | 1        |
| CPL              | Volume correction factor for pressure<br>Value will be rounded according to input 'API 11.2.2 rounding'  | -     | CPL    |                  | 1        |
| F                | Compressibility factor<br>The output value will be either rounded or not depending input 'API 11.2.2. rounding'  | 1/psi | F      |                  | 0        |
| Range            | With respect to the standard the input values are:<br>0: In Range<br>1: Out of Range<br>This includes the boundaries for relative density and temperature and also the check of the pseudo-critical temperature. | -     |        | OOR              | 0        |

### Calculations

The calculations are in either full or partial compliance with the standard, depending on the selected type of API rounding.

## fxAPI\_MPMS\_11\_2\_2M

### Description

The API MPMS 11.2.2M standard consists of a printed table that contains compressibility factors to correct hydrocarbon volumes under pressure to the corresponding volumes at the equilibrium pressure for the metered temperature.

The table contains compressibility factors related to meter temperature and the density at 15°C.

This metric standard corresponds with API MPMS 11.2.2 (the U.S. customary version)

### Boundaries

API MPMS 11.2.2M defines the following limits on the input values:

- 350 to 637 kg/m<sup>3</sup>
- -46 to 60 °C
- 0 to 152 bar(g)

Also the check on the **pseudo-critical** temperature as defined for fxAPI\_MPMS\_11\_2\_2 is applied.

### Compliance

- 11.2.2M - Compressibility Factors for Hydrocarbons: 350 - 637 Kilograms per Cubic Meter Density (15°C) and -46°C to 60 °C Metering Temperature - First Edition, October 1986

### Function inputs

| Function inputs      | Remark  | EU                | SW tag   | Range     | Default |
|----------------------|---|-------------------|----------|-----------|---------|
| Name                 | Optional tag name, tag description and tag group  |                   |          |           |         |
| Density at 15°C      |   | kg/m <sup>3</sup> |          | 0..750    | 0       |
| Observed Temperature |   | °C                |          | -100..150 | 60      |
| Observed Pressure    |   | bar(g)            |          | -1..200   | 0       |
| Equilibrium Pressure | The equilibrium pressure is considered to be 0 psig for liquids which have an equilibrium pressure less than atmospheric pressure (in compliance with API MPMS 12.2 par. 12.2.5.4)  | bar(g)            | EQUIPRES | 0..200    | 0       |
| API 11.2.2M rounding | 0: Disabled<br>The calculation of the compressibility factor F and CPL is performed with full precision.<br>1: Enabled<br>API-MPMS 11.2.2M rounding and truncating rules are applied.<br>The compressibility factor F is rounded in accordance with the standard. |                   | APIROUND | -         | 0       |

### Function outputs

| Function outputs         | Remark  | EU    | SW tag | Alarm            | Fallback |
|--------------------------|---|-------|--------|------------------|----------|
| Status                   | 0: Normal<br>1: Input argument out of range<br>2: Calculation error   |       | STS    | FIOOR<br>CALCERR | 1        |
| CPL                      | Volume correction factor for pressure<br>Value will be rounded according to input 'API 11.2.2M rounding'        | -     | CPL    |                  | 1        |
| F                        | Compressibility factor<br>The output value will be either rounded or not depending input 'API 11.2.2M rounding' | 1/bar | F      |                  | 0        |
| Calculation out of range | With respect to the standard the input values are:<br>0: In Range<br>1: Out of Range                            | -     |        | OOR              | 0        |

### Calculations

The calculations are in either full or partial compliance with the standard, depending on the selected type of API rounding.

## fxAPI\_MPMS\_11\_3\_2\_1

### Description

The function calculates the density of Ethylene (C<sub>2</sub>H<sub>4</sub>, also called Ethene) based on the API MPMS 11.3.2.1 Equation Of State in **USC units**. This API chapter is also known as API Standard 2565.

### Boundaries

The equation of state is valid from 65...165 °F and 200 ... 2100 psia.

### References

- Supplement to API MPMS 11.3.1.1 (API Std. 1565) Ethylene Density, 1974, Reaffirmed 1993.

### Function inputs

| Function inputs | Remark   | EU   | Range     | Default |
|-----------------|--|------|-----------|---------|
| Name            | Optional tag name, tag description and tag group   |      |           |         |
| Temperature     |  | °F   | -100..300 | 0       |
| Pressure        |  | psia | 0...3000  | 0       |
| API rounding    | 0: Disabled<br>The calculations are performed with full precision. A convergence limit of 1e-10 lbm/ft <sup>3</sup> will be applied for the iterative calculations.<br>1: Enabled<br>The calculations are performed in full compliance with the standard. The input, intermediate and output values are rounded as specified and also the iteration limit as specified in the standard is used to achieve convergence. | -    |           | 1       |

### Function outputs

| Function outputs     | Remark   | EU                 | Fallback |
|----------------------|--|--------------------|----------|
| Status               | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence   |                    |          |
| Density              |  | lb/ft <sup>3</sup> | 0        |
| Compressibility      |  | -                  | 0        |
| Equilibrium pressure | Equilibrium pressure at the observed temperature.<br>This property is not currently calculated, as it is not defined in the standard how to do this. | psia               | 0        |
| Range                | With respect to the standard the inputs are:<br>0: In Range<br>1: Out of Range   | -                  | 0        |

### Calculations

The calculations are in compliance with the standard.

## fxAPI\_MPMS\_11\_3\_3\_2

### Description

The API MPMS 11.3.3.2 standard consists of a table with the density values (lbm/ft<sup>3</sup>) of propylene liquid as a function of pressure and temperature. Also part of the standard is the Calculation Procedure to obtain the table values.

### Boundaries

The Calculation Procedure of API MPMS 11.3.3.2 defines the following limits on the input values:

- 30 to 165 °F
- 0 to 1600 psig

### Compliance

- API MPMS 11.3.3.2 Propylene Compressibility Tables, 1974, Reaffirmed 1997.

### Function inputs

| Function inputs      | Remark   | EU   | Range   | Default |
|----------------------|--|------|---------|---------|
| Name                 | Optional tag name, tag description and tag group   |      |         |         |
| Observed temperature |  | °F   | 0..200  | 60      |
| Observed pressure    |  | psia | 0..2000 | 0       |
| API rounding         | 0: Disabled<br>The calculations are performed with full precision.<br>A convergence limit of 1e-10 lbm/ft <sup>3</sup> will be applied for the iterative calculations.<br>1: Enabled<br>The calculated density is rounded to 5 decimal places (same as table values).<br>A convergence limit of 5e-6 lbm/ft <sup>3</sup> will be applied as defined in the standard. | -    |         | 1       |

### Function outputs

| Function outputs         | Remark   | EU                  | SW tag   | Alarm                      | Fallback |
|--------------------------|--|---------------------|----------|----------------------------|----------|
| Status                   | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence   | -                   | STS      | FLOOR<br>CALCERR<br>NOCONV | 1        |
| Density                  | At the observed pressure and temperature   | lbm/ft <sup>3</sup> | DENS     |                            | 0        |
| CTPL                     | Volume correction factor for temperature and pressure (also referred to as the compressibility factor), equals the density at the observed conditions of pressure and temperature value divided by 32.6058 lbm/scf.<br>The value of 32.6058 lbm/scf is specified in the Calculation Procedure of the standard as the propylene standard density at 60 °F and the corresponding vapor pressure. | -                   | CTPL     |                            | 1        |
| Equilibrium pressure     | Equilibrium pressure at the observed temperature.<br>Also referred to as vapor pressure or saturated pressure  | psia                | EQUIPRES |                            | 0        |
| Calculation out of range | With respect to the standard the input values are:<br>0: In Range<br>1: Out of Range   | -                   |          | OOR                        | 0        |

### Calculations

The calculations are in full or partial compliance with the standard depending on input 'API rounding'.



## fxAPI\_RD60F\_1980

### Description

#### Relative Density (T, P) <--> Relative Density (60°F, equilibrium pressure)

This function converts a relative density value at the observed temperature and pressure to the relative density at 60°F and the equilibrium pressure (typically 0 psig) or vice versa.

The temperature conversion is according to API-2540, Tables 23A/24A (Generalized Crude Oils) and 23B/24B (Refined Oil Products), while the volume correction for pressure according to API MPMS 11.2.1.

In 1982 API published tables 5D, 6D, 53D and 54D for lubricating oil products as part of API MPMS 11.1. Although tables 23D and 24D are not covered in an official API standard the Flow-X series of flow computer supports tables 23D and 24D as well by combining the calculation of tables 23A/B and 24A/B with the K0 and K1 constants published in the other tables for lubricating oils.

Note: this function is a combination of API2540 and API 11.2.1. For the calculation from observed to standard conditions an iterative calculation is required. The rounding and truncating of input and intermediate values is implemented such that the example calculations as specified in both standards are exactly reproduced.

### Compliance

- API MPMS 11.1 Volume X (API Standard 2540) - Table 23A - Generalized Crude Oils, Correction of Observed Relative Density to Relative Density at 60/60°F - First Edition, August 1980
- API MPMS 11.1 Volume X (API Standard 2540) - Table 23B - Generalized Products, Correction of Observed Relative Density to Relative Density at 60/60°F - First Edition, August 1980
- API MPMS 11.1 Volume X (API Standard 2540) - Table 24A - Generalized Crude Oils, Correction of Volume to 60°F against Relative Density at 60/60°F - First Edition, August 1980
- API MPMS 11.1 Volume X (API Standard 2540) - Table 24B - Generalized Products Correction of Volume to 60°F against Relative Density at 60/60°F - First Edition, August 1980
- API MPMS 11.2.1 - Compressibility Factors for Hydrocarbons: 0 - 90°API Gravity Range - First Edition, August 1984

### Function inputs

| Function inputs        | Remark   | EU   | SW tag     | Range     | Default |
|------------------------|--|------|------------|-----------|---------|
| Name                   | Optional tag name, tag description and tag group   |      |            |           |         |
| Input relative density | Depending on the conversion method this is the relative density either at the observed temperature and observed pressure or at 60 °F and the equilibrium pressure  | -    |            | 0..1.3    | 0       |
| Observed temperature   |  | °F   |            | -100..400 | 60      |
| Observed pressure      |  | psig |            | -10..2000 | 0       |
| Product                | 1: A - Crude Oil<br>2: B - Auto select<br>Selection based on relative density at 60 °F<br>3: B - Gasoline<br>4: B - Transition Area<br>5: B - Jet Fuels<br>6: B - Fuel Oil<br>7: D - Lubricating Oil   |      | PRDTYP     | -         | 1       |
| API-2540 rounding      | 0: Disabled<br>The calculations are performed with full precision and the final CTL value is rounded as specified by input 'CTL decimal places'<br>1: Enabled for computational value<br>API-2540 rounding and truncating rules are applied and, in case of conversion method 2 (standard to observed), the computational value for CTL as specified in Table 24 is used, meaning that the CTL value has:<br>4 decimal places if CTL >=1<br>5 decimal places if CTL < 1.<br>2: Enabled for table value<br>API-2540 rounding and truncating rules are applied and, in case of conversion method 2 (standard to observed), the table value for CTL as specified in Table 24 meaning that the CTL value has 4 decimal places in all cases<br>3: Enabled with 5 decimal places<br>API-2540 rounding and truncating rules are applied, and, in case of conversion method 2 (standard to observed), the CTL value has 5 decimal places in all cases.<br>Note: although not strictly in accordance with the standard, this option is more commonly used than option 'Enabled for computational value'<br>Note: for conversion type 1 'From observed to standard conditions' the CTL |      | API2540RND | -         | 0       |

| Function inputs       | Remark  | EU   | SW tag     | Range   | Default |
|-----------------------|---|------|------------|---------|---------|
|                       | factor is rounded to 6 decimal places when input 'API 2540 rounding' > 0, as in accordance with table 23.   |      |            |         |         |
| Hydrometer correction | Only applies for conversion method<br>'1: From observed to standard conditions'<br>0: Disabled<br>1: Enabled  | -    | HYDROCOR   |         | 0       |
| API 11.2.1 rounding   | 0: Disabled<br>The calculation of the compressibility factor F is performed with full precision<br>1: Enabled<br>API-MPMS 11.2.1 rounding and truncating rules are applied. The compressibility factor F is rounded to 3 decimal places as specified in the standard. | -    | API1121RND |         | 0       |
| Equilibrium pressure  | The equilibrium pressure is considered to be 0 psig for liquids which have an equilibrium pressure less than atmospheric pressure (in compliance with API MPMS 12.2 par. 12.2.5.4)  | psig | EQUIPRES   | 0..2000 | 0       |
| Conversion method     | 1: From observed to standard conditions<br>2: From standard to observed conditions  |      | CONVERSION |         | 1       |

### Function outputs

| Function outputs        | Remark   | EU    | SW tag | Alarm                      | Fallback |
|-------------------------|--|-------|--------|----------------------------|----------|
| Status                  | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence   | -     | STS    | FIOOR<br>CALCERR<br>NOCONV | 1        |
| Output relative density | Depending on the conversion method this is the relative density either at 60 °F and the equilibrium pressure or at the observed temperature and observed pressure  | -     | RD     |                            | 0        |
| CTL                     | Volume correction factor for temperature.<br>Value will be rounded according to input 'API2540 rounding'   | -     | CTL    |                            | 1        |
| CPL                     | Volume correction factor for pressure<br>Value will be rounded according to input 'API 11.2.1 rounding'  | -     | CPL    |                            | 1        |
| CTPL                    | Combined volume correction factor<br>CTPL = CTL * CPL  | -     | CTPL   |                            | 1        |
| K0                      | Actual value of constant K0 used for CTL calculation   | -     | K0     |                            | 0        |
| K1                      | Actual value of constant K1 used for CTL calculation   | -     | K1     |                            | 0        |
| K2                      | Actual value of constant K2 used for CTL calculation   | -     | K2     |                            | 0        |
| Alpha                   | Thermal expansion factor   | 1/°F  | ALPHA  |                            | 0        |
| F                       | Compressibility factor   | 1/psi | F      |                            | 0        |
| Product                 | When input 'Product' is 'B - Auto select', then the output is set to the actual selected product of table 23B/24B (enumerative value as defined for input 'Product'), else the output is set equal to input 'Product'. | -     | PRDCUR |                            | 0        |
| CTL calc out of range   | With respect to the standard used for the calculation of CTL the combination of input values is:<br>0: In Range<br>1: Out of Range   |       |        | CTLOOR                     | 0        |
| CPL calc out of range   | With respect to the standard used for the calculation of CPL the combination of input values is:<br>0: In Range<br>1: Out of Range   |       |        | CPLOOR                     | 0        |

### Calculations

The calculations depend on the conversion method.

#### Conversion method 1: from observed to standard conditions.

The function performs the following iterative algorithm to calculate the relative density at standard conditions:

- 1 First the inputs are rounded in accordance with the API2540 standard, provided that API2540 rounding is enabled.
- 2 The observed density [kg/m<sup>3</sup>] is calculated from the observed relative density
- 3 The hydrometer correction on the observed density is applied, provided that this correction is enabled
- 4 At the start of the iteration the initial value for density and relative density at [60 °F, equilibrium pressure] is set to respectively the observed density and the observed relative density. The initial CPL value is set to 1.
- 5 When the type of product is set to 'B – Auto select' (automatic selection of the refined product range) the K0, K1 and K2

factors are determined based on the relative density at [60 °F, equilibrium pressure]. The Transition area is only taken in consideration in the 2<sup>nd</sup> iteration loop, as specified in the standard.

- 6 The Alpha factor is calculated according from the density at [60 °C, equilibrium pressure] and the K0, K1 and K2 factor. If API2540 rounding is enabled, then the intermediate results are rounded or truncated as specified API-2540 Table 23.
- 7 The CTL value is calculated according to API-2540 Table 23 from the Alpha factor and the differential temperature (= observed temperature – 60°F). If API2540 rounding is enabled, then the intermediate results are rounded or truncated as specified API-2540 Table 23.
- 8 Depending on the type of API2540 rounding the calculated CTL value is rounded to 6 decimal places or not rounded at all.
- 9 The density at [60 °F, equilibrium pressure] is calculated by dividing the observed density by the new CTL value and the CPL value from the previous iteration.

- 10 The relative density at [60 °F, equilibrium pressure] is calculated from the density at [60 °F, equilibrium pressure]
- 11 Because API 11.2.1 requires the API gravity value at 60 °F, the API gravity at [60 °F, equilibrium pressure] is calculated from the density at [60 °F, equilibrium pressure].
- 12 The compressibility factor is calculated according to API MPMS 11.2.1 from the API gravity at [60 °F, equilibrium pressure] and the 'Observed temperature'. If API 11.2.1 rounding is enabled then the API gravity and temperature are rounded and the calculations are performed in accordance with the rounding and truncating rules of the standard.
- 13 The CPL value is calculated from the compressibility factor and the 'Observed pressure' and 'Equilibrium pressure' input values.
- 14 The density at [60°F, equilibrium pressure] is calculated by dividing the observed density by CTL and the new CPL value.
- 15 If API2540 rounding is enabled then the density at [60°F, equilibrium pressure] value is rounded to 3 decimal places as specified in the standard.
- 16 The relative density at [60 °F, equilibrium pressure] is calculated from the density at [60 °F, equilibrium pressure]
- 17 If API2540 rounding is enabled then the relative density at [60°F, equilibrium pressure] value is rounded to 4 decimal places as specified in the standard.
- 18 Steps 5 through 17 are repeated taking the density value from step 14 as the start value for the next iteration until the absolute difference between two consecutive density values is either 0.05 (or 0.07 for the transition area) or 0.000001, depending of API2540 rounding being enabled or not.
- 19 For refined products the entire iteration loop is repeated if the relative density at [60°F, equilibrium pressure] appears to be in a different product region than the observed relative density. This is required because a different product region means different K0, K1 and K2 factors.
- 20 If API 11.2.4 rounding is enabled, then the relative density value at [60°F, equilibrium pressure] is rounded to 0.0001

**Conversion method 2:** from standard to observed conditions.

The function performs straightforward calculations to determine the relative density at observed conditions:

- 1 First the inputs are rounded in accordance with the API2540 standard, provided that API2540 rounding is enabled.
- 2 The density at [60°F, equilibrium pressure] is calculated from the input relative density
- 3 When the type of product is set to 'B – Auto select' (automatic selection of the refined product range) the K0, K1 and K2 factors are determined based on the input relative density
- 4 The Alpha factor is calculated according from the density at [60°F, equilibrium pressure] and the K0, K1 and K2 factor. If API2540 rounding is enabled, then the intermediate results are rounded or truncated as specified API-2540 Table 24.
- 5 The CTL value is calculated according to API-2540 Table 24 from the Alpha factor and the differential temperature (= observed temperature – 60°F). If API2540 rounding is enabled, then the intermediate results are rounded or truncated as specified API-2540 Table 24.
- 6 Depending on the type of API2540 rounding the calculated CTL value is rounded to 4 or 5 decimal places or not rounded at all.
- 7 Because API 11.2.1 requires the API gravity value at 60 °F, the API gravity at [60 °F, equilibrium pressure] is calculated from the density at [60 °F, equilibrium pressure].
- 8 The compressibility factor is calculated according to API MPMS 11.2.1 from the input density and temperature'. If API 11.2.1 rounding is enabled then the input density and temperature are rounded and the calculations are performed in accordance with the rounding and truncating rules of the standard.
- 9 The CPL value is calculated from the compressibility factor and the 'Observed pressure' and 'Equilibrium pressure' input values.
- 10 The relative density at observed temperature and pressure is calculated from the input relative density and the CTL and the CPL values.

## fxAPI\_SG60F\_1952

### Description

#### Specific Gravity (T, P) <--> Specific Gravity (60°F, equilibrium pressure)

This function converts a specific gravity value at the observed temperature and pressure to the specific gravity at 60°F and the equilibrium pressure (typically 0 psig) or vice versa.

The temperature conversion is according to ASTM-IP Petroleum Measurements Tables 1952 (Also known as API-1952 tables) Table 24.

Note: this function is a combination of the API 1952 Tables and API 11.2.1. For the calculation from observed to standard conditions an iterative calculation is required. The rounding and truncating of input and intermediate values is implemented such that the example calculations as specified in both standards are exactly reproduced.

### Compliance

- ASTM-IP Petroleum Measurement Tables, American Edition, United States Units of Measurement, 1952
- API MPMS 11.2.1 - Compressibility Factors for Hydrocarbons: 0 - 90°API Gravity Range - First Edition, August 1984

### Function inputs

| Function inputs        | Remark  | EU   | SW tag     | Range     | Default |
|------------------------|---|------|------------|-----------|---------|
| Name                   | Optional tag name, tag description and tag group  |      |            |           |         |
| Input Specific Gravity | Depending on the conversion method this is the Specific Gravity either at the observed temperature and observed pressure or at 60 °F and the equilibrium pressure   | -    |            | 0..1.3    | 0       |
| Observed temperature   |   | °F   |            | -100..400 | 60      |
| Observed pressure      |   | psig |            | -10..2000 | 0       |
| API 11.2.1 rounding    | 0: Disabled<br>The calculation of the compressibility factor F is performed with full precision<br>1: Enabled<br>API-MPMS 11.2.1 rounding and truncating rules are applied. The compressibility factor F is rounded to 3 decimal places as specified in the standard. | -    | API1121RND |           | 0       |
| Equilibrium pressure   | The equilibrium pressure is considered to be 0 psig for liquids which have an equilibrium pressure less than atmospheric pressure (in compliance with API MPMS 12.2 par. 12.2.5.4).   | psig | EQUIPRES   | 0..2000   | 0       |
| Conversion method      | 1: From observed to standard conditions<br>2: From standard to observed conditions  |      | CONVERSION |           | 1       |

### Function outputs

| Function outputs        | Remark  | EU    | SW tag | Alarm                      | Fallback |
|-------------------------|---|-------|--------|----------------------------|----------|
| Status                  | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence  | -     | STS    | FLOOR<br>CALCERR<br>NOCONV | 1        |
| Output Specific Gravity | Depending on the conversion method this is the Specific Gravity either at 60 °F and the equilibrium pressure or at the observed temperature and observed pressure | -     | RD     |                            | 0        |
| CTL                     | Volume correction factor for temperature.   | -     | CTL    |                            | 1        |
| CPL                     | Volume correction factor for pressure<br>Value will be rounded according to input 'API 11.2.1 rounding'   | -     | CPL    |                            | 1        |
| CTPL                    | Combined volume correction factor<br>CTPL = CTL * CPL   | -     | CTPL   |                            | 1        |
| F                       | Compressibility factor  | 1/psi | F      |                            | 0        |
| CTL calc out of range   | With respect to the standard used for the calculation of CTL the combination of input values is:<br>0: In Range<br>1: Out of Range                                |       |        | CTLOOR                     | 0        |
| CPL calc out of range   | With respect to the standard used for the calculation of CPL the combination of input values is:<br>0: In Range<br>1: Out of Range                                |       |        | CPLOOR                     | 0        |

## Calculations

The calculations depend on the conversion method.

### Conversion method 1: from observed to standard conditions.

The function performs the following iterative algorithm to calculate the Specific Gravity at standard conditions:

- 1 At the start of the iteration the initial value for Specific Gravity at [60 °F, equilibrium pressure] is set to the Observed Specific Gravity. The initial CPL value is set to 1.
- 2 The CTL value is determined from the Specific Gravity at [60 °F, equilibrium pressure] according to API 1952 Table 24.
- 3 The Specific Gravity at [60 °F, equilibrium pressure] is calculated from the Observed specific gravity, the new CTL value and the CPL value from the previous iteration.
- 4 Because API 11.2.1 requires the API gravity value at 60 °F, the API gravity at [60 °F, equilibrium pressure] is calculated from the Specific gravity at [60 °F, equilibrium pressure].
- 5 The compressibility factor is calculated according to API MPMS 11.2.1 from the API gravity at [60 °F, equilibrium pressure] and the 'Observed temperature'. If API 11.2.1 rounding is enabled then the API gravity and temperature are rounded and the calculations are performed in accordance with the rounding and truncating rules of the standard.
- 6 The CPL value is calculated from the compressibility factor and the 'Observed pressure' and 'Equilibrium pressure' input values.
- 7 The Specific Gravity at [60°F, equilibrium pressure] is calculated by dividing the Observed Specific Gravity by the CTL and the new CPL value.
- 8 Steps 2 through 7 are repeated taking the specific gravity value from step 7 as the start value for the next iteration until the absolute difference between two consecutive specific gravity values is 0.0001.

### Conversion method 2: from standard to observed conditions.

The function performs straightforward calculations to determine the Specific Gravity at observed conditions:

- 1 The CTL value is calculated according to API 1952 Table 24
- 2 Because API 11.2.1 requires the API gravity value at 60 °F, the API gravity is calculated from the 'Input Specific Gravity'.
- 3 The compressibility factor is calculated according to API MPMS 11.2.1 from the API gravity and the 'Observed temperature'. If API 11.2.1 rounding is enabled then the input density and temperature are rounded and the calculations are performed in accordance with the rounding and truncating rules of the standard.
- 4 The CPL value is calculated from the compressibility factor and the 'Observed pressure' and 'Equilibrium pressure' input values.
- 5 The output Specific Gravity (at observed temperature and pressure) is calculated from the input Specific Gravity and the CTL and the CPL values.

## fxAPI\_RD60F\_NGL\_LPG

### Description

#### Relative Density (T, P) <--> Relative Density (60°F, Pe)

This function converts the relative density value at the observed temperature and pressure to the relative density value at 60°F and the equilibrium pressure or vice versa.

The temperature correction is according to API MPMS 11.2.4:2007 (GPA TP-25 / GPA TP-27), while the pressure correction is according to API MPMS 11.2.2:1984.

The calculation of the equilibrium pressure is according to GPA TP-15 (API MPMS 11.2.2 Addendum:1994).

### Compliance

- API MPMS 11.2.4: Temperature Correction for the Volume of NGL and LPG Tables 23E, 24E, 53E, 54E, 59E & 60E, September 2007
- GPA TP-27: Temperature Correction for the Volume of NGL and LPG Tables 23E, 24E, 53E, 54E, 59E & 60E, September 2007
- GPA TP-25: Temperature Correction for the volume of Light Hydrocarbons – Tables 24E and 23E, 1998
- API MPMS 11.2.2 - Compressibility Factors for Hydrocarbons: 0.350 - 0.637 Relative Density (60°F/60°F) and -50°F to 140°F Metering Temperature - Second Edition, October 1986
- API MPMS 11.2.5: A Simplified Vapor Pressure Correlation for Commercial NGLs, September 2007
- GPA TP-15: A Simplified Vapor Pressure Correlation for Commercial NGLs, September 2007 (also covers GPA TP-15 1988)
- API MPMS 11.2.2 Addendum : Compressibility Factors for Hydrocarbons: Correlation of Vapor Pressure for Commercial Natural Gas Liquids (same as GPA TP-15:1988)

### Function inputs

| Name                       | Remark   | EU   | SW tag     | Range     | Default |
|----------------------------|--|------|------------|-----------|---------|
| Name                       | Optional tag name, tag description and tag group   |      |            |           |         |
| Input relative density     | Depending on the conversion method this represents the relative density either at the observed temperature and pressure or at 60 °F and the equilibrium pressure   | -    |            | 0..0.75   | 0       |
| Observed temperature       | Temperature at which the relative density is observed  | °F   |            | -100..300 | 60      |
| Observed pressure          | Pressure at which the relative density is observed   | psia |            | -10..2500 | 0       |
| API 11.2.4 rounding        | 0: Disabled<br>The calculations are performed with full precision and the output values are not rounded<br>1: Enabled<br>The input and output values are rounded as defined in the standard  |      | API1124RND |           | 0       |
| API 11.2.2 rounding        | 0: Disabled<br>The calculations are performed with full precision and the output values are not rounded<br>1: Enabled<br>The input and output values are rounded as defined in the standard  |      | API1122RND |           | 0       |
| Equilibrium pressure mode  | 1: Use Input<br>The value of input 'Equilibrium pressure value' is used for the calculation of CPL<br>2: GPA TP-15<br>The equilibrium pressure is calculated in accordance with GPA TP-15  |      | EQUIPMODE  |           | 2       |
| Equilibrium pressure value | Only used when input 'Equilibrium pressure mode' is set to 'Use input'. The value will be used for the calculation of the CPL  | psia | EQUIPINP   |           | 0       |
| GPA TP-15 rounding         | 0: Disabled<br>Full precision (no rounding and truncating applied)<br>1: Enabled<br>Rounding as defined in ' GPA TP15:1988 / API MPMS 11.2.2 Addendum':1994  | -    | TP15RND    |           | 0       |
| P100 Correlation           | 0: Disabled<br>The standard correlation is commonly used for pure products such as propane, butane and natural gasoline. It only requires the relative density and the temperature to calculate the vapor pressure<br>1: Enabled<br>The improved correlation requires the vapor pressure at 100°F (37.8 °C). This method is better suited for varied NGL mixes Where different product mixes could have the same specific gravity but different equilibrium pressures. | -    | P100CORR   |           | 0       |
| Vapor pressure at 100°F    |  | psia | EQUIP100F  | 0..2500   | 0       |
| Conversion method          | 1: From observed to standard conditions<br>2: From standard to observed conditions   |      | CONVMETH   |           | 1       |

### Function outputs

| Name   | Remark    | EU | SW tag | Alarm | Fallback |
|--------|-----------|----|--------|-------|----------|
| Status | 0: Normal | -  | STS    |       |          |

| Name                    | Remark   | EU    | SW tag   | Alarm                      | Fallback               |
|-------------------------|--|-------|----------|----------------------------|------------------------|
|                         | 1: Input argument out of range<br>2: Calculation error<br>3: No convergence  |       |          | FIOOR<br>CALCERR<br>NOCONV |                        |
| Output relative density | Depending on the conversion method this represents the relative density either at 60 °F and the equilibrium pressure or at the observed temperature and pressure   | -     | DENS     |                            | Input relative density |
| CTL                     | Volume correction factor for temperature.<br>Value will be rounded according to input 'API 11.2.4 rounding'  | -     | CTL      |                            | 1                      |
| CPL                     | Volume correction factor for pressure<br>Value will be rounded according to input 'API 11.2.2. rounding'   | -     | CPL      |                            | 1                      |
| CTPL                    | Combined volume correction factor<br>CTPL = CTL * CPL  | -     | CTPL     |                            | 1                      |
| F                       | Compressibility factor<br>The output value will be either rounded or not depending input 'API rounding'  | 1/psi | F        |                            | 0                      |
| Equilibrium pressure    | The equilibrium pressure calculated by GPA TP-15<br>Will be set to 0 when equilibrium pressure is below atmospheric pressure   | psia  | EQUIPCUR |                            | 0                      |
| CTL calc out of range   | With respect to the API 11.2.4 standard the combination of input values is:<br>0: In Range<br>1: Out of Range<br>The following range checks apply:<br>0.21 <= RD <= 0.74<br>-50.8 <= T <= 199.4 °F<br>Table 23E reference fluid ranges   |       |          | CTLOOR                     | 0                      |
| CPL calc out of range   | With respect to API 11.2.2M the combination of input values is:<br>0: In Range<br>1: Out of Range<br>The following range checks apply:<br>350 <= Density 15 °C <= 637 kg/m <sup>3</sup><br>-46 °C <= T <= 60 °C<br>Also the check on the <b>pseudo-critical</b> temperature as defined for fxAPI_MPMS_11_2_2 is applied.   |       |          | CPLOOR                     | 0                      |
| GPA TP-15 out of range  | Only set when the GPA TP-15 calculation is enabled<br>With respect to the GPA TP-15 standard the combination of input values is:<br>0: In Range<br>1: Out of Range<br>The following range checks apply:<br>For lower range:<br>0.350 <= RD60 < 0.425<br>-50 to (695.51*RD60 - 155.51) °F<br>Higher range:<br>0.425 <= RD60 <= 0.676<br>-50 to 140 °F<br>with RD60 being the relative density at 60°F | -     |          | TP15OOR                    | 0                      |

## Calculations

The calculations depend on the conversion method.

### Conversion method 1: from observed to standard conditions.

The function performs the following iterative algorithm to calculate the relative density at 60 °F and the equilibrium pressure.

- When API 11.2.4 rounding is enabled, the input relative density and temperature values are rounded in accordance with the standard
- At the start of the iteration the relative density at [60 °F, equilibrium pressure] is set equal to the observed relative density and the CPL value is set to 1.
- First the relative density corrected for pressure is calculated by dividing the observed relative density by the CPL value.
- The CTL value and the relative density at [60 °F, equilibrium pressure] is calculated from the relative density corrected for pressure and the observed temperature according to Table 23E
- Depending on the value of input 'Equilibrium pressure mode', either value of input 'Equilibrium pressure value' is used or the equilibrium pressure (vapor pressure) is calculated according to GPA TP-15. Whether the GPA TP-15 rounding and truncation rules are applied is dictated by input 'GPA-TP15 rounding'

- The compressibility factor F is calculated according to API MPMS 11.2.2 from the relative density at [60 °F, equilibrium pressure] and the 'Observed temperature', with, depending on input API 11.2.2, rounding and truncation according to the standard.
- The CPL value is calculated from the compressibility factor, the equilibrium pressure and the 'Observed pressure' input value.
- The new value for relative density at [60°F, equilibrium pressure] is calculated by dividing the observed density by the CTL and CPL values.
- Steps 3 though 8 are repeated taking the density value from step 8 as the starting value until the absolute difference between two consecutive density values is less than the convergence limit.

To avoid convergence problems different convergence limits are applied, depending on whether API 11.2.2 and/or GPA TP-15 rounding is applied:

If API 11.2.2M rounding is enabled -> Limit = 0.00005 kg/m<sup>3</sup>  
 else if GPA TP-15 rounding is enabled -> Limit = 0.000005 kg/m<sup>3</sup>  
 else -> Limit = 0.00000001 kg/m<sup>3</sup>

10 If API 11.2.4 rounding is enabled, then the relative density at [60°F, equilibrium pressure] is rounded to 0.0001

**Conversion method 2:** from standard to observed conditions.

The function performs straightforward calculations to determine the density at observed conditions:

- 1 When API 11.2.4 rounding is enabled, the input relative density and temperature values are rounded in accordance with the standard
- 2 The CTL value is calculated according to API MPMS 11.2.4 (GPA TP-27) Table 24E from the density at [15 °C, equilibrium pressure] and the 'Observed temperature'.
- 3 Depending on the value of input 'Equilibrium pressure mode', either value of input 'Equilibrium pressure value' is used or the equilibrium pressure (vapor pressure) is calculated according to GPA TP-15.
- 4 The compressibility factor is calculated according to API MPMS 11.2.2 from the input relative density and the 'Observed temperature'.
- 5 The CPL value is calculated from the compressibility factor, the equilibrium pressure and the 'Observed pressure' input value.
- 6 If API 11.2.4 rounding is enabled, then the CTL value is rounded at [60°F, equilibrium pressure] is rounded to 0.00001
- 7 The relative density at the observed conditions is calculated by multiplying the input relative density by the CTL value and the CPL value.



## fxAPI\_Table5\_1952

### Description

°API (T) --> °API (60°F)

This function converts an API gravity value at the observed temperature to the API gravity value at 60°F in accordance with API 1952 Table 5.

### Function inputs

| Function inputs      | Remark   | EU   | SW tag | Range     | Default |
|----------------------|--|------|--------|-----------|---------|
| Name                 | Optional tag name, tag description and tag group |      |        |           |         |
| Observed API         | Observed API gravity                             | °API |        | -20..120  | 0       |
| Observed temperature | Temperature at which the API gravity is observed | °F   |        | -100..400 | 60      |

### Function outputs

| Function outputs         | Remark   | EU   | SW tag | Alarm   | Fallback |
|--------------------------|--|------|--------|---------|----------|
| Status                   | 0: Normal  | -    | STS    |         | 1        |
|                          | 1: Input argument out of range                     |      |        | FLOOR   |          |
|                          | 2: Calculation error                               |      |        | CALCERR |          |
|                          | 3: No convergence                                  |      |        | NOCONV  |          |
| API at 60 °F             | API gravity at 60°F                                | °API | API    |         | 0        |
| Calculation out of range | With respect to the standard the input values are: | -    |        | OOR     | 0        |
|                          | 0: In Range  |      |        |         |          |
|                          | 1: Out of Range                                    |      |        |         |          |

### Calculations

The table values are the standard, so no calculations are involved. The function performs an interpolation between the table values that correspond to the input values.

### Compliance

- ASTM-IP Petroleum Measurement Tables, American Edition, United States Units of Measurement, 1952

## fxAPI\_Table5\_1980

### Description

°API (T) --> °API (60°F)

This function converts an API gravity value at the observed temperature to the API gravity value at 60°F.

The temperature conversion is according to API MPMS 11.1:1980 (API-2540), Tables 5A (Generalized Crude Oils) and 5B (Refined Oil Products) and API MPMS 11.1 Chapter XIII Table 5D: 1984 (Lubricating Oils).

The function provides the option to correct for readings taken from a hydrometer as specified in the API-2540 standard.

### Function inputs

| Function inputs       | Remark  | EU   | SW tag   | Range     | Default |
|-----------------------|---|------|----------|-----------|---------|
| Name                  | Optional tag name, tag description and tag group  |      |          |           |         |
| Observed API          | Observed API gravity  | °API |          | -20..120  | 0       |
| Observed temperature  | Temperature at which the API gravity is observed  | °F   |          | -100..400 | 60      |
| Product               | 1: A - Crude Oil<br>2: B - Auto select<br>Selection based on °API at 60 °F<br>3: B - Gasoline<br>4: B - Transition Area<br>5: B - Jet Fuels<br>6: B - Fuel Oil<br>7: D - Lubricating Oil  |      | PRDTYP   |           | 1       |
| API2540 rounding      | 0: Disabled<br>The calculations are performed with full precision.<br>A convergence limit of 0.000001 kg/m3 will be applied for the iterative calculations.<br>1: Enabled<br>API-2540 rounding and truncating rules are applied.<br>A convergence limit of 0.05 kg/m3 will be applied as defined in the standard. |      | APIROUND |           | 0       |
| Hydrometer correction | 0: Disabled<br>1: Enabled   |      | HYDROCOR |           | 0       |

### Function outputs

| Function outputs         | Remark  | EU   | SW tag | Alarm                      | Fallback |
|--------------------------|---|------|--------|----------------------------|----------|
| Status                   | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence  | -    | STS    | FLOOR<br>CALCERR<br>NOCONV | 1        |
| API at 60 °F             | API gravity at 60°F   | °API | API    |                            | 0        |
| CTL                      | Volume correction factor for temperature.   | -    | CTL    |                            | 1        |
| K0                       | Actual value of constant K0 used for CTL calculation  | -    | K0     |                            | 0        |
| K1                       | Actual value of constant K1 used for CTL calculation  | -    | K1     |                            | 0        |
| K2                       | Actual value of constant K2 used for CTL calculation  | -    | K2     |                            | 0        |
| Alpha                    | Thermal expansion factor  | 1/°F | ALPHA  |                            | 0        |
| Product                  | When input 'Product' is 'B - Auto select', then the output is set to the actual selected product of table 5B (enumerative value as defined for input 'Product'), else the output is set equal to input 'Product'. | -    | PRDCUR |                            | 0        |
| Calculation out of range | With respect to the standard the input values are:<br>0: In Range<br>1: Out of Range  | -    |        | 00R                        | 0        |

### Calculations

The calculations are in full or partial compliance with the standard depending on input 'API 2540 rounding'.

### Compliance

- API MPMS 11.1 Volume X (API Standard 2540) - Table 5A - Generalized Crude Oils, Correction of Observed API Gravity to API Gravity at 60°F - First Edition, August 1980
- API MPMS 11.1 Volume X (API Standard 2540) - Table 5B - Generalized Products, Correction of Observed API Gravity to API Gravity at 60°F- First Edition, August 1980
- API MPMS 11.1 Volume XIII - Table 5D - Generalized Lubricating Oils, Correction of Observed API Gravity to API Gravity at 60°F - January 1982

## fxAPI\_Table5\_2004

### Description

°API (T, P) --> °API (60°F, 0 psig)

This function converts an API gravity value at the observed temperature and pressure to the API gravity value at 60°F and 0 psig.

The temperature and pressure correction is according to API MPMS 11.1:2004.

An iterative calculation needs to be applied to convert the observed API gravity to the value at base conditions.

### Function inputs

| Function inputs      | Remark  | EU   | SW tag   | Range     | Default |
|----------------------|---|------|----------|-----------|---------|
| Name                 | Optional tag name, tag description and tag group  |      |          |           |         |
| Observed API         | Observed API gravity  | °API |          | -20..180  | 0       |
| Observed temperature | Temperature at which the API gravity is observed  | °F   |          | -100..400 | 60      |
| Observed pressure    | Pressure at which the API gravity is observed   | psig |          | -10..2000 | 0       |
| Product              | 1: A - Crude Oil<br>2: B - Auto select<br>Selection based on °API at 60 °F<br>3: B - Gasoline<br>4: B - Transition Area<br>5: B - Jet Fuels<br>6: B - Fuel Oil<br>7: D - Lubricating Oil  |      | PRDTYP   |           | 1       |
| API rounding         | 0: Disabled<br>The calculations are performed with full precision and the final CTL, CPL and CTPL values are rounded as specified by the inputs 'CTL / CPL / CTPL decimal places'<br>1: Enabled<br>The input and output values are rounded in compliance with the standard. The CTL, CPL and CTPL value are rounded to 5 decimal places |      | APIROUND |           | 0       |

### Function outputs

| Function outputs         | Remark   | EU    | SW tag | Alarm                      | Fallback |
|--------------------------|--|-------|--------|----------------------------|----------|
| Status                   | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence within 15 iterations  | -     | STS    | FIOOR<br>CALCERR<br>NOCONV |          |
| API at 60 °F             | API gravity at 60°F and 0 psig   | -     | API    |                            | 0        |
| CTL                      | Volume correction factor for temperature.<br>Value will be rounded according to input 'API rounding'   | -     | CTL    |                            | 1        |
| CPL                      | Volume correction factor for pressure<br>Value will be rounded according to input 'API rounding'   | -     | CPL    |                            | 1        |
| CTPL                     | Combined volume correction factor<br>CTPL = CTL * CPL  | -     | CTPL   |                            | 1        |
| K0                       | Actual value of constant K0 used for CTL calculation   | -     | K0     |                            | 0        |
| K1                       | Actual value of constant K1 used for CTL calculation   | -     | K1     |                            | 0        |
| K2                       | Actual value of constant K2 used for CTL calculation   | -     | K2     |                            | 0        |
| Alpha                    | Thermal expansion factor   | 1/°F  | ALPHA  |                            | 0        |
| F                        | Compressibility factor   | 1/psi | F      |                            | 0        |
| Product                  | When input 'Product' is 'B - Auto select', then the output is set to the actual selected product of table B (enumerative value as defined for input 'Product'), else the output is set equal to input 'Product'. | -     | PRDCUR |                            | 0        |
| Calculation out of range | With respect to the standard the input values are:<br>0: In Range<br>1: Out of Range   | -     |        | OOR                        | 0        |

### Calculations

The calculations are in either full or partial compliance with the standard, depending on whether API rounding is enabled or not.

Note: As opposed to API-2540, the 2004 standard does not include a correction for readings taken from a hydrometer and assumes that the equilibrium pressure is below atmospheric pressure, so taking 0 psig as the base pressure.

### Compliance

- API MPMS 11.1 Temperature and Pressure Volume Correction Factors for Generalized Crude Oils, Refined Products and Lubricating Oils, May 2004

fxAPI\_Table6\_1952

Description

°API (60°F, 0 psig) --> CTL

This function calculates the volume correction factor for temperature from the API gravity value at 60°F and the observed temperature according to API 1952 Table 6.

Compliance

- ASTM-IP Petroleum Measurement Tables, American Edition, United States Units of Measurement, 1952

Function inputs

| Function inputs      | Remark   | EU   | SW tag | Range     | Default |
|----------------------|--|------|--------|-----------|---------|
| Name                 | Optional tag name, tag description and tag group |      |        |           |         |
| API at 60 °F         | API gravity at 60°F and the equilibrium pressure | °API |        | -20..120  | 0       |
| Observed temperature |  | °F   |        | -100..400 | 60      |

Function outputs

| Function outputs         | Remark   | EU | SW tag | Alarm | Fallback |
|--------------------------|--|----|--------|-------|----------|
| Status                   | 0: Normal  | -  | STS    |       | 1        |
|                          | 1: Input argument out of range                     |    |        | FIOOR |          |
|                          | 2: Calculation error                               |    |        | CALC  |          |
| CTL                      | Volume correction factor for temperature.          | -  | CTL    |       | 1        |
| Calculation out of range | With respect to the standard the input values are: | -  |        |       | 0        |
|                          | 0: In Range  |    |        |       |          |
|                          | 1: Out of Range                                    |    |        | OOR   |          |

Calculations

The table values are the standard, so no calculations are involved. The function performs an interpolation between the table values that correspond to the input values.

Boundaries

Table 6 contains values for the following range:

| Input value          | Normal Range | EU   |
|----------------------|--------------|------|
| API Gravity at 60 °F | 0 .. 100     | °API |
| Observed temperature | 0 .. 300     | °F   |

Note that the table does not cover the full range, e.g. for an API gravity of 70 the table only specifies values between 0 .. 150 °F.

## fxAPI\_Table6\_1980

### Description

**°API (60°F, 0 psig) --> CTL**

This function calculates the volume correction factor for temperature from the API gravity value at 60°F and the observed temperature.

The temperature conversion is according to API-2540, Tables 6A (Generalized Crude Oils) and 6B (Refined Oil Products) and API MPMS 11.1 Chapter XIII Table 6D: 1984 (Lubricating Oils).

### Compliance

- API MPMS 11.1 Volume X (API Standard 2540) - Table 6A - Generalized Crude Oils, Correction of Volume to 60°F against API Gravity at 60°F - First Edition, August 1980
- API MPMS 11.1 Volume X (API Standard 2540) - Table 6B - Generalized Products, Correction of Volume to 60°F against API Gravity at 60°F - First Edition, August 1980
- API MPMS 11.1 Volume XIII - Table 6D - Generalized Lubricating Oils, Correction of Volume to 60°F Against API Gravity at 60°F - January 1982

### Function inputs & outputs

| Function inputs      | Remark   | EU   | SW tag   | Range     | Default |
|----------------------|--|------|----------|-----------|---------|
| Name                 | Optional tag name, tag description and tag group   |      |          |           |         |
| API at 60 °F         | API gravity at 60°F and the equilibrium pressure   | °API |          | -20..120  | 0       |
| Observed temperature |  | °F   |          | -100..400 | 60      |
| Product              | 1: A - Crude Oil<br>2: B - Auto select<br>Selection based on °API at 60 °F<br>3: B - Gasoline<br>4: B - Transition Area<br>5: B - Jet Fuels<br>6: B - Fuel Oil<br>7: D - Lubricating Oil   |      | PRDTYP   | -         | 1       |
| API2540 rounding     | 0: Disabled<br>The calculations are performed with full precision and the final CTL value is rounded as specified by input 'CTL decimal places'<br>1: Enabled for computational value<br>API-2540 rounding and truncating rules are applied and the computational value for CTL as specified in the standard is used, meaning that the CTL value has:<br>4 decimal places if CTL >=1<br>5 decimal places if CTL < 1.<br>2: Enabled for table value<br>API-2540 rounding and truncating rules are applied and the table value for CTL as specified in the standard meaning that the CTL value has 4 decimal places in all cases<br>3: Enabled with 5 decimal places<br>API-2540 rounding and truncating rules are applied, while the CTL value has 5 decimal places in all cases.<br>Note: although not strictly in accordance with the standard, this option is more commonly used than option 'Enabled for computational value' |      | APIROUND | -         | 0       |

| Function outputs         | Remark  | EU   | SW tag | Alarm         | Fallback |
|--------------------------|---|------|--------|---------------|----------|
| Status                   | 0: Normal<br>1: Input argument out of range<br>2: Calculation error   | -    | STS    | FLOOR<br>CALC | 1        |
| CTL                      | Volume correction factor for temperature.<br>Value will be rounded according to input 'API2540 rounding'  | -    | CTL    |               | 1        |
| K0                       | Actual value of constant K0 used for CTL calculation  | -    | K0     |               | 0        |
| K1                       | Actual value of constant K1 used for CTL calculation  | -    | K1     |               | 0        |
| K2                       | Actual value of constant K2 used for CTL calculation  | -    | K2     |               | 0        |
| Alpha                    | Thermal expansion factor  | 1/°F | ALPHA  |               | 0        |
| Product                  | When input 'Product' is 'B - Auto select', then the output is set to the actual selected product of table 6B (enumerative value as defined for input 'Product'), else the output is set equal to input 'Product'. | -    | PRDCUR |               | 0        |
| Calculation out of range | With respect to the standard the input values are:<br>0: In Range<br>1: Out of Range  | -    |        |               | 0        |
|                          |   |      |        | OOR           |          |

### Calculations

The calculations are in full or partial compliance with the standard depending on input 'API 2540 rounding'.

## fxAPI\_Table6\_2004

### Description

°API (60°F, 0 psig) --> °API (T, P)

This function converts an API gravity value at 60°F and 0 psig to the API gravity value at the observed temperature and pressure. The temperature and pressure correction is according to API MPMS 11.1:2004.

Note: As opposed to API-2540 that the equilibrium pressure is below atmospheric pressure, so taking 0 psig as the base pressure.

### Compliance

- API MPMS 11.1 Temperature and Pressure Volume Correction Factors for Generalized Crude Oils, Refined Products and Lubricating Oils, May 2004

### Function inputs

| Function inputs      | Remark   | EU   | SW tag   | Range     | Default |
|----------------------|--|------|----------|-----------|---------|
| Name                 | Optional tag name, tag description and tag group   |      |          |           |         |
| API at 60 °F         | API gravity at 60°F and 0 psig   | °API |          | -20..120  | 0       |
| Observed temperature | Temperature at which the API gravity is observed   | °F   |          | -100..400 | 60      |
| Observed pressure    | Pressure at which the API gravity is observed  | psig |          | -10..2000 | 0       |
| Product              | 1: A - Crude Oil<br>2: B - Auto select<br>Selection based on °API at 60 °F<br>3: B - Gasoline<br>4: B - Transition Area<br>5: B - Jet Fuels<br>6: B - Fuel Oil<br>7: D - Lubricating Oil                                 |      | PRDTYP   |           | 1       |
| API rounding         | 0: Disabled<br>The calculations are performed with full precision<br>1: Enabled<br>The input and output values are rounded in compliance with the standard. The CTL, CPL and CTPL value are rounded to 5 decimal places. |      | APIROUND |           | 0       |

### Function outputs

| Function outputs         | Remark   | EU    | SW tag | Alarm         | Fallback |
|--------------------------|--|-------|--------|---------------|----------|
| Status                   | 0: Normal<br>1: Input argument out of range<br>2: Calculation error  | -     | STS    | FLOOR<br>CALC |          |
| Observed API             | API gravity at the observed temperature and pressure   | -     | API    |               | 0        |
| CTL                      | Volume correction factor for temperature.  | -     | CTL    |               | 1        |
| CPL                      | Volume correction factor for pressure  | -     | CPL    |               | 1        |
| CTPL                     | Combined volume correction factor<br>CTPL = CTL * CPL  | -     | CTPL   |               | 1        |
| K0                       | Actual value of constant K0 used for CTL calculation   | -     | K0     |               | 0        |
| K1                       | Actual value of constant K1 used for CTL calculation   | -     | K1     |               | 0        |
| K2                       | Actual value of constant K2 used for CTL calculation   | -     | K2     |               | 0        |
| Alpha                    | Thermal expansion factor   | 1/°F  | ALPHA  |               | 0        |
| F                        | Compressibility factor   | 1/psi | F      |               | 0        |
| Product                  | When input 'Product' is 'B - Auto select', then the output is set to the actual selected product of table B (enumerative value as defined for input 'Product'), else the output is set equal to input 'Product'. | -     | PRDCUR |               | 0        |
| Calculation out of range | With respect to the standard the input values are:<br>0: In Range<br>1: Out of Range   | -     |        |               | 0        |
|                          |  |       |        | OOR           |          |

### Calculations

The calculations are in either full or partial compliance with the standard, depending on whether API rounding is enabled or not.

## fxAPI\_Table23\_1952

### Description

#### Specific Gravity (T) --> Specific Gravity (60°F)

This function converts a specific gravity value at the observed temperature to the specific gravity at 60° according to the API 1952 Table 23.

### Compliance

- ASTM-IP Petroleum Measurement Tables, American Edition, United States Units of Measurement, 1952

### Function inputs

| Function inputs           | Remark   | EU | SW tag | Range     | Default |
|---------------------------|--|----|--------|-----------|---------|
| Name                      | Optional tag name, tag description and tag group |    |        |           |         |
| Observed specific gravity | Specific gravity at the observed temperature.    | -  |        | 0..1.3    | 0       |
| Observed temperature      |  | °F |        | -100..400 | 60      |

### Function outputs

| Function outputs         | Remark   | EU | SW tag | Alarm | Fallback |
|--------------------------|--|----|--------|-------|----------|
| Status                   | 0: Normal<br>1: Input argument out of range  | -  | STS    | FLOOR |          |
| Specific gravity 60 °F   | Specific gravity at 60°F   | -  | RD     |       | 0        |
| Calculation out of range | With respect to the standard the input values are:<br>0: In Range<br>1: Out of Range | -  |        | OOR   | 0        |

### Calculations

The table values are the standard, so no calculations are involved. The function performs an interpolation between the table values that correspond to the input specific gravity and input temperature.

In case the combination of input values ('Observed specific gravity' and 'Observed temperature') is not covered by the table, the output 'Specific gravity at 60 °F' is set to 0 and output 'Calculation out of range' is set to 1.

### Boundaries

Table 23 contains values for the following range:

| Input value               | Normal Range   | EU |
|---------------------------|----------------|----|
| Observed specific gravity | 0.420 .. 1.099 |    |
| Observed temperature      | 0 .. 150       | °F |

Note that the table does not cover the full range, e.g. for an Observed specific gravity of 0.420 the table only specifies values between 120 .. 140 °F

## fxAPI\_Table23\_1980

### Description

#### Relative Density (T) --> Relative Density (60°F)

This function converts a relative density value at the observed temperature to the relative density at 60°.

The temperature conversion is according to API-2540, Tables 23A (Generalized Crude Oils) and 23B (Refined Oil Products).

In 1982 API published tables 5D, 6D, 53D and 54D for lubricating oil products as part of API MPMS 11.1. Although tables 23d and 24d are not covered in an official API standard the Flow-X series of flow computer supports tables 23D and 24D as well by combining the calculation of tables 23A/B and 24A/B with the K0 and K1 constants published in the other tables for lubricating oils.

### Function inputs

| Function inputs           | Remark  | EU | SW tag   | Range     | Default |
|---------------------------|---|----|----------|-----------|---------|
| Name                      | Optional tag name, tag description and tag group  |    |          |           |         |
| Observed relative density | Relative density at observed temperature and pressure   | -  |          | 0..1.3    | 0       |
| Observed temperature      |   | °F |          | -100..400 | 60      |
| Product                   | 1: A - Crude Oil<br>2: B - Auto select<br>Selection based on relative density at 60 °F<br>3: B - Gasoline<br>4: B - Transition Area<br>5: B - Jet Fuels<br>6: B - Fuel Oil<br>7: D - Lubricating Oil  |    | PRDTYP   |           | 1       |
| API2540 rounding          | 0: Disabled<br>The calculations are performed with full precision.<br>A convergence limit of 0.000001 kg/m3 will be applied for the iterative calculations.<br>1: Enabled<br>API-2540 rounding and truncating rules are applied.<br>A convergence limit of 0.05 kg/m3 will be applied as defined in the standard. |    | APIROUND |           | 0       |
| Hydrometer correction     | 0: Disabled<br>1: Enabled   |    | HYDROCOR |           | 0       |

### Function outputs

| Function outputs         | Remark   | EU   | SW tag | Alarm                   | Fallback |
|--------------------------|--|------|--------|-------------------------|----------|
| Status                   | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence   | -    | STS    | FIOOR<br>CALC<br>NOCONV |          |
| Relative density 60 °F   | Relative density at 60°F and the equilibrium pressure  | -    | RD     |                         | 0        |
| CTL                      | Volume correction factor for temperature.  | -    | CTL    |                         | 1        |
| K0                       | Actual value of constant K0 used for CTL calculation   | -    | K0     |                         | 0        |
| K1                       | Actual value of constant K1 used for CTL calculation   | -    | K1     |                         | 0        |
| K2                       | Actual value of constant K2 used for CTL calculation   | -    | K2     |                         | 0        |
| Alpha                    | Thermal expansion factor   | 1/°F | ALPHA  |                         | 0        |
| Product                  | When input 'Product' is 'B - Auto select', then the output is set to the actual selected product of table 23B (enumerative value as defined for input 'Product'), else the output is set equal to input 'Product'. | -    | PRDCUR |                         | 0        |
| Calculation out of range | With respect to the standard the input values are:<br>0: In Range<br>1: Out of Range   | -    |        | OOR                     | 0        |

### Calculations

The calculations are in full or partial compliance with the standard depending on input 'API 2540 rounding'.

An iterative calculation needs to be applied to convert the observed relative density to the value at base conditions. The function provides the option to correct for readings taken from a hydrometer as specified in the API-2540 standard.

### Compliance

- API MPMS 11.1 Volume X (API Standard 2540) - Table 23A - Generalized Crude Oils, Correction of Observed Relative Density to Relative Density at 60/60°F - First Edition, August 1980
- API MPMS 11.1 Volume X (API Standard 2540) - Table 23B - Generalized Products, Correction of Observed Relative Density to Relative Density at 60/60°F - First Edition, August 1980



## fxAPI\_Table23\_2004

### Description

#### Relative Density (T, P) --> Relative Density (60°F, 0 psig)

This function converts a relative density value at the observed temperature and pressure to the relative density value at 60°F and 0 psig.

The temperature and pressure correction is according to API MPMS 11.1:2004.

An iterative calculation needs to be applied to convert the observed relative density to the value at base conditions.

### Function inputs

| Function inputs           | Remark   | EU   | SW tag   | Range     | Default |
|---------------------------|--|------|----------|-----------|---------|
| Name                      | Optional tag name, tag description and tag group   |      |          |           |         |
| Observed Relative density | Relative density at the observed temperature and pressure  | -    |          | 0 ..1.3   | 0       |
| Observed temperature      | Temperature at which the relative density is observed °F   |      |          | -100..400 | 60      |
| Observed pressure         | Pressure at which the relative density is observed   | psig |          | -10..2000 | 0       |
| Product                   | 1: A - Crude Oil<br>2: B - Auto select<br>Selection based on relative density at 60 °F<br>3: B - Gasoline<br>4: B - Transition Area<br>5: B - Jet Fuels<br>6: B - Fuel Oil<br>7: D - Lubricating Oil   |      | PRDTYP   |           | 1       |
| API rounding              | 0: Disabled<br>The calculations are performed with full precision and the final CTL, CPL and CTPL values are rounded as specified by the inputs 'CTL / CPL / CTPL decimal places'<br>1: Enabled<br>The input and output values are rounded in compliance with the standard. The CTL, CPL and CTPL value are rounded to 5 decimal places. |      | APIROUND |           | 0       |

### Function outputs

| Function outputs          | Remark   | EU    | SW tag | Alarm | Fallback |
|---------------------------|--|-------|--------|-------|----------|
| Status                    | 0: Normal<br>1: Input argument out of range<br>Outputs will be set to fallback values<br>2: Calculation error<br>Outputs will be set to fallback values<br>3: No convergence within 15 iterations<br>Outputs will be set to values of last iteration | -     |        |       | 1        |
| Relative density at 60 °F | Relative density at 60°F and 0 psig  | -     | RD     |       | 0        |
| CTL                       | Volume correction factor for temperature.<br>Value will be rounded according to input 'API rounding'   | -     | CTL    |       | 1        |
| CPL                       | Volume correction factor for pressure<br>Value will be rounded according to input 'API rounding'   | -     | CPL    |       | 1        |
| CTPL                      | Combined volume correction factor<br>CTPL = CTL * CPL  | -     | CTPL   |       | 1        |
| K0                        | Actual value of constant K0 used for CTL calculation   | -     | K0     |       | 0        |
| K1                        | Actual value of constant K1 used for CTL calculation   | -     | K1     |       | 0        |
| K2                        | Actual value of constant K2 used for CTL calculation   | -     | K2     |       | 0        |
| Alpha                     | Thermal expansion factor   | 1/°F  | ALPHA  |       | 0        |
| F                         | Compressibility factor   | 1/psi | F      |       | 0        |
| Product                   | When input 'Product' is 'B - Auto select', then the output is set to the actual selected product of table B (enumerative value as defined for input 'Product'), else the output is set equal to input 'Product'.                                     | -     | PRDCUR |       | 0        |
| Calculation out of range  | With respect to the standard the input values are:   | -     |        | OOR   | 0        |

Note: As opposed to API-2540, the 2004 standard does not include a correction for readings taken from a hydrometer and assumes that the equilibrium pressure is below atmospheric pressure, so taking 0 psig as the base pressure.

### Compliance

- API MPMS 11.1 Temperature and Pressure Volume Correction Factors for Generalized Crude Oils, Refined Products and Lubricating Oils, May 2004

| Function outputs | Remark          | EU | SW tag | Alarm | Fallback |
|------------------|-----------------|----|--------|-------|----------|
|                  | 0: In Range     |    |        |       |          |
|                  | 1: Out of Range |    |        |       |          |

Calculations

The calculations are in either full or partial compliance with the standard, depending on whether API rounding is enabled or not.

## fxAPI\_Table23E

### Description

#### Relative Density (T) --> Relative Density (60°F)

This function converts the relative density value at the observed temperature to the corresponding relative density at 60°F. The temperature correction is according to API MPMS 11.2.4:2007 (GPA TP-25 / GPA TP-27).

### Compliance

- API MPMS 11.2.4: Temperature Correction for the Volume of NGL and LPG Tables 23E, 24E, 53E, 54E, 59E & 60E, September 2007
- GPA TP-27: Temperature Correction for the Volume of NGL and LPG Tables 23E, 24E, 53E, 54E, 59E & 60E, September 2007
- GPA TP-25: Temperature Correction for the volume of Light Hydrocarbons – Tables 24E and 23E, 1998

### Function inputs

| Function inputs           | Remark  | EU | SW tag   | Range     | Default |
|---------------------------|---|----|----------|-----------|---------|
| Name                      | Optional tag name, tag description and tag group  |    |          |           |         |
| Observed relative density | Relative density at the observed temperature  | -  |          | 0..0.75   | 0       |
| Observed temperature      | Temperature at which the relative density is observed   | °F |          | -100..300 | 60      |
| API rounding              | 0: Disabled<br>The calculations are performed with full precision and the output values are not rounded<br>1: Enabled<br>The input and output values are rounded as defined in the standard |    | APIROUND |           | 0       |

### Function outputs

| Function outputs          | Remark   | EU | SW tag | Alarm                      | Fallback |
|---------------------------|--|----|--------|----------------------------|----------|
| Status                    | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence | -  | STS    | FLOOR<br>CALCERR<br>NOCONV | 1        |
| Relative density at 60 °F | Relative density at 60°F   |    | RD     |                            | 0        |
| CTL                       | Volume correction factor for temperature.  | -  | CTL    |                            | 1        |
| Calculation out of range  | With respect to the standard the input values are:<br>0: In Range<br>1: Out of Range     | -  |        | OOR                        | 0        |

### Calculations

The calculations are in either full or partial compliance with the standard, depending on the selected type of API rounding.

## fxAPI\_Table24\_1952

### Description

#### Specific Gravity (60°F) --> CTL

This function returns the volume correction factor for temperature Ctl from the observed temperature and the specific gravity at 60° according to the API 1952 Table 24.

### Compliance

- ASTM-IP Petroleum Measurement Tables, American Edition, United States Units of Measurement, 1952

### Function inputs

| Function inputs        | Remark   | EU | SW tag | Range     | Default |
|------------------------|--|----|--------|-----------|---------|
| Name                   | Optional tag name, tag description and tag group |    |        |           |         |
| Specific gravity 60 °F | Specific gravity at 60°F                         | -  |        | 0..1.3    | 0       |
| Observed temperature   |  | °F |        | -100..400 | 60      |

### Function outputs

| Function outputs         | Remark   | EU | SW tag | Alarm | Fallback |
|--------------------------|--|----|--------|-------|----------|
| Status                   | 0: Normal<br>1: Input argument out of range  | -  | STS    | FIOOR |          |
| CTL                      | Volume correction factor for temperature.  | -  | CTL    |       | 1        |
| Calculation out of range | With respect to the standard the input values are:<br>0: In Range<br>1: Out of Range | -  |        | OOR   | 0        |

### Calculations

The table values are the standard, so no calculations are involved. The function performs an interpolation between the table values that correspond to the input specific gravity and input temperature.

In case the combination of input values ('Specific gravity 60 °F' and Observed temperature') is not covered by the table, the output 'CTL' is set to 1 and output 'Calculation out of range' is set to 1.

### Boundaries

Table 23 contains values for the following range:

| Input value               | Normal Range   | EU |
|---------------------------|----------------|----|
| Observed specific gravity | 0.500 .. 1.100 |    |
| Observed temperature      | -50 .. +300    | °F |

Note that the table does not cover the full range, e.g. for an Specific gravity at 60 °F of 0.500 the table only specifies values between -50 .. 95 °F

## fxAPI\_Table24\_1980

### Description

#### Relative Density (60°F) --> CTL

This function calculates the volume correction factor for temperature CTL from the relative density value at 60°F and the observed temperature.

The temperature conversion is according to API-2540, Tables 24A (Generalized Crude Oils) and 24B (Refined Oil Products). In 1982 API published tables 5D, 6D, 53D and 54D for lubricating oil products as part of API MPMS 11.1. Although tables 23d and 24d are not covered in an official API standard the Flow-X series of flow computer supports tables 23D and 24D as well by combining the calculation of tables 23A/B and 24A/B with the K0 and K1 constants published in the other tables for lubricating oils.

### Function inputs

| Function inputs           | Remark  | EU | SW tag   | Range     | Default |
|---------------------------|---|----|----------|-----------|---------|
| Name                      | Optional tag name, tag description and tag group  |    |          |           |         |
| Relative Density at 60 °F | Relative density at 60°F and the equilibrium pressure   | -  |          | 0..1.3    | 0       |
| Observed temperature      |   | °F |          | -100..400 | 60      |
| Product                   | 1: A - Crude Oil<br>2: B - Auto select<br>Selection based on relative density at 60 °F<br>3: B - Gasoline<br>4: B - Transition Area<br>5: B - Jet Fuels<br>6: B - Fuel Oil<br>7: D - Lubricating Oil  |    | PRDTYP   | -         | 1       |
| API2540 rounding          | 0: Disabled<br>The calculations are performed with full precision and the final CTL value is rounded as specified by input 'CTL decimal places'<br>1: Enabled for computational value<br>API-2540 rounding and truncating rules are applied and the computational value for CTL as specified in the standard is used, meaning that the CTL value has:<br>4 decimal places if CTL >=1<br>5 decimal places if CTL < 1.<br>2: Enabled for table value<br>API-2540 rounding and truncating rules are applied and the <b>table</b> value for CTL as specified in the standard meaning that the CTL value has 4 decimal places in all cases<br>3: Enabled with 5 decimal places<br>API-2540 rounding and truncating rules are applied, while the CTL value has 5 decimal places in all cases.<br>Note: although not strictly in accordance with the standard, this option is more commonly used than option 'Enabled for computational value' |    | APIROUND | -         | 0       |

### Function outputs

| Function outputs         | Remark   | EU   | SW tag | Alarm            | Fallback      |
|--------------------------|--|------|--------|------------------|---------------|
| Status                   | 0: Normal<br>1: Input argument out of range<br>2: Calculation error  | -    | STS    | FIOOR<br>CALCERR |               |
| CTL                      | Volume correction factor for temperature.<br>Value will be rounded according to input 'API2540 rounding'   | -    | CTL    |                  | 1             |
| K0                       | Actual value of constant K0 used for CTL calculation   | -    | K0     |                  | 0             |
| K1                       | Actual value of constant K1 used for CTL calculation   | -    | K1     |                  | 0             |
| K2                       | Actual value of constant K2 used for CTL calculation   | -    | K2     |                  | 0             |
| Alpha                    | Thermal expansion factor   | 1/°F | ALPHA  |                  | 0             |
| Product                  | When input 'Product' is 'B - Auto select', then the output is set to the actual selected product of table 24B (enumerative value as defined for input 'Product'), else the output is set equal to input 'Product'. | -    | PRDCUR |                  | Input Product |
| Calculation out of range | With respect to the standard the input values are:<br>0: In Range<br>1: Out of Range   | -    |        | OOR              | 0             |

### Compliance

- API MPMS 11.1 Volume X (API Standard 2540) - Table 24A - Generalized Crude Oils, Correction of Volume to 60°F against Relative Density at 60/60°F - First Edition, August 1980
- API MPMS 11.1 Volume X (API Standard 2540) - Table 24B - Generalized Products, Correction of Volume to 60°F against Relative Density at 60/60°F - First Edition, August 1980

**Calculations**

The calculations are in full or partial compliance with the standard depending on input 'API 2540 rounding'.

## fxAPI\_Table24\_2004

### Description

#### Relative Density (60°F, 0 psig) --> Relative Density (T, P)

This function converts a relative density value at 60°F and 0 psig to the relative density value at the observed temperature and pressure.

The temperature and pressure correction is according to API MPMS 11.1:2004.

Note: The 2004 standard assumes that the equilibrium pressure is below atmospheric pressure, so taking 0 psig as the base pressure.

### Compliance

- API MPMS 11.1 Temperature and Pressure Volume Correction Factors for Generalized Crude Oils, Refined Products and Lubricating Oils, May 2004

### Function inputs

| Function inputs           | Remark  | EU   | SW tag   | Range     | Default |
|---------------------------|---|------|----------|-----------|---------|
| Name                      | Optional tag name, tag description and tag group  |      |          |           |         |
| Relative density at 60 °F | Relative density at 60°F and 0 psig   | -    |          | 0 ..1.3   | 0       |
| Observed temperature      | Temperature at which the API gravity is observed  | °F   |          | -100..400 | 60      |
| Observed pressure         | Pressure at which the API gravity is observed   | psig |          | -10..2000 | 0       |
| Product                   | 1: A - Crude Oil<br>2: B - Auto select<br>Selection based on relative density at 60 °F<br>3: B - Gasoline<br>4: B - Transition Area<br>5: B - Jet Fuels<br>6: B - Fuel Oil<br>7: D - Lubricating Oil  |      | PRDTYP   |           | 1       |
| API rounding              | 0: Disabled<br>The calculations are performed with full precision and the final CTL, CPL and CTPL values are rounded as specified by the inputs 'CTL / CPL/ CTPL decimal places'<br>1: Enabled<br>The input and output values are rounded in compliance with the standard. The CTL, CPL and CTPL value are rounded to 5 decimal places. |      | APIROUND |           | 0       |

### Function outputs

| Function outputs          | Remark   | EU    | SW tag | Alarm            | Fallback |
|---------------------------|--|-------|--------|------------------|----------|
| Status                    | 0: Normal<br>1: Input argument out of range<br>2: Calculation error  | -     | STS    | FIOOR<br>CALCERR |          |
| Observed relative density | Relative density at the observed temperature and pressure  | -     | RD     |                  | 0        |
| CTL                       | Volume correction factor for temperature.<br>Value will be rounded according to input 'API rounding'   | -     | CTL    |                  | 1        |
| CPL                       | Volume correction factor for pressure<br>Value will be rounded according to input 'API rounding'   | -     | CPL    |                  | 1        |
| CTPL                      | Combined volume correction factor<br>CTPL = CTL * CPL  | -     | CTPL   |                  | 1        |
| K0                        | Actual value of constant K0 used for CTL calculation   | -     | K0     |                  | 0        |
| K1                        | Actual value of constant K1 used for CTL calculation   | -     | K1     |                  | 0        |
| K2                        | Actual value of constant K2 used for CTL calculation   | -     | K2     |                  | 0        |
| Alpha                     | Thermal expansion factor   | 1/°F  | ALPHA  |                  | 0        |
| F                         | Compressibility factor   | 1/psi | F      |                  | 0        |
| Product                   | When input 'Product' is 'B - Auto select', then the output is set to the actual selected product of table B (enumerative value as defined for input 'Product'), else the output is set equal to input 'Product'. | -     | PRDCUR |                  | 0        |
| Calculation out of range  | With respect to the standard the input values are:<br>0: In Range<br>1: Out of Range   | -     |        | OOR              | 0        |

### Calculations

The calculations are in either full or partial compliance with the standard, depending on whether API rounding is enabled or not.

## fxAPI\_Table24E

### Description

#### Relative Density (60°F) --> CTL

This function calculates the volume correction factor for temperature from the relative density value at 60°F and the observed temperature.

The temperature correction is according to API MPMS 11.2.4:2007 (GPA TP-25 / GPA TP-27).

### Compliance

- API MPMS 11.2.4: Temperature Correction for the Volume of NGL and LPG Tables 23E, 24E, 53E, 54E, 59E & 60E, September 2007
- GPA TP-27: Temperature Correction for the Volume of NGL and LPG Tables 23E, 24E, 53E, 54E, 59E & 60E, September 2007
- GPA TP-25: Temperature Correction for the volume of Light Hydrocarbons – Tables 24E and 23E, 1998

### Function inputs

| Function inputs           | Remark  | EU | SW tag   | Range     | Default |
|---------------------------|---|----|----------|-----------|---------|
| Name                      | Optional tag name, tag description and tag group  |    |          |           |         |
| Relative density at 60 °F | Relative density at 60°F  | -  |          | 0..0.75   | 0       |
| Observed temperature      | Temperature at which the relative density is observed   | °F |          | -100..300 | 60      |
| API rounding              | 0: Disabled<br>The calculations are performed with full precision and the output values are not rounded<br>1: Enabled<br>The input and output values are rounded as defined in the standard |    | APIROUND |           | 0       |

### Function outputs

| Function outputs         | Remark   | EU | SW tag | Alarm         | Fallback |
|--------------------------|--|----|--------|---------------|----------|
| Status                   | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence             | -  | STS    | FIOOR<br>CALC |          |
| CTL                      | Volume correction factor for temperature<br>Value will be rounded according to inputs 'API rounding' | -  | CTL    |               | 1        |
| Calculation out of range | With respect to the standard the input values are:<br>0: In Range<br>1: Out of Range                 | -  |        | OOR           | 0        |

### Calculations

The calculations are in either full or partial compliance with the standard, depending on the selected type of API rounding.



## fxAPI\_Table53\_1952

### Description

#### Density (T) --> Density (15°C)

This function converts a density value at the observed temperature to the density at 15°C according to the API 1952 Table 53.

### Compliance

- ASTM-IP Petroleum Measurement Tables, Metric Edition, Metric Units of Measurement, 1952

### Function inputs

| Function inputs      | Remark   | EU    | SW tag | Range     | Default |
|----------------------|--|-------|--------|-----------|---------|
| Name                 | Optional tag name, tag description and tag group |       |        |           |         |
| Observed density     | Density at the observed temperature.             | kg/m3 |        | 0..1300   | 0       |
| Observed temperature |  | °C    |        | -100..200 | 15      |

### Function outputs

| Function outputs         | Remark   | EU    | SW tag | Alarm | Fallback |
|--------------------------|--|-------|--------|-------|----------|
| Status                   | 0: Normal  | -     | STS    |       |          |
|                          | 1: Input argument out of range   |       |        | FLOOR |          |
| Density at 15 °C         | Density at 15 °C   | kg/m3 | DENS15 |       | 0        |
| Calculation out of range | With respect to the standard the input values are:<br>0: In Range<br>1: Out of Range | -     |        | OOR   | 0        |

### Calculations

The table values are the standard, so no calculations are involved. The function performs an interpolation between the table values that correspond to the input specific gravity and input temperature.

In case the combination of input values ('Observed density' and 'Observed temperature') is not covered by the table, the output 'Density at 15 °C' is set to 0 and output 'Calculation out of range' is set to 1.

### Boundaries

Table 53 contains values for the following range:

| Input value          | Normal Range | EU    |
|----------------------|--------------|-------|
| Observed density     | 420 .. 1099  | kg/m3 |
| Observed temperature | -25 .. 125   | °C    |

Note that the table does not cover the full range, e.g. for an Observed specific gravity of 0.420 the table only specifies values between 45 .. 60 °C

## fxAPI\_Table53\_1980

### Description

#### Density (T) --> Density (15°C)

This function converts a density value at the observed temperature to the density value at 15°C.

The temperature conversion is according to API-2540, Tables 53A (Generalized Crude Oils) and 53B (Refined Oil Products) and API MPMS 11.1 Chapter XIV Table 53D: 1984 (Lubricating Oils).

The function provides the option to correct for readings taken from a hydrometer as specified in the API-2540 standard.

### Function inputs

| Function inputs       | Remark  | EU    | SW tag   | Range     | Default |
|-----------------------|---|-------|----------|-----------|---------|
| Name                  | Optional tag name, tag description and tag group  |       |          |           |         |
| Observed density      | Density at observed temperature   | kg/m3 |          | 0..1300   | 0       |
| Observed temperature  |   | °C    |          | -100..200 | 15      |
| Product               | 1: A - Crude Oil<br>2: B - Auto select<br>Selection based on density at 15 °C<br>3: B - Gasoline<br>4: B - Transition Area<br>5: B - Jet Fuels<br>6: B - Fuel Oil<br>7: D - Lubricating Oil   |       | PRDTYP   |           | 1       |
| API2540 rounding      | 0: Disabled<br>The calculations are performed with full precision.<br>A convergence limit of 0.000001 kg/m3 will be applied for the iterative calculations.<br>1: Enabled<br>API-2540 rounding and truncating rules are applied.<br>A convergence limit of 0.05 kg/m3 will be applied as defined in the standard. |       | APIROUND |           | 0       |
| Hydrometer correction | 0: Disabled<br>1: Enabled   |       | HYDROCOR |           | 0       |

### Function outputs

| Function outputs         | Remark   | EU        | SW tag | Alarm                      | Fallback |
|--------------------------|--|-----------|--------|----------------------------|----------|
| Status                   | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence   | -         | STS    | FIOOR<br>CALCERR<br>NOCONV |          |
| Density at 15 °C         | Density at 15°C  | kg/m3 (s) | DENS15 |                            | 0        |
| CTL                      | Volume correction factor for temperature.  | -         | CTL    |                            | 1        |
| K0                       | Actual value of constant K0 used for CTL calculation   | -         | K0     |                            | 0        |
| K1                       | Actual value of constant K1 used for CTL calculation   | -         | K1     |                            | 0        |
| K2                       | Actual value of constant K2 used for CTL calculation   | -         | K2     |                            | 0        |
| Alpha                    | Thermal expansion factor   | 1/°C      | ALPHA  |                            | 0        |
| Product                  | When input 'Product' is 'B - Auto select', then the output is set to the actual selected product of table 53B (enumerative value as defined for input 'Product'), else the output is set equal to input 'Product'. | -         | PRDCUR |                            | 0        |
| Calculation out of range | With respect to the standard the input values are:<br>0: In Range<br>1: Out of Range   | -         |        | OOR                        | 0        |

### Calculations

The calculations are in full or partial compliance with the standard depending on input 'API 2540 rounding'.

### Compliance

- API MPMS 11.1 Volume X (API Standard 2540) - Table 53A - Generalized Crude Oils, Correction of Observed Density to Density at 15°C - First Edition, August 1980
- API MPMS 11.1 Volume X (API Standard 2540) - Table 53B - Generalized Products, Correction of Observed Density to Density at 15°C - First Edition, August 1980
- API MPMS 11.1 Volume XIV - Table 53D - Generalized Lubricating Oils, Correction of Observed Density to Density at 15°C - January 1982

## fxAPI\_Table53\_2004

### Description

#### Density (T, P) --> Density (15°C, 0 bar(g))

This function converts a density value at the observed temperature and pressure to the density value at 15°C and 0 bar(g).

The temperature and pressure correction is according to API MPMS 11.1:2004.

An iterative calculation needs to be applied to convert the observed density to the value at base conditions.

#### Function inputs and outputs

| Function inputs      | Remark   | EU     | SW tag   | Range     | Default |
|----------------------|--|--------|----------|-----------|---------|
| Name                 | Optional tag name, tag description and tag group   |        |          |           |         |
| Observed density     | Density at the observed temperature and pressure   | kg/m3  |          | 0..1300   | 0       |
| Observed temperature | Temperature at which the density is observed   | °C     |          | -100..200 | 15      |
| Observed pressure    | Pressure at which the density is observed  | bar(g) |          | -1..250   | 0       |
| Product              | 1: A - Crude Oil<br>2: B - Auto select<br>Selection based on density at 15 °C<br>3: B - Gasoline<br>4: B - Transition Area<br>5: B - Jet Fuels<br>6: B - Fuel Oil<br>7: D - Lubricating Oil  |        | PRDTYP   |           | 1       |
| API rounding         | 0: Disabled<br>The calculations are performed with full precision and the final CTL, CPL and CTPL values are rounded as specified by the inputs 'CTL / CPL / CTPL decimal places'<br>1: Enabled<br>The input and output values are rounded in compliance with the standard. The CTL, CPL and CTPL value are rounded to 5 decimal places. |        | APIROUND |           | 0       |

| Function outputs         | Remark   | EU    | SW tag | Alarm                      | Fallback |
|--------------------------|--|-------|--------|----------------------------|----------|
| Status                   | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence   | -     | STS    | FIOOR<br>CALCERR<br>NOCONV |          |
| Density at 15 °C         | Density at 15°C and 0 bar(g)   | -     | DENS15 |                            | 0        |
| CTL                      | Volume correction factor for temperature.<br>Value will be rounded according to input 'API rounding'   | -     | CTL    |                            | 1        |
| CPL                      | Volume correction factor for pressure<br>Value will be rounded according to input 'API rounding'   | -     | CPL    |                            | 1        |
| CTPL                     | Combined volume correction factor<br>CTPL = CTL * CPL  | -     | CTPL   |                            | 1        |
| K0                       | Actual value of constant K0 used for CTL calculation   | -     | K0     |                            | 0        |
| K1                       | Actual value of constant K1 used for CTL calculation   | -     | K1     |                            | 0        |
| K2                       | Actual value of constant K2 used for CTL calculation   | -     | K2     |                            | 0        |
| Alpha                    | Thermal expansion factor at 60 °F !  | 1/°C  | ALPHA  |                            | 0        |
| F                        | Compressibility factor   | 1/bar | F      |                            | 0        |
| Product                  | When input 'Product' is 'B - Auto select', then the output is set to the actual selected product of table B (enumerative value as defined for input 'Product'), else the output is set equal to input 'Product'. | -     | PRDCUR |                            | 0        |
| Calculation out of range | With respect to the standard the input values are:<br>0: In Range<br>1: Out of Range   | -     |        | OOR                        | 0        |

#### Calculations

The calculations are in either full or partial compliance with the standard, depending on whether API rounding is enabled or not.

Note: As opposed to API-2540, the 2004 standard does not include a correction for readings taken from a hydrometer and assumes that the equilibrium pressure is below atmospheric pressure, so taking 0 psig as the base pressure.

#### Compliance

- API MPMS 11.1 Temperature and Pressure Volume Correction Factors for Generalized Crude Oils, Refined Products and Lubricating Oils, May 2004

## fxAPI\_Table53E

### Description

#### Density (T) --> Density (15°C)

This function converts the density value at the observed temperature to the corresponding density at 15°C.  
The temperature correction is according to API MPMS 11.2.4:2007 (GPA TP-27).

### Function inputs

| Function inputs      | Remark  | EU    | SW tag | Range     | Default |
|----------------------|---|-------|--------|-----------|---------|
| Name                 | Optional tag name, tag description and tag group  |       |        |           |         |
| Observed density     | Density at the observed temperature   | kg/m3 |        | 0..750    | 0       |
| Observed temperature | Temperature at which the relative density is observed   | °C    |        | -100..150 | 15      |
| API rounding         | 0: Disabled<br>The calculations are performed with full precision and the output values are not rounded<br>1: Enabled<br>The input and output values are rounded as defined in the standard |       |        |           | 0       |

### Compliance

- API MPMS 11.2.4: Temperature Correction for the Volume of NGL and LPG Tables 23E, 24E, 53E, 54E, 59E & 60E, September 2007
- GPA TP-27: Temperature Correction for the Volume of NGL and LPG Tables 23E, 24E, 53E, 54E, 59E & 60E, September 2007

### Function outputs

| Function outputs         | Remark   | EU | SW tag | Alarm                      | Fallback |
|--------------------------|--|----|--------|----------------------------|----------|
| Status                   | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence | -  | STS    | FIOOR<br>CALCERR<br>NOCONV |          |
| Density at 15°C          |  |    | DENS15 |                            |          |
| CTL                      | Volume correction factor for temperature.  | -  | CTL    |                            | 1        |
| Calculation out of range | With respect to the standard the input values are:<br>0: In Range<br>1: Out of Range     | -  |        | OOR                        | 0        |

### Calculations

The calculations are in either full or partial compliance with the standard, depending on the selected type of API rounding.

## fxAPI\_Table54\_1952

### Description

#### Density (15°C) --> CTL

This function determines the volume correction factor for temperature CTL from the relative density value at 15°C and the observed temperature according to the API 1952 Table 54.

### Compliance

- ASTM-IP Petroleum Measurement Tables, Metric Edition, Metric Units of Measurement, 1952

### Function inputs

| Function inputs      | Remark   | EU    | SW tag | Range     | Default |
|----------------------|--|-------|--------|-----------|---------|
| Name                 | Optional tag name, tag description and tag group |       |        |           |         |
| Density 15 °C        | Specific gravity at 60°F                         | Kg/m3 |        | 0..1300   | 0       |
| Observed temperature |  | °C    |        | -100..200 | 15      |

### Function outputs

| Function outputs         | Remark   | EU | SW tag | Alarm | Fallback |
|--------------------------|--|----|--------|-------|----------|
| Status                   | 0: Normal<br>1: Input argument out of range  | -  | STS    | FIOOR |          |
| CTL                      | Volume correction factor for temperature.  | -  | CTL    |       | 1        |
| Calculation out of range | With respect to the standard the input values are:<br>0: In Range<br>1: Out of Range | -  |        | OOR   | 0        |

### Calculations

The table values are the standard, so no calculations are involved. The function performs an interpolation between the table values that correspond to the input specific gravity and input temperature.

In case the combination of input values ('Specific gravity 60 °F' and Observed temperature') is not covered by the table, the output 'CTL' is set to 1 and output 'Calculation out of range' is set to 1.

### Boundaries

Table 54 contains values for the following range:

| Input value          | Normal Range | EU    |
|----------------------|--------------|-------|
| Density at 15 °C     | 500 .. 1100  | kg/m3 |
| Observed temperature | -50 .. +150  | °C    |

Note that the table does not cover the full range, e.g. for a Density at 15 °C of 500 kg/m3 the table only specifies values between -50 .. 55 °C

## fxAPI\_Table54\_1980

### Description

#### Density (15°C) --> CTL

This function calculates the volume correction factor for temperature CTL from the relative density value at 15°C and the observed temperature.

The temperature conversion is according to API-2540, Tables 54A (Generalized Crude Oils) and 54B (Refined Oil Products) and API MPMS 11.1 Chapter XIV Table 54D: 1984 (Lubricating Oils).

### Compliance

- API MPMS 11.1 Volume X (API Standard 2540) - Table 54A - Generalized Crude Oils, Correction of Volume to 15°C against Density at 15°F - First Edition, August 1980
- API MPMS 11.1 Volume X (API Standard 2540) - Table 54B - Generalized Products, Correction of Volume to 15°C against Density at 15°C - First Edition, August 1980
- API MPMS 11.1 Volume XIV - Table 54D - Generalized Lubricating Oils, Correction of Volume to 15°C Against Density at 15°C - January 1982

### Function inputs

| Function inputs      | Remark   | EU    | SW tag   | Range     | Default |
|----------------------|--|-------|----------|-----------|---------|
| Name                 | Optional tag name, tag description and tag group   |       |          |           |         |
| Density at 15 °C     | Density at 15°C and the equilibrium pressure   | kg/m3 |          | 0..1300   | 0       |
| Observed temperature |  | °C    |          | -100..200 | 15      |
| Product              | 1: A - Crude Oil<br>2: B - Auto select<br>3: B - Gasoline<br>4: B - Transition Area<br>5: B - Jet Fuels<br>6: B - Fuel Oil<br>7: D - Lubricating Oil   |       | PRDTYP   | -         | 1       |
| API2540 rounding     | 0: Disabled<br>The calculations are performed with full precision and the final CTL value is rounded as specified by input 'CTL decimal places'<br>1: Enabled for computational value<br>API-2540 rounding and truncating rules are applied and the <b>computational</b> value for CTL as specified in the standard is used, meaning that the CTL value has:<br>4 decimal places if CTL >=1<br>5 decimal places if CTL < 1.<br>2: Enabled for table value<br>API-2540 rounding and truncating rules are applied and the <b>table</b> value for CTL as specified in the standard meaning that the CTL value has 4 decimal places in all cases<br>3: Enabled with 5 decimal places<br>API-2540 rounding and truncating rules are applied, while the CTL value has 5 decimal places in all cases.<br>Note: although not strictly in accordance with the standard, this option is more commonly used than option 'Enabled for computational value' |       | APIROUND | -         | 0       |

### Function outputs

| Function outputs         | Remark   | EU   | SW tag | Alarm            | Fallback |
|--------------------------|--|------|--------|------------------|----------|
| Status                   | 0: Normal<br>1: Input argument out of range<br>2: Calculation error  |      | STS    | FLOOR<br>CALCERR |          |
| CTL                      | Volume correction factor for temperature.<br>Value will be rounded according to input 'API2540 rounding'   | -    | CTL    |                  | 1        |
| K0                       | Actual value of constant K0 used for CTL calculation   | -    | K0     |                  | 0        |
| K1                       | Actual value of constant K1 used for CTL calculation   | -    | K1     |                  | 0        |
| K2                       | Actual value of constant K2 used for CTL calculation   | -    | K2     |                  | 0        |
| Alpha                    | Thermal expansion factor   | 1/°C | ALPHA  |                  |          |
| Product                  | When input 'Product' is 'B - Auto select', then the output is set to the actual selected product of table 54B (enumerative value as defined for input 'Product'), else the output is set equal to input 'Product'. | -    | PRDCUR |                  |          |
| Calculation out of range | With respect to the standard the input values are:<br>0: In Range<br>1: Out of Range   | -    |        | OOR              |          |

### Calculations

The calculations are in full or partial compliance with the standard depending on input 'API 2540 rounding'.

## fxAPI\_Table54\_2004

### Description

**Density (15°C, 0 bar(g)) --> Density (T, P)**

This function converts a density value at 15°C and 0 bar(g) to the density value at the observed temperature and pressure.

The temperature and pressure correction is according to API MPMS 11.1:2004.

Note: The 2004 standard assumes that the equilibrium pressure is below atmospheric pressure, so taking 0 psig as the base pressure.

### Compliance

- API MPMS 11.1 Temperature and Pressure Volume Correction Factors for Generalized Crude Oils, Refined Products and Lubricating Oils, May 2004

### Function inputs

| Function inputs      | Remark   | EU     | SW tag   | Range     | Default |
|----------------------|--|--------|----------|-----------|---------|
| Name                 | Optional tag name, tag description and tag group   |        |          |           |         |
| Density at 15 °C     | Density at 15°C and 0 bar(g)   | kg/m3  |          | 0..1300   | 0       |
| Observed temperature | Temperature at which the density is observed   | °C     |          | -100..200 | 15      |
| Observed pressure    | Pressure at which the density is observed  | bar(g) |          | -1..250   | 0       |
| Product              | 1: A - Crude Oil<br>2: B - Auto select<br>Selection based on density at 15 °C<br>3: B - Gasoline<br>4: B - Transition Area<br>5: B - Jet Fuels<br>6: B - Fuel Oil<br>7: D - Lubricating Oil  |        | PRDTYP   |           | 1       |
| API rounding         | 0: Disabled<br>The calculations are performed with full precision and the final CTL, CPL and CTPL values are rounded as specified by the inputs 'CTL / CPL / CTPL decimal places'<br>1: Enabled<br>The input and output values are rounded in compliance with the standard. The CTL, CPL and CTPL value are rounded to 5 decimal places. |        | APIROUND |           | 0       |

### Function outputs

| Function outputs         | Remark   | EU    | SW tag | Alarm            | Fallback |
|--------------------------|--|-------|--------|------------------|----------|
| Status                   | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence   |       | STS    | FIOOR<br>CALCERR |          |
| Observed density         | Density at the observed temperature and pressure   | -     | DENS   |                  | 0        |
| CTL                      | Volume correction factor for temperature.<br>Value will be rounded according to input 'API rounding'   | -     | CTL    |                  | 1        |
| CPL                      | Volume correction factor for pressure<br>Value will be rounded according to input 'API rounding'   | -     | CPL    |                  | 1        |
| CTPL                     | Combined volume correction factor<br>CTPL = CTL * CPL  | -     | CTPL   |                  | 1        |
| K0                       | Actual value of constant K0 used for CTL calculation   | -     | K0     |                  | 0        |
| K1                       | Actual value of constant K1 used for CTL calculation   | -     | K1     |                  | 0        |
| K2                       | Actual value of constant K2 used for CTL calculation   | -     | K2     |                  | 0        |
| Alpha                    | Thermal expansion factor at 60 °F !  | 1/°C  | ALPHA  |                  | 0        |
| F                        | Compressibility factor   | 1/bar | F      |                  | 0        |
| Product                  | When input 'Product' is 'B - Auto select', then the output is set to the actual selected product of table B (enumerative value as defined for input 'Product'), else the output is set equal to input 'Product'. | -     | PRDCUR |                  | 0        |
| Calculation out of range | With respect to the standard the input values are:<br>0: In Range<br>1: Out of Range   | -     |        | OOR              | 0        |

### Calculations

The calculations are in either full or partial compliance with the standard, depending on whether API rounding is enabled or not.

## fxAPI\_Table54E

### Description

#### Density (15°C) --> CTL

This function calculates the volume correction factor for temperature from the relative density value at 15°C and the observed temperature.

The temperature correction is according to API MPMS 11.2.4:2007 (GPA TP-27).

### Function inputs

| Function inputs      | Remark  | EU | SW tag | Range     | Default |
|----------------------|---|----|--------|-----------|---------|
| Name                 | Optional tag name, tag description and tag group  |    |        |           |         |
| Density at 15°C      |   | -  |        | 0..750    | 0       |
| Observed temperature | Temperature at which the relative density is observed   | °C |        | -100..150 | 15      |
| API rounding         | 0: Disabled<br>The calculations are performed with full precision and the output values are not rounded<br>1: Enabled<br>The input and output values are rounded as defined in the standard |    |        |           | 0       |

### Function outputs

| Function outputs         | Remark  | EU | SW tag | Alarm            | Fallback |
|--------------------------|---|----|--------|------------------|----------|
| Status                   | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence            | -  | STS    | FLOOR<br>CALCERR | 1        |
| CTL                      | Volume correction factor for temperature<br>Value will be rounded according to input 'API rounding' | -  | CTL    |                  | 1        |
| Calculation out of range | With respect to the standard the input values are:<br>0: In Range<br>1: Out of Range                | -  |        | OOR              | 0        |

### Calculations

The calculations are in either full or partial compliance with the standard, depending on the selected type of API rounding.

### Compliance

- API MPMS 11.2.4: Temperature Correction for the Volume of NGL and LPG Tables 23E, 24E, 53E, 54E, 59E & 60E, September 2007
- GPA TP-27: Temperature Correction for the Volume of NGL and LPG Tables 23E, 24E, 53E, 54E, 59E & 60E, September 2007



## fxAPI\_Table59\_2004

### Description

#### Density (T, P) --> Density (20°C, 0 bar(g))

This function converts a density value at the observed temperature and pressure to the density value at 20°C and 0 bar(g).

The temperature and pressure correction is according to API MPMS 11.1:2004.

An iterative calculation needs to be applied to convert the observed density to the value at base conditions.

### Function inputs

| Function inputs      | Remark  | EU     | SW tag   | Range    | Default |
|----------------------|---|--------|----------|----------|---------|
| Name                 | Optional tag name, tag description and tag group  |        |          |          |         |
| Observed density     | Density at the observed temperature and pressure  | kg/m3  |          | 0..1300  | 0       |
| Observed temperature | Temperature at which the density is observed  | °C     |          | -10..200 | 20      |
| Observed pressure    | Pressure at which the density is observed   | bar(g) |          | -1..250  | 0       |
| Product              | 1: A - Crude Oil<br>2: B - Auto select<br>Selection based on density at 20 °C<br>3: B - Gasoline<br>4: B - Transition Area<br>5: B - Jet Fuels<br>6: B - Fuel Oil<br>7: D - Lubricating Oil   |        | PRDTYP   |          | 1       |
| API rounding         | 0: Disabled<br>The calculations are performed with full precision and the final CTL, CPL and CTPL values are rounded as specified by the inputs 'CTL / CPL/ CTPL decimal places'<br>1: Enabled<br>The input and output values are rounded in compliance with the standard. The CTL, CPL and CTPL value are rounded to 5 decimal places. |        | APIROUND |          | 0       |

Note: As opposed to API-2540, the 2004 standard does not include a correction for readings taken from a hydrometer and assumes that the equilibrium pressure is below atmospheric pressure, so taking 0 psig as the base pressure.

### Compliance

- API MPMS 11.1 Temperature and Pressure Volume Correction Factors for Generalized Crude Oils, Refined Products and Lubricating Oils, May 2004

### Function outputs

| Function outputs         | Remark   | EU    | SW tag | Alarm                      | Fallback |
|--------------------------|--|-------|--------|----------------------------|----------|
| Status                   | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence   | -     | STS    | FIOOR<br>CALCERR<br>NOCONV |          |
| Density at 20 °C         | Density at 20°C and 0 bar(g)   | -     | DENS20 |                            | 0        |
| CTL                      | Volume correction factor for temperature.<br>Value will be rounded according to input 'API rounding'   | -     | CTL    |                            | 1        |
| CPL                      | Volume correction factor for pressure<br>Value will be rounded according to input 'API rounding'   | -     | CPL    |                            | 1        |
| CTPL                     | Combined volume correction factor<br>CTPL = CTL * CPL  | -     | CTPL   |                            | 1        |
| K0                       | Actual value of constant K0 used for CTL calculation   | -     | K0     |                            | 0        |
| K1                       | Actual value of constant K1 used for CTL calculation   | -     | K1     |                            | 0        |
| K2                       | Actual value of constant K2 used for CTL calculation   | -     | K2     |                            | 0        |
| Alpha                    | Thermal expansion factor at 60 °F !  | 1/°C  | ALPHA  |                            | 0        |
| F                        | Compressibility factor   | 1/bar | F      |                            | 0        |
| Product                  | When input 'Product' is 'B - Auto select', then the output is set to the actual selected product of table B (enumerative value as defined for input 'Product'), else the output is set equal to input 'Product'. | -     | PRDCUR |                            | 0        |
| Calculation out of range | With respect to the standard the input values are:<br>0: In Range<br>1: Out of Range   | -     |        | OOR                        | 0        |

### Calculations

The calculations are in either full or partial compliance with the standard, depending on whether API rounding is enabled or not.

## fxAPI\_Table59E

### Description

#### Density (T) --> Density (20°C)

This function converts the density value at the observed temperature to the corresponding density at 20°C.  
The temperature correction is according to API MPMS 11.2.4:2007 (GPA TP-27).

### Function inputs

| Function inputs      | Remark  | EU    | SW tag   | Range     | Default |
|----------------------|---|-------|----------|-----------|---------|
| Name                 | Optional tag name, tag description and tag group  |       |          |           |         |
| Observed density     | Density at the observed temperature   | kg/m3 |          | 0..750    | 0       |
| Observed temperature | Temperature at which the relative density is observed   | °C    |          | -100..200 | 20      |
| API rounding         | 0: Disabled<br>The calculations are performed with full precision and the output values are not rounded<br>1: Enabled<br>The input and output values are rounded as defined in the standard |       | APIROUND |           | 0       |

### Compliance

- API MPMS 11.2.4: Temperature Correction for the Volume of NGL and LPG Tables 23E, 24E, 53E, 54E, 59E & 60E, September 2007
- GPA TP-27: Temperature Correction for the Volume of NGL and LPG Tables 23E, 24E, 53E, 54E, 59E & 60E, September 2007

### Function outputs

| Function outputs         | Remark   | EU | SW tag | Alarm                      | Fallback |
|--------------------------|--|----|--------|----------------------------|----------|
| Status                   | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence | -  | STS    | FLOOR<br>CALCERR<br>NOCONV |          |
| Density at 20°C          |  |    | DENS20 |                            | 0        |
| CTL                      | Volume correction factor for temperature.  | -  | CTL    |                            | 1        |
| Calculation out of range | With respect to the standard the input values are:<br>0: In Range<br>1: Out of Range     | -  |        | OOR                        | 0        |

### Calculations

The calculations are in either full or partial compliance with the standard, depending on the selected type of API rounding.

## fxAPI\_Table60\_2004

### Description

**Density (20°C, 0 bar(g)) --> Density (T, P)**

This function converts a density value at 20°C and 0 bar(g) to the density value at the observed temperature and pressure. The temperature and pressure correction is according to API MPMS 11.1:2004.

Note: The 2004 standard assumes that the equilibrium pressure is below atmospheric pressure, so taking 0 psig as the base pressure.

### Compliance

- API MPMS 11.1 Temperature and Pressure Volume Correction Factors for Generalized Crude Oils, Refined Products and Lubricating Oils, May 2004

### Function inputs

| Function inputs      | Remark   | EU     | SW tag   | Range     | Default |
|----------------------|--|--------|----------|-----------|---------|
| Name                 | Optional tag name, tag description and tag group   |        |          |           |         |
| Density at 20 °C     | Density at 20°C and 0 bar(g)   | kg/m3  |          | 0..1300   | 0       |
| Observed temperature | Temperature at which the density is observed   | °C     |          | -100..200 | 60      |
| Observed pressure    | Pressure at which the density is observed  | bar(g) |          | -1..250   | 0       |
| Product              | 1: A - Crude Oil<br>2: B - Auto select<br>Selection based on density at 20 °C<br>3: B - Gasoline<br>4: B - Transition Area<br>5: B - Jet Fuels<br>6: B - Fuel Oil<br>7: D - Lubricating Oil  |        | PRDTYP   |           | 1       |
| API rounding         | 0: Disabled<br>The calculations are performed with full precision and the final CTL, CPL and CTPL values are rounded as specified by the inputs 'CTL / CPL / CTPL decimal places'<br>1: Enabled<br>The input and output values are rounded in compliance with the standard. The CTL, CPL and CTPL value are rounded to 5 decimal places. |        | APIROUND |           | 0       |

### Function outputs

| Function outputs         | Remark   | EU    | SW tag | Alarm            | Fallback |
|--------------------------|--|-------|--------|------------------|----------|
| Status                   | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence   | -     | STS    | FIOOR<br>CALCERR |          |
| Observed density         | Density at the observed temperature and pressure   | -     | DENS   |                  | 0        |
| CTL                      | Volume correction factor for temperature.<br>Value will be rounded according to input 'API rounding'   | -     | CTL    |                  | 1        |
| CPL                      | Volume correction factor for pressure<br>Value will be rounded according to input 'API rounding'   | -     | CPL    |                  | 1        |
| CTPL                     | Combined volume correction factor<br>CTPL = CTL * CPL  | -     | CTPL   |                  | 1        |
| K0                       | Actual value of constant K0 used for CTL calculation   | -     | K0     |                  | 0        |
| K1                       | Actual value of constant K1 used for CTL calculation   | -     | K1     |                  | 0        |
| K2                       | Actual value of constant K2 used for CTL calculation   | -     | K2     |                  | 0        |
| Alpha                    | Thermal expansion factor at 60 °F !  | 1/°C  | ALPHA  |                  | 0        |
| F                        | Compressibility factor   | 1/bar | F      |                  | 0        |
| Product                  | When input 'Product' is 'B - Auto select', then the output is set to the actual selected product of table B (enumerative value as defined for input 'Product'), else the output is set equal to input 'Product'. | -     | PRDCUR |                  | 0        |
| Calculation out of range | With respect to the standard the input values are:<br>0: In Range<br>1: Out of Range   | -     |        | OOR              | 0        |

### Calculations

The calculations are in either full or partial compliance with the standard, depending on whether API rounding is enabled or not.

## fxAPI\_Table60E

### Description

#### Density (20°C) --> CTL

This function calculates the volume correction factor for temperature from the relative density value at 20°C and the observed temperature.

The temperature correction is according to API MPMS 11.2.4:2007 (GPA TP-27).

### Function inputs

| Function inputs      | Remark  | EU | SW tag   | Range     | Default |
|----------------------|---|----|----------|-----------|---------|
| Name                 | Optional tag name, tag description and tag group  |    |          |           |         |
| Density at 20°C      |   | -  |          | 0..750    | 0       |
| Observed temperature | Temperature at which the relative density is observed   | °C |          | -100..150 | 20      |
| API rounding         | 0: Disabled<br>The calculations are performed with full precision and the output values are not rounded<br>1: Enabled<br>The input and output values are rounded as defined in the standard |    | APIROUND |           | 0       |

### Function outputs

| Function outputs         | Remark  | EU | SW tag | Alarm            | Fallback |
|--------------------------|---|----|--------|------------------|----------|
| Status                   | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence            | -  | STS    | FLOOR<br>CALCERR |          |
| CTL                      | Volume correction factor for temperature<br>Value will be rounded according to input 'API rounding' | -  | CTL    |                  | 1        |
| Calculation out of range | With respect to the standard the input values are:<br>0: In Range<br>1: Out of Range                | -  |        | OOR              | 0        |

### Calculations

The calculations are in either full or partial compliance with the standard, depending on the selected type of API rounding.

### Compliance

- API MPMS 11.2.4: Temperature Correction for the Volume of NGL and LPG Tables 23E, 24E, 53E, 54E, 59E & 60E, September 2007
- GPA TP-27: Temperature Correction for the Volume of NGL and LPG Tables 23E, 24E, 53E, 54E, 59E & 60E, September 2007

## fxASTM\_D1550\_RD60

### Description

This function calculates the relative density at 60°F and 0 psig of Butadiene based on ASTM Designation 1550. The ASTM-D1550 standard specifies several tables. This function uses table 1, which contains values for the relative density at 60°F as a function of the observed relative density and the observed temperature. The compressibility factor is calculated in accordance with API MPMS 11.2.2:1984.

### Compliance

- ASTM Designation: D1550 -94 (Reapproved 2005), Standard ASTM Butadiene Measurement Table 1 Reduction of observed specific gravity to specific gravity at 15.6/15. °C (60/60°F)
- API MPMS 11.2.2 - Compressibility Factors for Hydrocarbons: 0.350 - 0.637 Relative Density (60°F/60°F) and -50°F to 140°F Metering Temperature - Second Edition, October 1986

### Boundaries

ASTM D1550 table 1 consists of table values with a resolution of 0.005 for the relative density and 1°F for the temperature. The function applies a linear interpolation between table values based on the input values. The table specifies relative density at 60°F values that are limited to a low value of 0.621 and a high value of 0.634. When the combination of input values lies outside the range covered by the table, the function outputs either the low or high table value depending on whether the input values lay below or above the table limits.

API MPMS 11.2.2 applies for the following range:

- 0.350 to 0.637 (relative density)
- 50 to 140 °F
- 0 to 2200 psig

### Function inputs

| Function inputs           | Remark  | EU   | Range     | Default |
|---------------------------|---|------|-----------|---------|
| Name                      | Optional tag name, tag description and tag group  |      |           |         |
| Observed relative density |   | -    | 0..1      | 0       |
| Observed temperature      | Temperature at which the relative density is observed   | °F   | -100..150 | 20      |
| Observed pressure         | Pressure at which the relative density is observed  | Psig | -10..2500 | 0       |
| API 11.2.2 rounding       | 0: Disabled<br>The calculations are performed with full precision<br>1: Enabled<br>The input and intermediate values are rounded and truncated as defined in the standard |      |           | 0       |

### Function outputs

| Function outputs                    | Remark  | EU    | SW tag   | Alarm            | Fallback |
|-------------------------------------|---|-------|----------|------------------|----------|
| Status                              | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence                              | -     | STS      | FIOOR<br>CALCERR |          |
| Relative density at 60°F            |   | -     | RD60     |                  | 0        |
| F                                   | Compressibility factor<br>The output value will be either rounded or not depending input 'API 11.2.2 rounding'        | 1/psi | F        |                  | 0        |
| CTL                                 | Volume correction factor for temperature.   | -     | CTL      |                  | 1        |
| CPL                                 | Volume correction factor for pressure<br>Value will be rounded according to input 'API 11.2.2 rounding'               | -     | CPL      |                  | 1        |
| ASTM D1550 calculation out of range | With respect to ASTM D1550 table 1 the input values are:<br>0: In Range<br>1: Out of Range                            | -     | ASTM_OOR |                  | 0        |
| API 11.2.2 calculation out of range | With respect to API 11.2.2 the conditions of density, temperature and pressure are:<br>0: In Range<br>1: Out of Range |       | API_OOR  |                  |          |

### Calculations

The function performs the following iterative algorithm to calculate the relative density at 60 °F and 0 psig. No rounding is applied

- At the start of the iteration the relative density at [60 °F, 0 psig] is set equal to the observed relative density and the CPL value is set to 1.
- The relative density corrected for pressure is calculated by dividing the observed relative density by the CPL value.
- The CTL value and the relative density at [60 °F, equilibrium pressure] is calculated from the relative density corrected for pressure and the observed temperature according to ASTM D1550 Table 1

- The compressibility factor F is calculated according to API MPMS 11.2.2 from the relative density at [60 °F, equilibrium pressure] and the 'Observed temperature'. Depending on setting 'API 11.2.2. rounding' the rounding and truncation rules of API 11.2.2. are applied for this step.
- The CPL value is calculated from the calculated compressibility factor and the 'Observed pressure' input value.
- The new value for relative density at [60°F, 0 psig] is calculated by dividing the observed density by the CTL and CPL values.
- Steps 2 through 6 are repeated until the absolute difference between two consecutive relative density values is less than the convergence limit of 1e-8.

- 8 When no convergence is achieved in 20 iterations then the status output is set to 'No convergence' and the relative density output is set to 0.

## fxASTM\_D1550\_Ctl

### Description

This function calculates the Ctl value (VCF) of Butadiene based on the ASTM Designation 1550. The standard specifies several tables. This function uses table 2, which contains values for the volume correction factor as a function of the relative density at 60°F and the observed temperature.

### Function inputs

| Function inputs          | Remark  | EU | SW tag | Range     | Default |
|--------------------------|---|----|--------|-----------|---------|
| Name                     | Optional tag name, tag description and tag group      |    |        |           |         |
| Relative density at 60°F |   | -  |        | 0..1      | 0       |
| Observed temperature     | Temperature at which the relative density is observed | °F |        | -100..150 | 20      |

### Compliance

- ASTM Designation: D1550 -94 (Reapproved 2005), Standard ASTM Butadiene Measurement Table 2 Reduction of Observed Volume to 15.6°C (60°F) Against Specific Gravity 60/60°F

### Function outputs

| Function outputs         | Remark   | EU | SW tag | Alarm            | Fallback |
|--------------------------|--|----|--------|------------------|----------|
| Status                   | 0: Normal<br>1: Input argument out of range<br>2: Calculation error                  | -  | STS    | FLOOR<br>CALCERR |          |
| Ctl                      | Volume correction factor for temperature. The output value will NOT be rounded.      | -  | CTL    |                  | 1        |
| Calculation out of range | With respect to the standard the input values are:<br>0: In Range<br>1: Out of Range | -  |        | OOR              | 0        |

### Calculations

The Standard consists of a set of table values with a resolution of 0.001 for the relative density at 60°F and 1°F for temperature. The function applies a linear interpolation between table values based on the unrounded input values. When an input value lies outside the range of the table the function limits the input value to the minimum or maximum value of the table.

fxASTM\_D4311M\_09\_C

Description

This function calculates the Ctl value (VCF) for Asphalt according to ASTM D4311/D4311M-09, using US Customary units.

Compliance

- ASTM Designation: D4311/D4311M-09, Standard Practice for Determining Asphalt Volume Correction to a Base Temperature

Function inputs

| Function inputs      | Remark   | EU | SW tag | Range   | Default |
|----------------------|--|----|--------|---------|---------|
| Name                 | Optional tag name, tag description and tag group |    |        |         |         |
| API gravity at 60°F  |  | -  |        | 0..34.9 | 0       |
| Observed temperature |  | °F |        | 0..500  | 60      |

Function outputs

| Function outputs | Remark  | EU | SW tag | Alarm   | Fallback |
|------------------|---|----|--------|---------|----------|
| Status           | 0: Normal   | -  | STS    |         |          |
|                  | 1: Input argument out of range  |    |        | FLOOR   |          |
|                  | 2: Calculation error  |    |        | CALCERR |          |
| Ctl              | Volume correction factor for temperature. The output value will NOT be rounded. | -  | CTL    |         | 1        |

Calculations

The calculations are in accordance with appendix X1. FORMULAS USED IN DETERMINING VOLUME CORRECTIONS TO A BASE TEMPERATURE of the standard.



## fxASTM\_D4311M\_09\_M

### Description

This function calculates the Ctl value (VCF) for Asphalt according to ASTM D4311/D4311M-09, using metric units.

### Compliance

- ASTM Designation: D4311/D4311M-09, Standard Practice for Determining Asphalt Volume Correction to a Base Temperature

### Function inputs

| Function inputs      | Remark   | EU    | SW tag | Range      | Default |
|----------------------|--|-------|--------|------------|---------|
| Name                 | Optional tag name, tag description and tag group |       |        |            |         |
| Density at 15°C      |  | kg/m3 |        | 800..1200  | 966     |
| Observed temperature |  | °C    |        | -25..274.5 | 15      |

### Function outputs

| Function outputs | Remark  | EU | SW tag | Alarm            | Fallback |
|------------------|---|----|--------|------------------|----------|
| Status           | 0: Normal<br>1: Input argument out of range<br>2: Calculation error             | -  | STS    | FLOOR<br>CALCERR |          |
| Ctl              | Volume correction factor for temperature. The output value will NOT be rounded. | -  | CTL    |                  | 1        |

### Calculations

The calculations are in accordance with appendix X1. FORMULAS USED IN DETERMINING VOLUME CORRECTIONS TO A BASE TEMPERATURE of the standard.

## fxConvertUnit

### Description

This function converts a value expressed in a particular unit into the corresponding value expressed in another unit.

The input and output unit must belong category, otherwise the conversion fails.

### Function inputs

| Function inputs | Remark   | EU | SW tag | Range | Default |
|-----------------|--|----|--------|-------|---------|
| Name            |  |    |        |       |         |
| Input value     | The value to be converted  |    |        |       |         |
| Input unit      | Unit of the value to be converted<br>Use one of the "xu_..." unit constants. |    |        |       |         |
| Output unit     | Unit of the output value<br>Use one of the "xu_..." unit constants.          |    |        |       |         |

### Function outputs

| Function outputs   | Remark   | EU            | SW tag   | Alarm | Fallback |
|--------------------|--|---------------|----------|-------|----------|
| Output value       |  | <Output unit> | VAL      |       | 0        |
| Conversion failure | The conversion fails when the input unit and output unit do not belong to the same unit category (or also when the input unit and / or output unit are not a valid unit).<br>0: Normal<br>1: Failure |               | CONVFAIL |       |          |

## fxEthylene\_IUPAC\_C

### Description

The function calculates the compressibility factor and the density of Ethylene (C<sub>2</sub>H<sub>4</sub>, also called Ethene) based on the Equation Of State published by IUPAC and in **US customary units**.

### Boundaries

The limits of the tables are 104 K to 320 K (-272 .. +116 °F) for pressures up to 270 MPa (39160 psi) and 104K to 450K (-272 .. +350 °F) for pressures up to 40 MPa (5800 psi).

### References

- Ethylene (Ethene), International Thermodynamic Tables of the Fluid State Vol. 10 (1988), IUPAC, ISBN 0-63201-7090.

### Function inputs

| Function inputs | Remark   | EU   | Range     | Default |
|-----------------|--|------|-----------|---------|
| Name            | Optional tag name, tag description and tag group |      |           |         |
| Temperature     |  | °F   | -300..200 | 0       |
| Pressure        |  | psia | 0..50000  | 0       |

### Function outputs

| Function outputs     | Remark  | EU      | Fallback |
|----------------------|---|---------|----------|
| Status               | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence                      |         |          |
| Density              |   | lbm/ft3 | 0        |
| Compressibility      |   | -       | 0        |
| Equilibrium pressure | Equilibrium pressure at the observed temperature.<br>Also referred to as vapor pressure or saturated pressure | psia    | 0        |
| Range                | With respect to the combination of temperature and pressure is:<br>0: In Range<br>1: Out of Range             | -       | 0        |

### Calculations

The calculations are in compliance with the standard.



## fxEthylene\_NIST1045

### Description

The function calculates the density of Ethylene (C<sub>2</sub>H<sub>4</sub>, also called Ethene) based on the NIST-1045 Equation Of State in **metric units**.

### Boundaries

The equation of state is valid from 104 K to 400 K (-170 .. +127 °C) and for pressures up to 40 MPa (400 bar).

### References

- R.D. McCarty and R.T. Jacobsen "An Equation of State for Fluid Ethylene", National Bureau of Standards (NBS), US, Technical Note 1045, 1981.

### Function inputs

| Function inputs | Remark   | EU     | Range     | Default |
|-----------------|--|--------|-----------|---------|
| Name            | Optional tag name, tag description and tag group   |        |           |         |
| Temperature     |  | °C     | -200..200 | 0       |
| Pressure        |  | bar(a) | 500       | 0       |
| Rounding        | 0: Disabled<br>The calculations are performed with full precision. A convergence limit of 1e-10 kg/m <sup>3</sup> will be applied for the iterative calculations.<br>1: Enabled<br>The calculations are performed in full compliance with the standard. The input, intermediate and output values are rounded as specified and also the iteration limit as specified in the standard is used to achieve convergence. | -      |           | 1       |

### Function outputs

| Function outputs     | Remark  | EU                | Fallback |
|----------------------|---|-------------------|----------|
| Status               | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence                      |                   |          |
| Density              |   | kg/m <sup>3</sup> | 0        |
| Compressibility      |   | -                 | 0        |
| Equilibrium pressure | Equilibrium pressure at the observed temperature.<br>Also referred to as vapor pressure or saturated pressure | bar(a)            | 0        |
| Range                | With respect to the standard the inputs are:<br>0: In Range<br>1: Out of Range                                | -                 | 0        |

### Calculations

The calculations are in compliance with the standard.

## fxGasViscosity\_2004

### Description

The dynamic viscosity of natural gas is calculated in accordance with a method developed at the Rostock University in Germany and published in 2004 in the 'International Journal of the Thermophysics'. The estimated uncertainty of the calculated viscosity is 0.5% for natural gas (0.3% for pure methane).

### Boundaries

The limits of the tables are 250 K to 450 K (-24 .. +177 °C) for pressures up to 30 MPa (300 bar).

### Reference

- Viscosity Measurements and Predictions for Natural Gas, P. Schley, M. Jaeschke, C. Kuchenmeister and E. Vogel, International Journal of Thermophysics, Vol. 25, No. 6, November 2004 (© 2004)

### Function inputs

| Function inputs | Remark   | EU      | Range      | Default |
|-----------------|--|---------|------------|---------|
| Name            | Optional tag name, tag description and tag group                       |         |            |         |
| Density         | Density value  | kg/m3   | 0..2000    | 0       |
| Temperature     | Temperature value  | °C      | -200..+400 | 0       |
| Composition     | Standard composition as defined in section 'Standard gas composition'. | mol/mol | 0..1       | 0       |

### Function outputs

| Function outputs  | Remark  | EU   | Fallback |
|-------------------|---|------|----------|
| Status            | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence<br>4: Mole fractions do not add up to 1.0 +- 0.0001<br>6: Hardware not supported |      |          |
| Dynamic viscosity |   | Pa.s | 0        |
| Range             | With respect to the combination of temperature and pressure is:<br>0: In Range<br>1: Out of Range   |      | 0        |

### Calculations

The calculations are in accordance with the publication, which is based on the following 12 components: methane (+ hydrogen), nitrogen (+ helium + oxygen/argon), carbon dioxide, ethane, propane, n-butane, ibutane, n-pentane (+ benzene), isentane (+ neopentane), n-hexane (hexanes + toluene), n-heptane (heptanes), and n-octane (octanes + nonanes+ C10 plus higher + xylenes).

The function uses the 'Standard gas composition' as used by most gas property functions. The 22 components of input Composition are lumped to these 12 components as defined in the following table.

#### Notes:

- Components 'Water', 'Hydrogen sulphide' and 'Carbon monoxide' are not supported by the publication and will therefore be neglected by the function. The lumped composition is normalized to 1 and then used in the calculation.
- The publication also mentions components benzene, toluene and xylenes, which are not part of the 'Standard gas composition'. To adhere strictly to the publication, add 'Benzene' to input 'n-Pentane', 'Toluene' to input 'n-Hexane' and 'Xylenes' to input 'n-Octane'.

| Input component   | Added to / neglected |
|-------------------|----------------------|
| Methane           | Methane              |
| Nitrogen          | Nitrogen             |
| Carbon Dioxide    | Carbon Dioxide       |
| Ethane            | Ethane               |
| Propane           | Propane              |
| Water             | <b>Neglected</b>     |
| Hydrogen Sulphide | <b>Neglected</b>     |
| Hydrogen          | <b>Methane</b>       |
| Carbon Monoxide   | <b>Neglected</b>     |
| Oxygen            | <b>Nitrogen</b>      |
| i-Butane          | i-Butane             |
| n-Butane          | n-Butane             |
| i-Pentane         | i-Pentane            |
| n-Pentane         | n-Pentane            |
| n-Hexane          | n-Hexane             |
| n-Heptane         | n-Heptane            |
| n-Octane          | n-Octane             |
| n-Nonane          | <b>n-Octane</b>      |
| n-Decane          | <b>n-Octane</b>      |
| Helium            | <b>Nitrogen</b>      |
| Argon             | <b>Nitrogen</b>      |
| Neo-Pentane       | <b>Iso-Pentane</b>   |

## fxGERG2008\_Gas

### Description

The compressibility, density, speed of sound and isentropic coefficient of a gas are calculated from its composition, temperature and pressure in accordance with the GERG-2008 equation of state. The function uses an optimized routine that only applies when fluid is in the gaseous state (100% gas) and that requires limited CPU time (suitable for processing in the Flow-X flow computer).

### Compliance

- The GERG-2008 Wide-Range Equation of State for Natural Gases and Other Mixtures: An Expansion of GERG-2004. Kunz, O., Wagner, W. Submitted to J. Chem. Eng. Data 57 (2012).

### Boundaries

The GERG-2008 calculation has defined uncertainty bounds for fluids that lie within the 'Normal range'. Also an 'Expanded range' of gas mixtures is defined for which the calculation has a higher uncertainty. Using the calculation at conditions outside the 'Expanded range' is not recommended.

| Input value                     | Normal Range | Expanded Range | EU     |
|---------------------------------|--------------|----------------|--------|
| Pressure                        | 0 .. 35      | 0 .. 70        | MPa(a) |
| Temperature                     | 90..450      | 60..700        | K      |
| Pressure                        | 0 .. 350     | 0 .. 700       | bar(a) |
| Temperature                     | -183 .. +177 | -213 .. +426   | °C     |
| Pressure                        | 0 .. 5076    | 0 .. 10153     | psia   |
| Temperature                     | -298 .. +350 | -352 .. +800   | °F     |
| Mole fraction of all components | 0.00 .. 1.00 | 0.00 .. 1.00   | -      |

### Function inputs

| Function inputs  | Remark   | EU      | SW tag     | Range      | Default |
|------------------|--|---------|------------|------------|---------|
| Name             | Optional tag name, tag description and tag group   |         |            |            |         |
| Pressure         | Pressure value   | bar(a)  |            | 0..2000    | 1.01325 |
| Temperature      | Temperature value  | °C      |            | -200..+400 | 0       |
| Composition      | Standard composition as defined in section 'Standard gas composition.  | mol/mol | COMP       | 0..1       | 0       |
| neo-Pentane mode | Determines what to do when component neo-Pentane is larger than zero<br>1: Add to i-Pentane<br>2: Add to n-Pentane<br>3: Neglect | -       | NEOC5_MODE |            | 1       |

### Function outputs

| Function outputs    | Remark   | EU      | SW tag  | Alarm                                 | Fallback |
|---------------------|--|---------|---------|---------------------------------------|----------|
| Status              | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence<br>4: Mole fractions do not add up to 1.0 +/- 0.0001<br>6: Hardware not supported   |         | STS     | FLOOR<br>CALCERR<br>NOCONV<br>COMPERR |          |
| Compressibility     |  | -       | Z       |                                       | 1        |
| Mass Density        |  | kg/m3   | MASDENS |                                       | 0        |
| Molar Density       |  | kmol/m3 | MOLDENS |                                       | 0        |
| Molar Mass          |  | kg/kmol | MOLMASS |                                       | 0        |
| Speed of Sound      |  | m/s     | SOS     |                                       | 0        |
| Isentropic Exponent |  | -       | K       |                                       | 0        |
| Range               | 0: In Normal Range<br>All inputs are within the 'Normal Range'<br>1: In Extended Range<br>One or more inputs within the 'Extended Range, but none of the inputs outside the Extended rang (outputs values have higher uncertainty)<br>2: Out of Range<br>One or more inputs outside the 'Extended Range' (using the calculation is not recommended in this case) |         | RANGE   |                                       | 0        |
|                     |  |         |         | OOR                                   |          |

### Calculations

The calculations are as documented in the reference.

## fxGERG2008\_Flash

### Description

The compressibility and density of a gas/liquid mixture are calculated from its composition, temperature and pressure in accordance with the GERG2008 standard.

### Compliance

- Kunz, O., and W. Wagner. "The GERG-2008 wide-range equation of state for natural gases and other mixtures: An expansion of GERG-2004." Journal of Chemical & Engineering Data 57.11 (2012): 3032-3091.
- W. Wagner. "Description of the Software Package for the Calculation of Thermodynamic Properties from the GERG-2008 Wide-Range Equation of State for Natural Gases and Other Mixtures".

### Boundaries

The GERG2008 calculation has defined uncertainty bounds for gas mixtures that lie within the 'Normal range'. Also an 'Expanded range' of gas mixtures is defined for which the GERG2008 calculation has a higher uncertainty. Using the GERG2008 calculation for gas mixtures that lie outside the 'Expanded range' is not recommended.

### Function inputs

| Function inputs  | Remark   | EU      | SW tag     | Range      | Default |
|------------------|--|---------|------------|------------|---------|
| Name             | Optional tag name, tag description and tag group   |         |            |            |         |
| Pressure         | Pressure value   | bar(a)  |            | 0..2000    | 1.01325 |
| Temperature      | Temperature value  | °C      |            | -200..+400 | 0       |
| Composition      | Standard composition as defined in section 'Standard gas composition'.   | mol/mol | COMP       | 0..1       | 0       |
| neo-Pentane mode | Determines what to do when component neo-Pentane is larger than zero<br>1: Add to i-Pentane<br>2: Add to n-Pentane<br>3: Neglect | -       | NEOC5_MODE |            | 1       |

### Function outputs

| Function outputs       | Remark   | EU    | SW tag | Alarm                                 | Fallback |
|------------------------|--|-------|--------|---------------------------------------|----------|
| Status                 | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence<br>4: Mole fractions do not add up to 1.0 +/- 0.0001<br>6: Hardware not supported |       | STS    | FLOOR<br>CALCERR<br>NOCONV<br>COMPERR |          |
| Vapor fraction         |  |       | FV     |                                       | 0        |
| Compressibility vapor  | Compressibility of the vapor fraction of the mixture   |       | ZV     |                                       | 0        |
| Compressibility liquid | Compressibility of the liquid fraction of the mixture  |       | ZL     |                                       | 0        |
| Compressibility total  | Compressibility of the mixture   |       | Z      |                                       | 0        |
| Density vapor          | Density of the vapor fraction of the mixture   | kg/m3 | DV     |                                       | 0        |
| Density liquid         | Density of the liquid fraction of the mixture  | kg/m3 | DL     |                                       | 0        |
| Density total          | Density of the mixture   | kg/m3 | D      |                                       | 0        |

### Calculations

The calculations are as documented in the standard.

| Input value                      | Normal Range | Expanded Range | EU     |
|----------------------------------|--------------|----------------|--------|
| Pressure                         | 0 .. 350     | 0 .. 700       | bar(a) |
| Temperature                      | -183 .. +177 | -213 .. +427   | °C     |
| Mole fraction of Methane         | 0.00 .. 1.00 | 0.00 .. 1.00   | -      |
| Mole fraction of Ethane          | 0.00 .. 1.00 | 0.00 .. 1.00   | -      |
| Mole fraction of Propane         | 0.00 .. 1.00 | 0.00 .. 1.00   | -      |
| Mole fraction of Butanes         | 0.00 .. 1.00 | 0.00 .. 1.00   | -      |
| Mole fraction of Pentanes        | 0.00 .. 1.00 | 0.00 .. 1.00   | -      |
| Mole fraction of Hexanes Plus    | 0.00 .. 1.00 | 0.00 .. 1.00   | -      |
| Mole fraction of Carbon monoxide | 0.00 .. 1.00 | 0.00 .. 1.00   | -      |
| Mole fraction of Carbon dioxide  | 0.00 .. 1.00 | 0.00 .. 1.00   | -      |
| Mole fraction of Nitrogen        | 0.00 .. 1.00 | 0.00 .. 1.00   | -      |
| Mole fraction of Helium          | 0.00 .. 1.00 | 0.00 .. 1.00   | -      |
| Mole fraction of Argon           | 0.00 .. 1.00 | 0.00 .. 1.00   | -      |
| Mole fraction of Oxygen          | 0.00 .. 1.00 | 0.00 .. 1.00   | -      |
| Mole fraction of Hydrogen        | 0.00 .. 1.00 | 0.00 .. 1.00   | -      |
| Sulphide                         |              |                |        |
| Mole fraction of Hydrogen        | 0.00 .. 1.00 | 0.00 .. 1.00   | -      |
| Mole fraction of Water           | 0.00 .. 1.00 | 0.00 .. 1.00   | -      |



## fxGOST30319

### Description

Thermodynamic properties of a gas are calculated from its composition, temperature and pressure in accordance with GOST30319 standard, with the input and output values in **metric** units.

### Boundaries

The GOST30319 calculation has the normal range 263.15K..500K, 1bar..150bar and the extended range 125K..700K, 0bar..3500bar.

### Compliance

- GOST30319-2.96 - 1 July 1997

### Function inputs

| Function inputs       | Remark   | EU      | SW tag | Range      | Default |
|-----------------------|--|---------|--------|------------|---------|
| Name                  | Optional tag name, tag description and tag group   |         |        |            |         |
| Pressure              | Pressure value   | bar(a)  |        | 0..3500    | 1.01325 |
| Temperature           | Temperature value  | °C      |        | -250..+450 | 25      |
| Composition           | Standard composition as defined in section 'Standard gas composition.'   | mol/mol |        | 0..1       | 0       |
| neo-Pentane mode      | Determines what to do when component neo-Pentane is larger than zero<br>1: Add to i-Pentane<br>2: Add to n-Pentane<br>3: Neglect | -       |        |            | 1       |
| Reference pressure    |  | bar(a)  |        | 0..3500    | 0       |
| Reference temperature |  | °C      |        | -250..+450 | 25      |

### Function outputs

| Function outputs      | Remark   | EU     | SW tag   | Alarm                                 | Fallback |
|-----------------------|--|--------|----------|---------------------------------------|----------|
| Status                | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence<br>4: Mole fractions do not add up to 1.0 +/- 0.0001  |        | STS      | FLOOR<br>CALCERR<br>NOCONV<br>COMPERR |          |
| Compressibility ratio | Compressibility ratio between flow and base conditions   | -      | ZRATIO   |                                       | 1        |
| Flow compressibility  | Compressibility factor at flow conditions  | -      | ZF       |                                       | 1        |
| Base compressibility  | Compressibility factor at base conditions  | -      | ZB       |                                       | 1        |
| Critical density      |  | kg/m3  | CRITDENS |                                       | 0        |
| Reduced density       | Ratio between current and critical   | -      | REDUDENS |                                       | 1        |
| Critical temperature  |  | °C     | CRITTEMP |                                       | 0        |
| Reduced temperature   | Ratio between current and critical   | -      | REDUTEMP |                                       | 1        |
| Critical pressure     |  | bar(a) | CRITPRES |                                       | 0        |
| Reduced pressure      | Ratio between current and critical   | -      | REDUPRES |                                       | 1        |
| Pitzer factor         | Denoted as Capital Omega   | -      | PITZER   |                                       | 0        |
| Range                 | 0: In Normal Range<br>All inputs are within the 'Normal Range'<br>1: In Extended Range<br>One or more inputs within the 'Extended Range', but none of the inputs outside the Extended range (outputs values have higher uncertainty)<br>2: Out of Range<br>One or more inputs outside the 'Extended Range' (using the calculation is not recommended in this case) |        | OOR      |                                       | 0        |
|                       |  |        |          | OOR                                   |          |

### Calculations

The calculations are performed according to the source code of Sick GmbH.

## fxGOST30319\_AGA8

### Description

Compressibility of a gas are calculated from its composition, temperature and pressure in accordance with GOST30319 standard, with the input and output values in **metric** units.

### Boundaries

The GOST30319 calculation has the normal range 263.15K..500K, 1bar..150bar and the extended range 125K..700K, 0bar..3500bar.

### Compliance

- GOST30319-2.96, chapter AGA8 - 1 July 1997

### Function inputs

| Function inputs       | Remark   | EU      | SW tag | Range      | Default |
|-----------------------|--|---------|--------|------------|---------|
| Name                  | Optional tag name, tag description and tag group   |         |        |            |         |
| Pressure              | Pressure value   | bar(a)  |        | 0..3500    | 1.01325 |
| Temperature           | Temperature value  | °C      |        | -250..+450 | 25      |
| Composition           | Standard composition as defined in section 'Standard gas composition.  | mol/mol |        | 0..1       | 0       |
| neo-Pentane mode      | Determines what to do when component neo-Pentane is larger than zero<br>1: Add to i-Pentane<br>2: Add to n-Pentane<br>3: Neglect | -       |        |            | 1       |
| Reference pressure    |  | bar(a)  |        | 0..3500    | 0       |
| Reference temperature |  | °C      |        | -250..+450 | 25      |

### Function outputs

| Function outputs      | Remark  | EU    | SW tag | Alarm                                 | Fallback |
|-----------------------|---|-------|--------|---------------------------------------|----------|
| Status                | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence<br>4: Mole fractions do not add up to 1.0 +/- 0.0001 |       | STS    | FIOOR<br>CALCERR<br>NOCONV<br>COMPERR |          |
| Compressibility ratio | Compressibility ratio between flow and base conditions  | -     | ZRATIO |                                       | 1        |
| Flow compressibility  | Compressibility factor at flow conditions   | -     | ZF     |                                       | 1        |
| Base compressibility  | Compressibility factor at base conditions   | -     | ZB     |                                       | 1        |
| Heating value         |   | MJ/m3 | HV     |                                       | 0        |

### Calculations

The calculations are performed according to the source code of Sick GmbH.

## fxGOST30319\_SGERG91

### Description

Thermodynamic properties of a gas are calculated from its density, speed of sound, fractions of nitrogen and carbon dioxide, temperature and pressure in accordance with GOST30319 standard, with the input and output values in **metric** units.

### Compliance

- GOST30319-2.96, chapter GERG91mod (1996)
- GOST30319-2.2015, chapter GERG91mod (2015)

### Boundaries

The 'Range' output of this function is set as follows

|                | 1996         | 2015         |         |
|----------------|--------------|--------------|---------|
| Pressure       | 1 ..120      | 1 ..75       | bar(a)  |
| Temperature    | 250..340     | 250..350     | K       |
| Carbon dioxide | 0.00 .. 0.20 | 0.00 .. 0.20 | mol/mol |
| Nitrogen       | 0.00 .. 0.15 | 0.00 .. 0.20 | mol/mol |
| Normal density | 0.66 .. 1.00 | 0.66 .. 1.05 | kg/m3   |

### Function inputs

| Function inputs | Remark   | EU      | SW tag | Range      | Default |
|-----------------|--|---------|--------|------------|---------|
| Name            | Optional tag name, tag description and tag group   |         |        |            |         |
| Pressure        | Pressure value                                     | bar(a)  |        | 0..2000    | 7       |
| Temperature     | Temperature value                                  | °C      |        | -200..+300 | 25      |
| N2              | Nitrogen fraction                                  | mol/mol |        | 0..1       | 0.01    |
| CO2             | Carbon dioxide fraction                            | mol/mol |        | 0..1       | 0.02    |
| Normal density  | Density at base conditions                         | kg/m3   |        | 0.66..1.0  |         |
| Speed of sound  | Optional, needed for the calculation of molar mass | m/s     |        |            | 0       |
| Edition         | Year of edition<br>1: 1997<br>2: 2015              | -       |        | -          | 1       |

### Description

| Function outputs      | Remark  | EU      | SW tag   | Alarm            | Fallback |
|-----------------------|---|---------|----------|------------------|----------|
| Status                | 0: Normal<br>1: Input argument out of range<br>2: Calculation error |         | STS      | FLOOR<br>CALCERR |          |
| Base compressibility  | Compressibility factor at base conditions                           | -       | ZB       |                  | 1        |
| Flow compressibility  | Compressibility factor at flow conditions                           | -       | ZF       |                  | 1        |
| Compressibility ratio | Compressibility ratio between flow and base conditions              | -       | ZRATIO   |                  | 1        |
| Base density          |   | kg/m3   | BASEDENS |                  | 0        |
| Flow density          | Compressibility ratio between flow and base conditions              | kg/m3   | FLOWDENS |                  | 0        |
| Heating value         |   | MJ/m3   | HV       |                  | 0        |
| Molar mass            | Only calculated if a valid Speed Of Sound specified                 | kg/kmol | MM       |                  | 0        |
| Range                 | The inputs are within the normal range of use                       |         | RANGE    |                  | 0        |

### Calculations

The calculations are performed according to the source code of Sick GmbH.

## fxGPA\_TP15

### Description

The GPA-TP15 standard defines a generalized correlation method to determine the vapor pressure (i.e. the equilibrium pressure) for natural gas liquids (NGL).

The vapor pressure is required by the API 11.2.2 and API 11.1:2004 calculations of the CPL value for light hydrocarbon liquids that have a vapor pressure above atmospheric pressure.

### References

- API MPMS 11.2.2 Addendum - Compressibility Factors for Hydrocarbons: Correlation Factors of Vapor Pressure for Commercial Natural Gas Liquids - First Edition, December 1994
- GPA Technical Publication TP-15 A Simplified Vapor Pressure Correlation for Commercial NGLs - 1988
- API MPMS 11.2.5 - A Simplified Vapor Pressure Correlation for Commercial NGLs - September 2007
- GPA Technical Publication TP-15 A Simplified Vapor Pressure Correlation for Commercial NGLs - September 2007
- ASTM Technical Publication [Stock No. PETROLTBL-TP15] - September, 2007

Note: the first two and the last three refer to one and the same standard. The current standard GPA-TP15 (2007) / API MPMS 11.2.5 extends the applicable range of the previous standard GPA TP-15 (1988) / API MPMS 11.2.2 Addendum 1994 while preserving the calculations and constants of the previous standard.

### Function input

| Function inputs          | Remark   | EU   | Range       | Default |
|--------------------------|--|------|-------------|---------|
| Name                     | Optional tag name, tag description and tag group   | -    | 0.3 .. 0.75 | 0       |
| Relative density at 60°F |  | °F   | -100..200   | 60      |
| Observed Temperature     |  | -    |             | 0       |
| API rounding             | 0: Disabled<br>Full precision (no rounding applied)<br>1: Enabled<br>Rounding as defined in ' GPA TP15:1988 / API MPMS 11.2.2 Addendum':1994   | -    |             | 0       |
| P100 Correlation         | 0: Disabled<br>The standard correlation is commonly used for pure products such as propane, butane and natural gasoline. It only requires the relative density and the temperature to calculate the vapor pressure<br>1: Enabled<br>The improved correlation requires the vapor pressure at 100°F (37.8 °C). This method is better suited for varied NGL mixes Where different product mixes could have the same specific gravity but different equilibrium pressures. | -    |             | 0       |
| Vapor pressure at 100°F  |  | psia | 0..500      | 0       |

### Function outputs

| Function outputs | Remark  | EU   | Fallback |
|------------------|---|------|----------|
| Status           | 0: Normal<br>1: Input argument out of range<br>2: Calculation error   |      |          |
| Vapor pressure   | Vapor pressure at 60°F  | psia | 0        |
| Range            | With respect to the 2007 standard the combination of relative density and temperature is:<br>0: In Range<br>1: Out of Range | -    | 0        |

### Calculations

The calculations are in either full or partial compliance with the standards, depending on the selected type of API rounding.

### Boundaries

The GPA TP-15:1988 / API MPMS 11.2.2 Addendum:1994 correlation method is valid for the following range.

- 0.490 to 0.676 (RD60)
- -50 to 140 °F

The GPA TP-15:2007 / API MPMS 11.2.5:2007 correlation method has been extended for lower density and is valid for the following ranges.

Lower range:

- 0.350 to 0.425 (RD60)
- -50 to (695.51\*RD60 - 155.51) °F

with RD60 being the relative density at 60°F

Higher range:

- 0.425 to 0.676 (relative density)
- -50 to 140 °F

## fxGPA2172\_C

### Description

This uses the procedure for calculating heating value, specific gravity and compressibility factor at **customary** (imperial) conditions from the compositional analysis of a natural gas mixture.

GPA2172 describes the calculation methods to determine the compositional properties based on the individual component values and it refers to the GPA Standard 2145 (GPA2145) standard for these individual component values.

The effect of water on the calculations is rather complicated and is accounted for with a simplified equation that is considered to be adequate for custody transfer applications.

Therefore compositional properties are calculated for the following gas compositions:

- Wet gas composition  
the water fraction of input 'Composition' is taken as the actual water fraction.
- Dry gas composition  
the water fraction is set to 0 and the composition is normalized to unity.
- Saturated gas composition  
the water fraction is set to the value when the gas is saturated with water and the composition is normalized to unity

GPA-2172 prescribes that the most recent edition of GPA2145 used for the individual component values. The function provides the option to use the values from a specific GPA2145 standard. In order to verify the function based on the examples of GPA2172 the function provides the option to GPA2145-89 (edition 1989) as well.

### Compliance

- GPA Standard 2172-96, Calculation of Gross Heating Value, Relative Density and Compressibility Factor for Natural Gas Mixtures from Compositional Analysis - 1996
- API MPMS 14.5
- ASTM D3588-98 (Reapproved 2003)
- GPA Standard 2145-89, Table of Physical Constants
- GPA Standard 2145-00, Table of Physical Constants
- GPA Standard 2145-03, Table of Physical Constants
- GPA Standard 2145-09, Table of Physical Constants
- GPA Standard 2145-16, Table of Physical Constants

### Function inputs

| Function inputs  | Remark   | EU      | SW tag     | Range | Default |
|------------------|--|---------|------------|-------|---------|
| Name             | Optional tag name, tag description and tag group   |         |            |       |         |
| Composition      | Standard composition as defined section 'Standard Gas Composition'   | mol/mol | COMP       | 0..1  | 0       |
| Edition          | Refers to the base conditions and the editions of the GPA2145 values.<br>Note that these base conditions are used for both the density and the heating value.<br>1: 60°F, 14.696 psia, GPA2145-89 (1989)<br>2: 60°F, 14.696 psia, GPA2145-00 (2000)<br>3: 60°F, 14.696 psia, GPA2145-03 (2003)<br>4: 60°F, 14.696 psia, GPA2145-09 (2009)<br>5: 60°F, 14.696 psia, GPA2145-16 (2016) | -       | EDITION    |       | 2       |
| neo-Pentane mode | Determines what to do when component neo-Pentane is larger than zero<br>1: Add to i-Pentane<br>2: Add to n-Pentane<br>3: Neglect   | -       | NEOC5_MODE |       | 1       |

### Function outputs

| Function outputs          | Remark   | EU        | SW tag      | Alarm                       | Fallback |
|---------------------------|--|-----------|-------------|-----------------------------|----------|
| Status                    | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: Composition error<br>Composition does not add up to 100% +/- 0.01%<br>In case of an error the output values will be set to the fallback values | -         | STS         | FIOOR<br>CALCERR<br>COMPERR |          |
| Gross Heating Value (Wet) |  | Btu/ft3   | VOLGHV_WET  |                             | 0        |
| Molar Mass (Wet)          |  | lbm/lbmol | MOLMASS_WET |                             | 0        |
| Molar Mass Ratio (Wet)    |  |           | ISG_WET     |                             | 0        |
| Relative Density (Wet)    | Based on the compressibility of <u>wet</u> air   | -         | RRD_WET     |                             | 0        |
| Compressibility (Wet)     |  | -         | Z_DWET      |                             | 0        |
| Gross Heating Value (Wet) |  | Btu/lbm   | MASGHV_WET  |                             | 0        |
| Net Heating Value (Wet)   |  | Btu/ft3   | VOLNHV_WET  |                             | 0        |
| Gross Heating Value (Dry) |  | Btu/ft3   | VOLGHV_DRY  |                             | 0        |
| Molar Mass (Dry)          |  | -         | MOLMASS_DRY |                             | 0        |
| Molar Mass Ratio (Dry)    |  | lbm/lbmol | ISG_DRY     |                             | 0        |
| Relative Density (Dry)    |  | -         | RRD_DRY     |                             | 0        |
| Compressibility (Dry)     |  | -         | Z_DRY       |                             | 0        |
| Gross Heating Value (Dry) |  | Btu/lbm   | MASGHV_DRY  |                             | 0        |
| Net Heating Value (Dry)   |  | Btu/ft3   | VOLNHV_DRY  |                             | 0        |

| Function outputs                | Remark  | EU        | SW tag      | Alarm | Fallback |
|---------------------------------|---|-----------|-------------|-------|----------|
| Gross Heating Value (Saturated) | The saturated Gross Heating Value is commonly used for custody transfer energy calculations | Btu/ft3   | VOLGHV_SAT  |       | 0        |
| Molar Mass (Saturated)          |   | lbm/lbmol | MOLMASS_SAT |       | 0        |
| Molar Mass Ratio (Saturated)    | Ideal specific gravity  | -         | ISG_SAT     |       | 0        |
| Relative Density (Saturated)    | Based on the compressibility of <u>saturated</u> air  | -         | RRD_SAT     |       | 0        |
| Compressibility (Saturated)     |   | -         | Z_SAT       |       | 0        |
| Gross Heating Value (Saturated) |   | Btu/lbm   | MASGHV_SAT  |       | 0        |
| Net Heating Value (Saturated)   |   | Btu/ft3   | VOLNHV_SAT  |       | 0        |

## Calculations

The calculations are as documented in the GPA-2172 standard using the GPA2145 table values. However the calculations are performed at full precision, so not with intermediate rounding as shown in the examples of the standard.

Please note that the function uses the input composition 'as is', so does not apply normalization to 1.

- When the water fraction input value is above the water fraction of the saturated gas then the function continues its calculations without any correction.
- GPA-2145 standard editions 2000 and 2003 do not specify properties for hydrogen, argon and carbon monoxide. The function processes these components like the other components but with all property values set to 0.

## Water vapour pressure

The saturated properties are dependent on the water vapour pressure water. GPA-2172 version 1996 states a slightly different value for the water vapour pressure than the 2009 and 2014 editions. Therefore the following values are used by this function.

| Edition       | Value [psia] | According to  |
|---------------|--------------|---------------|
| 1: GPA2145-89 | 0.25636      | GPA2172-96    |
| 2: GPA2145-00 | 0.25636      | GPA2172-96    |
| 3: GPA2145-03 | 0.25636      | GPA2172-96    |
| 4: GPA2145-09 | 0.2564       | GPA2172-09/14 |
| 5: GPA2145-16 | 0.2564       | GPA2172-09/14 |

## fxGPA2172\_M

### Description

This function uses the procedure for calculating heating value, specific gravity and compressibility factor at **metric** conditions from the compositional analysis of a natural gas mixture.

GPA2172 describes the calculation methods to determine the compositional properties based on the individual component values and it refers to the GPA Standard 2145 (GPA2145) standard for these individual component values.

The effect of water on the calculations is rather complicated and is accounted for with a simplified equation that is considered to be adequate for custody transfer applications.

Therefore compositional properties are calculated for the following gas compositions:

- Wet gas composition  
the water fraction of input 'Composition' is taken as the actual water fraction.
- Dry gas composition  
the water mole fraction of input 'Composition' is set to 0 and the composition is normalized to unity.
- Saturated gas composition  
the water fraction value of input 'Composition' is set to the water saturated mole fraction and the composition is normalized to unity

GPA-2172 prescribes that the most recent edition of GPA2145 used for the individual component values. The function provides the option to use the values from a specific GPA2145 standard.

### Compliance

- GPA Standard 2172-96, Calculation of Gross Heating Value, Relative Density and Compressibility Factor for Natural Gas Mixtures from Compositional Analysis - 1996
- API MPMS 14.5 (same as GPA2172-96)
- GPA Standard 2145-00, Table of Physical Constants
- GPA Standard 2145-03, Table of Physical Constants
- GPA Standard 2145-09, Table of Physical Constants
- GPA Standard 2145-16, Table of Physical Constants

### Function inputs

| Function inputs  | Remark  | EU      | SW tag     | Range | Default |
|------------------|---|---------|------------|-------|---------|
| Name             | Optional tag name, tag description and tag group  |         |            |       |         |
| Composition      | Standard composition as defined section 'Standard Gas Composition'.   | mol/mol | COMP       | 0..1  | 0       |
| Edition          | Refers to the base conditions and the editions of the GPA2145 values. Note that the same temperature value is used for the density and heating value.<br>1: 15°C, 1.01325 bar(a), GPA2145-00<br>2: 15°C, 1.01325 bar(a), GPA2145-03<br>3: 15°C, 1.01325 bar(a), GPA2145-09<br>4: 15°C, 1.01325 bar(a), GPA2145-16 | -       | EDITION    |       | 2<br>-  |
| neo-Pentane mode | Determines what to do when component neo-Pentane is larger than zero<br>1: Add to i-Pentane<br>2: Add to n-Pentane<br>3: Neglect  | -       | NEOC5_MODE |       | 1       |

### Function outputs

| Function outputs          | Remark   | EU      | SW tag      | Alarm                       | Fallback |
|---------------------------|--|---------|-------------|-----------------------------|----------|
| Status                    | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: Composition error<br>Composition does not add up to 100% +/- 0.01%<br>In case of an error the output values will be set to the fallback values | -       | STS         | FIOOR<br>CALCERR<br>COMPERR |          |
| Gross Heating Value (Wet) |  | MJ/m3   | VOLGHV_WET  |                             | 0        |
| Molar Mass (Wet)          |  | kg/kmol | MOLMASS_WET |                             | 0        |
| Molar Mass Ratio (Wet)    |  | -       | ISG_WET     |                             | 0        |
| Relative Density (Wet)    | Based on the compressibility of <u>wet</u> air   | -       | RRD_WET     |                             | 0        |
| Compressibility (Wet)     |  | -       | Z_DWET      |                             | 0        |
| Gross Heating Value (Dry) |  | MJ/kg   | MASGHV_WET  |                             | 0        |
| Net Heating Value (Wet)   |  | MJ/m3   | VOLNHV_WET  |                             | 0        |
| Gross Heating Value (Dry) |  | MJ/m3   | VOLGHV_DRY  |                             | 0        |
| Molar Mass (Dry)          |  | kg/kmol | MOLMASS_DRY |                             | 0        |
| Molar Mass Ratio (Dry)    |  | -       | ISG_DRY     |                             | 0        |
| Relative Density (Dry)    |  | -       | RRD_DRY     |                             | 0        |
| Compressibility (Dry)     |  | -       | Z_DRY       |                             | 0        |
| Gross Heating Value (Dry) |  | MJ/kg   | MASGHV_DRY  |                             | 0        |
| Net Heating Value (Dry)   |  | MJ/m3   | VOLNHV_DRY  |                             | 0        |

| Function outputs                | Remark  | EU                | SW tag      | Alarm | Fallback |
|---------------------------------|---|-------------------|-------------|-------|----------|
| Gross Heating Value (Saturated) | The saturated Gross Heating Value is commonly used for custody transfer energy calculations | MJ/m <sup>3</sup> | VOLGHV_SAT  |       | 0        |
| Molar Mass (Saturated)          |   | kg/kmol           | MOLMASS_SAT |       | 0        |
| Molar Mass Ratio (Saturated)    | Ideal specific gravity  | -                 | ISG_SAT     |       | 0        |
| Relative Density (Saturated)    | Based on the compressibility of <u>saturated</u> air  | -                 | RRD_SAT     |       | 0        |
| Compressibility (Saturated)     |   | -                 | Z_SAT       |       | 0        |
| Gross Heating Value (Saturated) |   | MJ/kg             | MASGHV_SAT  |       | 0        |
| Net Heating Value (Saturated)   |   | MJ/m <sup>3</sup> | VOLNHV_SAT  |       | 0        |

### Calculations

The calculations are as documented in the GPA-2172 standard using the GPA2145 table values. However the calculations are performed at full precision, so not with intermediate rounding as shown in the examples of the standard.

Please note that the function uses the input composition 'as is', so does not apply normalization to 1.

- When the water fraction input value is above the water fraction of the saturated gas then the function continues its calculations without any correction.
- GPA-2145 standard editions 2000 and 2003 do not specify properties for hydrogen, argon and carbon monoxide. The function processes these components like the other components but with all property values set to 0.




## fxIAPWS\_IF97\_C

### Description

The function calculates the density and enthalpy of steam and water according to IAPWS-IF97 in **US Customary units**.

IAPWS-IF97 defines calculations for 5 regions as shown in the picture below.

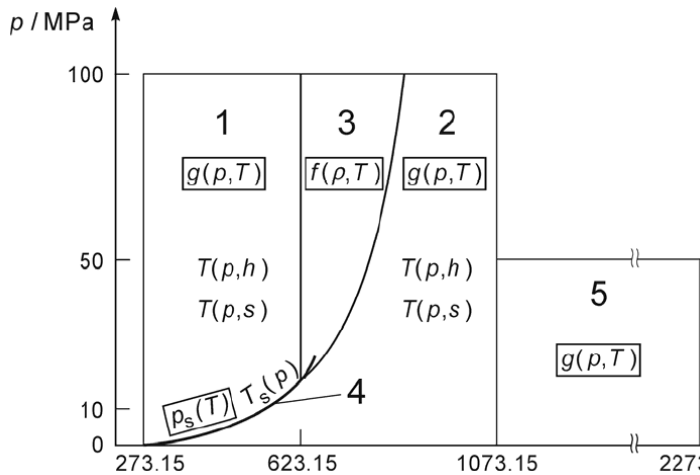

Region 1: Water

Region 2: Superheated steam

Region 3: Water

Region 4: Saturation line (saturated steam / water)

Region 5: Superheated steam

### Function inputs

| Function inputs | Remark  | EU   | Range     | Default |
|-----------------|---|------|-----------|---------|
| Name            | Optional tag name, tag description and tag group  |      |           |         |
| Temperature     |   | °F   | 0 .. 4000 | 0       |
| Pressure        |   | psia | 0..15000  | 0       |
| Phase           | The phase (water or steam) can be calculated automatically or be set to either steam or water.  |      |           |         |
|                 | 1: Auto-select (calculate from t and p inputs)  |      |           |         |
|                 | 2: Steam  |      |           |         |
|                 | 3: Water  |      |           |         |
|                 | If 'Steam' or 'Water' is selected, while the combination of temperature and pressure indicates the opposite phase, then the function uses either the saturation pressure (region 4) or the boundary pressure (intersection regions 2 and 3) instead of the input pressure for its calculations. |      |           |         |

### Function outputs

| Function outputs    | Remark  | EU       | Fallback |
|---------------------|---|----------|----------|
| Status              | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence  |          |          |
| Density             |   | lbm/ft3  | 0        |
| Enthalpy            | Energy flow = Mass flow * Enthalpy  | btu/lbm  | 0        |
| Region              | Actual IAPWS-IF97 region<br>0: Combination of t and p is outside the valid range<br>1: Water<br>2: Steam<br>3: Pressurized water<br>4: At the saturation line<br>5: High temperature steam (1472 ≤ T ≤ 3632 °F) | -        | 0        |
| Saturation pressure | Saturation pressure at the input temperature.<br>Note: only calculated up to the critical temperature of 647.096 K (+/- 705 °F), set to 0 for higher temperatures   | psia     | 0        |
| Dynamic viscosity   | The dynamic viscosity is required for flow rate calculations based on a differential  | lbm/ft.s | 0        |

### References

- Revised Release on the IAPWS Industrial Formulation 1997 for the Thermodynamic Properties of Water and Steam, August 2007.

### Boundaries

The IAPWS Industrial Formulation 1997 consists of a set of equations for different regions which cover the following range of validity:

- 32 ≤ T ≤ 1472 °F      p ≤ 14500 psia
- 1472 ≤ T ≤ 3632 °F      p ≤ 7250 psia

| Function outputs        | Remark  | EU | Fallback |
|-------------------------|---|----|----------|
| Ratio of specific heats | pressure measurement (e.g. orifice)   |    |          |
|                         | Equals the ratio of the specific heats $c_p / c_v$  | -  | 0        |
|                         | $c_p$ : specific heat at constant pressure  |    |          |
|                         | $c_v$ : specific heat at constant volume  |    |          |
|                         | This ratio can be used as the isentropic exponent value (also called 'kappa') when the real value is unknown.<br>The isentropic exponent is required for flow rate calculations based on a differential pressure measurement (e.g. orifice) |    |          |

## Calculations

The calculations are in compliance with the standard.

For regions 1, 2 and 5 the density can be calculated directly from the temperature in pressure. For region 3 an iterative calculation is required because the Equation Of State for this region calculates the pressure from a known temperature and density iteration. A convergence limit of 0.00001 kg/m<sup>3</sup> (+- 0.000006 lbm/ft<sup>3</sup>) is applied. A maximum of 20 iterations is applied.


The other properties can be calculated directly from the temperature and pressure for all regions.

## fxIAPWS\_IF97\_M

### Description

The function calculates the density and enthalpy of steam and water according to IAPWS-IF97 in **Metric units**.

IAPWS-IF97 defines calculations for 5 regions as shown in the picture below.

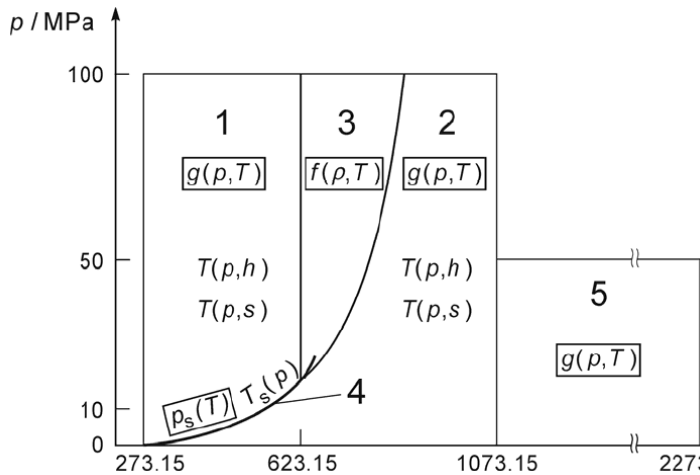

Region 1: Water

Region 2: Superheated steam

Region 3: Water

Region 4: Saturation line (saturated steam / water)

Region 5: Superheated steam

### Function inputs

| Function inputs | Remark  | EU     | Range       | Default |
|-----------------|---|--------|-------------|---------|
| Name            | Optional tag name, tag description and tag group  |        |             |         |
| Temperature     |   | °C     | -50 .. 2200 | 0       |
| Pressure        |   | bar(a) | 0..1100     | 0       |
| Phase           | The phase (water or steam) can be calculated automatically or be set to either steam or water.<br>1: Auto-select (calculate from t and p inputs)<br>2: Steam<br>3: Water<br>If 'Steam' or 'Water' is selected, while the combination of temperature and pressure indicates the opposite phase, then the function uses either the saturation pressure (region 4) or the boundary pressure (intersection regions 2 and 3) instead of the input pressure for its calculations. |        |             |         |

### Function outputs

| Function outputs        | Remark   | EU       | Fallback |
|-------------------------|--|----------|----------|
| Status                  | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence   |          |          |
| Density                 |  | kg/m3    | 0        |
| Enthalpy                | Energy flow = Mass flow * Enthalpy   | MJ/kg    | 0        |
| Region                  | Actual IAPWS-IF97 region<br>0: Combination of t and p is outside the valid range<br>1: Water<br>2: Steam<br>3: Pressurized water<br>4: At the saturation line<br>5: High temperature steam (800 ≤ T ≤ 2000 °C) | -        | 0        |
| Saturation pressure     | Saturation pressure at the input temperature<br>Note: only calculated up to the critical temperature of 647.096 K (+- 374 °C), set to 0 for higher temperatures  | bar(a)   | 0        |
| Dynamic viscosity       | The dynamic viscosity is required for flow rate calculations based on a differential pressure measurement (e.g. orifice)   | lbm/ft.s | 0        |
| Ratio of specific heats | Equals the ratio of the specific heats cp / cv   | -        | 0        |

### References

- Revised Release on the IAPWS Industrial Formulation 1997 for the Thermodynamic Properties of Water and Steam, August 2007.

### Boundaries

The IAPWS Industrial Formulation 1997 consists of a set of equations for different regions which cover the following range of validity:

- 0 ≤ T ≤ 800 °C      p ≤ 1000 bar(a)
- 800 ≤ T ≤ 2000 °C      p ≤ 500 bar(a)

| Function outputs | Remark  | EU | Fallback |
|------------------|---|----|----------|
|                  | cp : specific heat at constant pressure<br>cv : specific heat at constant volume<br><br>This ratio can be used as the isentropic exponent value (also called 'kappa') when the real value is unknown.<br>The isentropic exponent is required for flow rate calculations based on a differential pressure measurement (e.g. orifice) |    |          |

### Calculations

The calculations are in compliance with the standard.

For regions 1, 2 and 5 the density can be calculated directly from the temperature in pressure. For region 3 an iterative calculation is required because the Equation Of State for this region calculates the pressure from a known temperature and density iteration. A convergence limit of 0.00001 kg/m<sup>3</sup> is applied. A maximum of 20 iterations is applied.

The enthalpy can be calculated directly from the temperature and pressure for all regions.

## fxInterpolationCurve

### Description

This function calculates the output value from a set of reference points and the actual input value. The function can take an arbitrary number of reference points.

The function is typically used for applying a calibration curve to a K factor or a meter factor (liquid) or a meter error curve (gas).

Besides of the 1st calibration point (which is always used) the function will only use the calibration points (starting from the 2nd point) for which the x value is greater than the previous x value. All further points will be ignored.

### Function inputs

| Function inputs    | Remark   | EU | SW tag  | Range | Default |
|--------------------|--|----|---------|-------|---------|
| Name               | Optional tag name, tag description and tag group   |    |         |       |         |
| Input value        | Reference to the cell containing the actual input value (e.g. flow rate or pulse frequency)  |    |         |       |         |
| Reference values   | Array of reference values, assuming the following sequence:<br>Point 1 - Input value<br>Point 1 - Output value<br>Point 2 - Input value<br>Point 2 - Output value<br>etc....<br><br>The array must contain an even number of values with the input values in ascending order.<br>So it is required that Input 1 < Input 2 < Input 3 etc.<br>However, when an input value equals 0, then the function will not use this point and all subsequent points of the array. |    | REFVAL  |       |         |
| Extrapolation mode | Determines whether or not extrapolation must be applied when the input value is outside the linearization curve. When disabled either the first or last output value will be used.<br>0: Disabled<br>1: Enabled  |    | EXPMODE |       |         |

### Function outputs

| Function outputs | Remark   | EU                                 | SW tag | Alarm | Fallback |
|------------------|--|------------------------------------|--------|-------|----------|
| Output value     | Interpolated value   | Same as input 'Output reference 1' | VAL    |       | 0        |
| Date/time        | Latest modification date and time of the any of the reference point values |                                    | DTTM   |       |          |
| Out of range     | Input value is outside the range that is covered by the reference values   |                                    |        | OOR   |          |

### Calculations

$$y = (x - In_L) \cdot \frac{Out_H - Out_L}{In_H - In_L} + Out_L$$

Where:

|                  |  |
|------------------|--|
| x                | Input value  |
| y                | Interpolated value   |
| In <sub>L</sub>  | Closest input reference value that is smaller than the input value |
| In <sub>H</sub>  | Closest input reference value that is larger than the input value  |
| Out <sub>L</sub> | Output reference value that corresponds with In <sub>L</sub>       |
| Out <sub>H</sub> | Output reference value that corresponds with In <sub>H</sub>       |

## fxISO5167\_ISA1932Nozzle

### Description

The function calculates the mass flow rate for **ISA1932 Nozzle** pressure differential flow devices according to the ISO-5167 standard.

### Compliance

- ISO-5167 - 1991 Measurement of fluid flow by means of pressure differential devices, 1st edition, 1991
- ISO-5167 Amd.1 : 1998(E)
- ISO-5167 - 2003 Measurement of fluid flow by means of pressure differential devices inserted in circular cross-section conduits running full, 2nd edition, 2003

### Function inputs

| Function inputs                      | Remark   | EU          | Range | Default   |
|--------------------------------------|--|-------------|-------|-----------|
| Name                                 | Optional tag name, tag description and tag group   |             |       |           |
| Differential Pressure                | Differential pressure over the primary flow device measured at the up- and downstream pressure tapings, which need to be in the positions as specified in the standard   | mbar        |       | 0         |
| Pressure                             | Upstream pressure value of the fluid at metering conditions  | bar(a)      |       | 0         |
| Temperature                          | Down- or upstream temperature of the fluid at metering conditions  | °C          |       | 0         |
| Density                              | Down or upstream density of the fluid at metering conditions   | kg/m3       |       | 0         |
| Dynamic Viscosity                    | Dynamic viscosity of the fluid   | Pa.s        |       | 0         |
| Isentropic Exponent                  | Also referred to as $\kappa$ (kappa). For an ideal gas this coefficient is equal to the ratio of the specific heat capacity at constant pressure to the specific heat at constant volume. According to the ISO standard this ratio may be used, when the real value is unknown.  |             |       | 0         |
| Pipe Diameter                        | Internal diameter of the pipe at reference temperature   | mm          |       | 0         |
| Pipe Expansion factor                | The thermal expansion coefficient of the pipe material   | 1/°C        |       | 0.0000108 |
| Pipe Reference temperature           | The reference temperature that corresponds to the 'Pipe diameter' input value  | °C          |       | 20        |
| ISA1932 Nozzle Diameter              | ISA1932 Nozzle diameter at reference temperature   | mm          |       | 0         |
| ISA1932 Nozzle Expansion factor      | The thermal expansion coefficient of the ISA1932 Nozzle material   | 1/°C        |       | 0.0000163 |
| ISA1932 Nozzle Reference Temperature | The reference temperature that corresponds to the 'ISA1932 Nozzle diameter' input value  | °C          |       | 20        |
| Pressure Location                    | 1: Upstream<br>Input 'Pressure' represents the pressure at the upstream pressure tapping ( $p_1$ ).<br>Since the absolute pressure is usually measured at the upstream tapping this is the most common setting.<br>2: Downstream<br>Input 'Pressure' represents the pressure at the downstream tapping ( $p_2$ ).  | -           |       | 1         |
| Temperature Location                 | 1: Upstream<br>Input 'Temperature' represents the upstream temperature ( $t_1$ ).<br>2: Downstream<br>Input 'Temperature' represents the temperature at the downstream tapping ( $t_2$ ).<br>3: Recovered<br>Input 'Temperature' represents the downstream temperature at a location Where the pressure has fully recovered ( $t_3$ ).<br>Since temperature measurement is usually downstream of the flow device this is the most common setting.  | -           |       | 2         |
| Temperature Correction               | This parameter specifies how the temperature should be corrected from downstream to upstream conditions (or vice versa)<br>1: $(1-\kappa)/\kappa$<br>Isentropic expansion using $(1-\kappa)/\kappa$ as the temperature referral exponent<br>2: Constant<br>Isentropic expansion using input 'Temperature Exponent' as the temperature referral exponent [-].<br>Please note that this value must be < 0<br>3: Joule Thomson<br>Isenthalpic expansion using input 'Temperature Exponent' as the Joule Thomson coefficient [°C/bar].<br>This method is prescribed by ISO5167-1:2003. |             |       | 3         |
| Temperature Exponent                 | Refer to input Temperature Correction<br>Unit depends on input Temperature Correction value  | -<br>°C/bar |       | 0         |
| Density Location                     | This parameter specifies if and how the density should be corrected from downstream to upstream conditions (or vice versa).<br>1: Upstream<br>Input 'Density' represents the density at the upstream pressure tapping ( $\rho_1$ ).<br>2: Downstream<br>Input 'Density' represents the density at the downstream tapping ( $\rho_2$ ).<br>3: Recovered<br>Input 'Density' represents the density downstream at a location Where the pressure has fully recovered ( $\rho_3$ ).   | -           |       | 1         |
| Density Exponent.                    | This factor is used when density correction is enabled. The formula $1/\kappa$ will be used when the input value is set to 0, else the input value will be used.<br>For more details refer to section 'Density correction'.  | -           |       | 0         |
| Fluid                                | The type of fluid being measured<br>1: Gas   | -           |       | 1         |

| Function inputs | Remark  | EU | Range | Default |
|-----------------|---|----|-------|---------|
| Year Of Edition | 2: Liquid   |    |       |         |
|                 | 1: Edition 1991   | -  |       | 3       |
|                 | 2: Edition 1998   |    |       |         |
|                 | 3: Edition 2003   |    |       |         |
|                 | Only used for calculation of pressure loss, with options 1 and 2 giving the same result |    |       |         |

## Function outputs

| Function outputs                  | Remark  | EU      |
|-----------------------------------|---|---------|
| Status                            | 0: Normal (No error condition)<br>1: Input argument out of range<br>2: No convergence   | -       |
| Mass flow rate                    | The calculated mass flow rate   | tonne/h |
| Beta ratio                        | Nozzle to pipe ratio at upstream temperature  | -       |
| Nozzle diameter                   | At the upstream temperature   | mm      |
| Pipe diameter                     | At the upstream temperature   | mm      |
| Upstream pressure                 | Pressure at upstream tapping ( $p_1$ )  | bar(a)  |
| Pressure at downstream tapping    | Pressure at downstream tapping ( $p_2$ )  | bar(a)  |
| Recovered downstream pressure     | Fully recovered downstream pressure ( $p_3$ )   | bar(a)  |
| Upstream temperature              | Temperature at upstream tapping ( $t_1$ )   | °C      |
| Temperature at downstream tapping | Temperature at downstream tapping ( $t_2$ )   | °C      |
| Downstream Temperature            | 'Fully recovered' downstream temperature ( $t_3$ )  | °C      |
| Upstream density                  | Density at upstream tapping ( $\rho_1$ )  | kg/m3   |
| Density at downstream tapping     | Pressure at downstream tapping ( $\rho_2$ )   | kg/m3   |
| Downstream density                | 'Fully recovered' downstream density ( $\rho_3$ )   | kg/m3   |
| Reynolds number                   | The pipe Reynolds number (this is the Reynolds number upstream of the ISA1932 Nozzle and not the one within the device throat itself) | -       |
| Discharge coefficient             |   | -       |
| Expansion Factor                  |   | -       |
| Velocity of Approach              |   |         |
| Pressure Range                    | 0: Pressure is in valid range<br>1: Pressure is out of valid range  | -       |
| Reynolds Range                    | 0: Reynolds number is in valid range<br>1: Reynolds number is out of valid range  | -       |
| Diameter Range                    | 0: Device and pipe diameter and Beta ratio in valid range<br>1: Device diameter, pipe diameter and/or Beta ratio out of valid range   | -       |

## fxISO5167\_LongRadiusNozzle

### Description

The function calculates the mass flow rate for **Long Radius Nozzle** pressure differential flow devices according to the ISO-5167 standard.

### Compliance

ISO-5167 - 1991 Measurement of fluid flow by means of pressure differential devices, 1st edition, 1991  
 ISO-5167 Amd.1 : 1998(E)  
 ISO-5167 - 2003 Measurement of fluid flow by means of pressure differential devices inserted in circular cross-section conduits running full, 2nd edition, 2003

### Function inputs

| Function inputs                          | Remark   | EU          | Range | Default   |
|--|--|-------------|-------|-----------|
| Name                                     | Optional tag name, tag description and tag group   |             |       |           |
| Differential Pressure                    | Differential pressure over the primary flow device measured at the up- and downstream pressure tapings, which need to be in the positions as specified in the standard   | mbar        |       | 0         |
| Pressure                                 | Upstream pressure value of the fluid at metering conditions  | bar(a)      |       | 0         |
| Temperature                              | Down- or upstream temperature of the fluid at metering conditions  | °C          |       | 0         |
| Density                                  | Down or upstream density of the fluid at metering conditions   | kg/m3       |       | 0         |
| Dynamic Viscosity                        | Dynamic viscosity of the fluid   | Pa.s        |       | 0         |
| Isentropic Exponent                      | Also referred to as $\kappa$ (kappa). For an ideal gas this coefficient is equal to the ratio of the specific heat capacity at constant pressure to the specific heat at constant volume. According to the ISO standard this ratio may be used, when the real value is unknown.  | -           |       | 0         |
| Pipe Diameter                            | Internal diameter of the pipe at reference temperature   | mm          |       | 0         |
| Pipe Expansion factor                    | The thermal expansion coefficient of the pipe material   | 1/°C        |       | 0.0000108 |
| Pipe Reference temperature               | The reference temperature that corresponds to the 'Pipe diameter' input value  | °C          |       | 20        |
| Long Radius Nozzle Diameter              | Long Radius Nozzle diameter at reference temperature   | mm          |       | 0         |
| Long Radius Nozzle Expansion factor      | The thermal expansion coefficient of the Long Radius Nozzle material   | 1/°C        |       | 0.0000163 |
| Long Radius Nozzle Reference Temperature | The reference temperature that corresponds to the 'Long Radius Nozzle diameter' input value  | °C          |       | 20        |
| Pressure Location                        | 1: Upstream<br>Input 'Pressure' represents the pressure at the upstream pressure tapping ( $p_1$ ). Since the absolute pressure is usually measured at the upstream tapping this is the most common setting.<br>2: Downstream<br>Input 'Pressure' represents the pressure at the downstream tapping ( $p_2$ ).   | -           |       | 1         |
| Temperature Location                     | 1: Upstream<br>Input 'Temperature' represents the upstream temperature ( $t_1$ ).<br>2: Downstream<br>Input 'Temperature' represents the temperature at the downstream tapping ( $t_2$ ).<br>3: Recovered<br>Input 'Temperature' represents the downstream temperature at a location Where the pressure has fully recovered ( $t_3$ ). Since temperature measurement is usually downstream of the flow device this is the most common setting.   | -           |       | 2         |
| Temperature Correction                   | This parameter specifies how the temperature should be corrected from downstream to upstream conditions (or vice versa)<br>1: $(1-\kappa)/\kappa$<br>Isentropic expansion using $(1-\kappa)/\kappa$ as the temperature referral exponent<br>2: Constant<br>Isentropic expansion using input 'Temperature Exponent' as the temperature referral exponent [-]. Please note that this value must be < 0<br>3: Joule Thomson<br>Isenthalpic expansion using input 'Temperature Exponent' as the Joule Thomson coefficient [°C/bar]. This method is prescribed by ISO5167-1:2003. |             |       | 3         |
| Temperature Exponent                     | Refer to input Temperature Correction<br>Unit depends on input Temperature Correction value  | -<br>°C/bar |       | 0         |
| Density Location                         | This parameter specifies if and how the density should be corrected from downstream to upstream conditions (or vice versa).<br>1: Upstream<br>Input 'Density' represents the density at the upstream pressure tapping ( $\rho_1$ ).<br>2: Downstream<br>Input 'Density' represents the density at the downstream tapping ( $\rho_2$ ).<br>3: Recovered<br>Input 'Density' represents the density downstream at a location Where the pressure has fully recovered ( $\rho_3$ ).   | -           |       | 1         |
| Density Exponent.                        | This factor is used when density correction is enabled. The formula $1/\kappa$ will be used when the input value is set to 0, else the input value will be used.   | -           |       | 0         |



| Function inputs | Remark   | EU | Range | Default |
|-----------------|--|----|-------|---------|
|                 | For more details refer to section 'Density correction'.  |    |       |         |
| Fluid           | The type of fluid being measured<br>1: Gas<br>2: Liquid  | -  |       | 1       |
| Year Of Edition | 1: Edition 1991<br>2: Edition 1998<br>3: Edition 2003<br>Only used for calculation of pressure loss, with options 1 and 2 giving the same result | -  |       | 3       |

### Function outputs

| Function outputs                  | Remark  | EU      |
|-----------------------------------|---|---------|
| Status                            | 0: Normal (No error condition)<br>1: Input argument out of range<br>2: No convergence   | -       |
| Mass flow rate                    | The calculated mass flow rate   | tonne/h |
| Beta ratio                        | Nozzle to pipe ratio at upstream temperature  |         |
| Nozzle diameter                   | At the upstream temperature   |         |
| Pipe diameter                     | At the upstream temperature   |         |
| Upstream pressure                 | Pressure at upstream tapping ( $p_1$ )  | bar(a)  |
| Pressure at downstream tapping    | Pressure at downstream tapping ( $p_2$ )  | bar(a)  |
| Recovered downstream pressure     | Fully recovered downstream pressure ( $p_3$ )   | bar(a)  |
| Upstream temperature              | Temperature at upstream tapping ( $t_1$ )   | °C      |
| Temperature at downstream tapping | Temperature at downstream tapping ( $t_2$ )   | °C      |
| Downstream Temperature            | 'Fully recovered' downstream temperature ( $t_3$ )  | °C      |
| Upstream density                  | Density at upstream tapping ( $\rho_1$ )  | kg/m3   |
| Density at downstream tapping     | Pressure at downstream tapping ( $p_2$ )  | kg/m3   |
| Downstream density                | 'Fully recovered' downstream density ( $\rho_3$ )   | kg/m3   |
| Reynolds number                   | The pipe Reynolds number (this is the Reynolds number upstream of the Long Radius Nozzle and not the one within the device throat itself) | -       |
| Discharge coefficient             |   | -       |
| Expansion Factor                  |   | -       |
| Velocity of Approach              |   |         |
| Pressure Range                    | 0: Pressure is in valid range<br>1: Pressure is out of valid range  | -       |
| Reynolds Range                    | 0: Reynolds number is in valid range<br>1: Reynolds number is out of valid range  | -       |
| Diameter Range                    | 0: Device and pipe diameter and Beta ratio in valid range<br>1: Device diameter, pipe diameter and/or Beta ratio out of valid range       | -       |

## fxISO5167\_Orifice

### Description

The function calculates the mass flow rate for **Orifice** pressure differential flow devices according to the ISO-5167 standard and the ISO/TR 15377 technical report.

Orifices plates with the following type of pressure tapplings are supported by this function:


- ISO5167 Square-edged orifice with corner tapplings
- ISO5167 Square-edged orifice with flange tapplings
- ISO5167 Square-edged orifice with D and D/2 tapplings
- ISO/TR 15377 Quarter circle orifice with corner tapplings
- ISO/TR 15377 Quarter circle orifice with flange tapplings
- ISO/TR 15377 Conical entrance orifice with corner tapplings

### References

- ISO 5167 - Measurement of fluid flow by means of pressure differential devices, 1991
- ISO 5167 - Measurement of fluid flow by means of pressure differential devices, 1991
- Amendment 1 1998
- ISO 5167 - Measurement of fluid flow by means of pressure differential devices, 2003
- British standard 1042: Part 1: 1964
- ISO/TR 15377:2007 Measurement of fluid flow by means of pressure differential devices – Guidelines for the specification of orifice plates, nozzle and Venturi tubes beyond the scope of ISO 5167

### Function inputs

| Function inputs               | Remark  | EU                | Range      | Default   |
|-------------------------------|---|-------------------|------------|-----------|
| Name                          | Optional tag name, tag description and tag group  |                   |            |           |
| Differential Pressure         | Differential pressure over the primary flow device measured at the up- and downstream pressure tapplings, which need to be in the positions as specified in the standard  | mbar              | 0..10000   | 0         |
| Pressure                      | Down- or upstream pressure value ( $p_1$ ) of the fluid at metering conditions  | bar (a)           | 0..2000    | 0         |
| Temperature                   | Down- or upstream temperature of the fluid at metering conditions   | °C                | -240..1000 | 0         |
| Density                       | Down or upstream density of the fluid at metering conditions  | kg/m <sup>3</sup> | 0..2000    | 0         |
| Dynamic Viscosity             | Dynamic viscosity of the fluid  | Pa.s              | 0..1       | 0         |
| Isentropic Exponent           | Also referred to as $\kappa$ (kappa). For an ideal gas this coefficient is equal to the ratio of the specific heat capacity at constant pressure to the specific heat at constant volume. According to the ISO standard this ratio may be used, when the real value is unknown.   | -                 | 0..10      | 0         |
| Pipe Diameter                 | Internal diameter of the pipe at reference temperature  | mm                | 0..2000    | 0         |
| Pipe Expansion factor         | The thermal expansion coefficient of the pipe material  | 1/°C              | 0..1       | 0.0000108 |
| Pipe Reference temperature    | The reference temperature that corresponds to the 'Pipe diameter' input value   | °C                | -300..1000 | 20        |
| Orifice Diameter              | Orifice diameter at reference temperature   | mm                | 0..2000    | 0         |
| Orifice Expansion factor      | The thermal expansion coefficient of the orifice material   | 1/°C              | 0..1       | 0.0000163 |
| Orifice Reference Temperature | The reference temperature that corresponds to the 'Orifice diameter' input value  | °C                | -300..1000 | 20        |
| Configuration                 | The location of the pressure tapplings. Several configurations are permitted by the ISO5167 standard. Each configuration has a different calculation of the discharge coefficient and of the expansion factor<br>1: ISO5167 Corner<br>2: ISO5167 D and D/2<br>3: ISO5167 Flange<br>4: ISO15377 Quarter circle (*)<br>5: ISO15377 Conical entrance<br>(*) The calculation of the discharge and expansion factor are equal for the quarter circle orifice with corner and flange tapplings. | -                 |            | 2         |

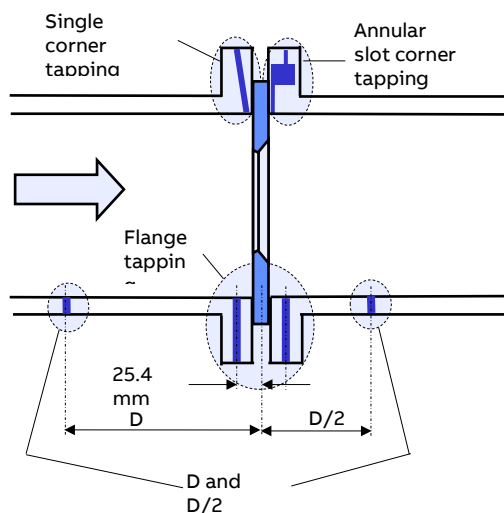

| Function inputs        | Remark  | EU                                 | Range | Default |
|------------------------|---|------------------------------------|-------|---------|
| Pressure Location      | 1: Upstream<br>Input 'Pressure' represents the pressure at the upstream pressure tapping ( $p_1$ ).<br>Since the absolute pressure is usually measured at the upstream tapping this is the most common setting.<br>2: Downstream<br>Input 'Pressure' represents the pressure at the downstream tapping ( $p_2$ ).   | -                                  |       | 1       |
| Temperature Location   | 1: Upstream<br>Input 'Temperature' represents the upstream temperature ( $t_1$ ).<br>2: Downstream<br>Input 'Temperature' represents the temperature at the downstream tapping ( $t_2$ ).<br>3: Recovered<br>Input 'Temperature' represents the downstream temperature at a location Where the pressure has fully recovered ( $t_3$ ).<br>Since temperature measurement is usually downstream of the flow device this is the most common setting.   | -                                  |       | 2       |
| Temperature Correction | This parameter specifies how the temperature should be corrected from downstream to upstream conditions (or vice versa)<br>1: $(1-\kappa)/\kappa$<br>Isentropic expansion using $(1-\kappa)/\kappa$ as the temperature referral exponent<br>2: Constant<br>Isentropic expansion using input 'Temperature Exponent' as the temperature referral exponent [-].<br>Please note that this value must be $< 0$<br>3: Joule Thomson<br>Isenthalpic expansion using input 'Temperature Exponent' as the Joule Thomson coefficient [ $^{\circ}\text{C}/\text{bar}$ ].<br>This method is prescribed by ISO5167-1:2003. |                                    |       | 3       |
| Temperature Exponent   | Refer to input Temperature Correction<br>Unit depends on input Temperature Correction value   | -<br>$^{\circ}\text{C}/\text{bar}$ |       | 0       |
| Density Location       | This parameter specifies if and how the density should be corrected from downstream to upstream conditions (or vice versa).<br>1: Upstream<br>Input 'Density' represents the density at the upstream pressure tapping ( $\rho_1$ ).<br>2: Downstream<br>Input 'Density' represents the density at the downstream tapping ( $\rho_2$ ).<br>3: Recovered<br>Input 'Density' represents the density downstream at a location Where the pressure has fully recovered ( $\rho_3$ ).  | -                                  |       | 1       |
| Density Exponent.      | This factor is used when density correction is enabled. The formula $1/\kappa$ will be used when the input value is set to 0, else the input value will be used.<br>For more details refer to section 'Density correction'.   | -                                  |       | 0       |
| Fluid                  | The type of fluid being measured<br>1: Gas<br>2: Liquid   | -                                  |       | 1       |
| Year Of Edition        | 1: Edition 1991<br>2: Edition 1998<br>3: Edition 2003<br>Note: Only applicable for ISO5167. ISO/TR15377 refers to ISO5167:2003.   | -                                  |       | 3       |
| Drain hole             | When input value is $> 0$ then an additional correction on the orifice diameter will be applied to account for the drain hole, as explained further on.   | mm                                 |       | 0       |

## Function outputs

| Function outputs                  | Remark   | EU                 | Fallback |
|-----------------------------------|--|--------------------|----------|
| Status                            | 0: Normal (No error condition)<br>1: Input argument out of range<br>2: No convergence  |                    |          |
| Mass flow rate                    | The calculated mass flow rate  | kg/s               | 0        |
| Beta ratio                        | Orifice to pipe diameter ratio at upstream temperature   | -                  | 0        |
| Orifice diameter                  | At the upstream temperature and optionally with a correction for the drain hole  | mm                 | 0        |
| Pipe diameter                     | At the upstream temperature  | mm                 | 0        |
| Upstream pressure                 | Pressure at upstream tapping ( $p_1$ )   | bar(a)             | 0        |
| Pressure at downstream tapping    | Pressure at downstream tapping ( $p_2$ )   | bar(a)             | 0        |
| Recovered downstream pressure     | Fully recovered downstream pressure ( $p_3$ )  | bar(a)             | 0        |
| Upstream temperature              | Temperature at upstream tapping ( $t_1$ )  | $^{\circ}\text{C}$ | 0        |
| Temperature at downstream tapping | Temperature at downstream tapping ( $t_2$ )  | $^{\circ}\text{C}$ | 0        |
| Downstream Temperature            | 'Fully recovered' downstream temperature ( $t_3$ )   | $^{\circ}\text{C}$ | 0        |
| Upstream density                  | Density at upstream tapping ( $\rho_1$ )   | kg/m3              | 0        |
| Density at downstream tapping     | Pressure at downstream tapping ( $p_2$ )   | kg/m3              | 0        |
| Downstream density                | 'Fully recovered' downstream density ( $\rho_3$ )  | kg/m3              | 0        |
| Reynolds number                   | The pipe Reynolds number (this is the Reynolds number upstream of the orifice and not the one within the device throat itself) | -                  | 0        |

| Function outputs      | Remark  | EU | Fallback |
|-----------------------|---|----|----------|
| Discharge coefficient |   | -  | 0        |
| Expansion Factor      |   | -  | 0        |
| Velocity of Approach  |   | -  | 0        |
| Pressure Range        | 0: Pressure is in valid range<br>1: Pressure is out of valid range  | -  | 0        |
| Reynolds Range        | 0: Reynolds number is in valid range<br>1: Reynolds number is out of valid range  | -  | 0        |
| Diameter Range        | 0: Device and pipe diameter and Beta ratio in valid range<br>1: Device diameter, pipe diameter and/or Beta ratio out of valid range | -  | 0        |

### Pressure correction

The relation between the pressure at the upstream tapping  $p_1$  and the pressure at the downstream tapping ( $p_2$ ) is as following:

$$p_2 = p_1 - \Delta p / 1000$$

The relation between the pressure at the upstream tapping and the fully recovered pressure ( $p_3$ ) is as following:

$$p_3 = p_1 - p_{LOSS}$$

The calculation of  $P_{LOSS}$  is as defined in the standard.

Where:

|              |                                     |          |
|--------------|-------------------------------------|----------|
| <b>p1</b>    | Pressure at upstream tapping        | [bar(a)] |
| <b>p2</b>    | Pressure at downstream tapping      | [bar(a)] |
| <b>p3</b>    | Fully recovered downstream pressure | [bar(a)] |
| <b>Δp</b>    | Differential pressure               | [mbar]   |
| <b>pLOSS</b> | Pressure loss over the meter        | [bar]    |

### Temperature correction

When input 'Temperature correction' is set to 1, then an isentropic expansion based on the isentropic coefficient is applied:

$$t_2 = (t_3 + 273.15) \cdot \left( \frac{p_3}{p_2} \right)^{\frac{1-\kappa}{\kappa}} - 273.15$$

$$t_1 = (t_3 + 273.15) \cdot \left( \frac{p_3}{p_1} \right)^{\frac{1-\kappa}{\kappa}} - 273.15$$

When input 'Temperature correction' is set to 2, then an isentropic expansion based on input 'Temperature exponent' is applied:

$$t_2 = (t_3 + 273.15) \cdot \left( \frac{p_3}{p_2} \right)^{K_{TE}} - 273.15$$

$$t_1 = (t_3 + 273.15) \cdot \left( \frac{p_3}{p_1} \right)^{K_{TE}} - 273.15$$

When input 'Temperature correction' is set to 3, then an isenthalpic expansion based on the linear Joule Thomson correction as defined in ISO5167-1:2003, taking input 'Temperature exponent' as the Joule Thomson coefficient:

$$t_1 = t_2 + (p_1 - p_2) \cdot \mu_{JT} \quad t_1 = t_3 + (p_1 - p_3) \cdot \mu_{JT}$$

Where:

|                       |                                     |        |
|-----------------------|-------------------------------------|--------|
| <b>t<sub>1</sub></b>  | Upstream temperature                | °C     |
| <b>t<sub>3</sub></b>  | Downstream temperature              | °C     |
| <b>p<sub>1</sub></b>  | Upstream pressure                   | bar(a) |
| <b>p<sub>3</sub></b>  | Fully recovered downstream pressure | bar(a) |
| <b>κ</b>              | Isentropic exponent                 | -      |
| <b>K<sub>TE</sub></b> | Temperature exponent                | -      |
| <b>μ<sub>JT</sub></b> | Joule Thomson coefficient           | °C/bar |

ISO-5167 edition 2003 prescribes an isenthalpic expansion instead of an isentropic expansion. This can be achieved by assigning a fixed Joule Thomson coefficient to input 'Temperature Exponent'.

Note: ISO is working a method to calculate the Joule Thomson rather than using a fixed value.

### Density correction

When input 'Density exponent' = 0, then the following isentropic corrections are applied (depending on the type of Density Correction)

$$\rho_1 = \rho_2 \cdot \left( \frac{p_1}{p_2} \right)^{\frac{1}{\kappa}} \quad \rho_1 = \rho_3 \cdot \left( \frac{p_1}{p_3} \right)^{\frac{1}{\kappa}}$$

Else the value of input 'Density Exponent' is used

$$\rho_1 = \rho_2 \cdot \left( \frac{p_1}{p_2} \right)^{K_{DE}} \quad \rho_1 = \rho_3 \cdot \left( \frac{p_1}{p_3} \right)^{K_{DE}}$$

Where:

|            |  |          |
|------------|--|----------|
| <b>p1</b>  | Upstream density                                   | [kg/m3]  |
| <b>p2</b>  | Density at the downstream tapping                  | [kg/m3]  |
| <b>p3</b>  | Density at the fully recovered downstream pressure | [kg/m3]  |
| <b>p1</b>  | Upstream pressure                                  | [bar(a)] |
| <b>p2</b>  | Pressure at the downstream tapping                 | [bar(a)] |
| <b>p3</b>  | Fully recovered downstream pressure                | [bar(a)] |
| <b>κ</b>   | Isentropic exponent                                | [-]      |
| <b>KDE</b> | Density exponent                                   | [-]      |

Note: In March 2007 the British DTI (Department of Trade and Industry) has recommended that the density correction method should not be based on isentropic expansion but on isenthalpic expansion instead.

The correction assumes that the density is measured at  $p_2$  (downstream pressure tapping pressure) and  $t_3$  (downstream recovered temperature). For this situation the following density correction is defined:

$$\rho_1 = \rho_M \cdot \frac{p_1 \cdot t_3 \cdot Z(p_2, t_3)}{p_2 \cdot t_1 \cdot Z(p_1, t_1)}$$

Where:

|                 |   |          |
|-----------------|---|----------|
| <b>p1</b>       | Upstream density  | [kg/m3]  |
| <b>pM</b>       | Measured density from the densitometer at p2 and t3               | [kg/m3]  |
| <b>p1</b>       | Upstream pressure   | [bar(a)] |
| <b>p2</b>       | Pressure at the downstream tapping                                | [bar(a)] |
| <b>t1</b>       | Upstream temperature  | °C       |
| <b>t3</b>       | Temperature at downstream side Where pressure has fully recovered | °C       |
| <b>Z(p1,t1)</b> | Compressibility at p1 and t1                                      | [-]      |
| <b>Z(p2,t3)</b> | Compressibility at p2 and t3                                      | [-]      |

When required, this correction should be applied outside the ISO5167 function by defining an additional compressibility calculation (e.g. AGA8) at  $p_2$  and  $t_3$  in the application and calculating the upstream density, Where the value of  $p_2$  is provided as an output by the ISO5167 function. Subsequently the upstream density is calculated and fed into the ISO5167 function (input 'Density') with input 'Density Correction' set to 'Upstream density'.

#### Correction for drain hole

When input 'Drain hole' is > 0 then the following correction factor is applied on the orifice diameter according to the British standard 1042: Part 1: 1964 and ISO/TR 15377:2007

$$C_{DH} = 1 + 0.55 * \left( \frac{d_{DH}}{d_0} \right)^2$$

Where:

|            |   |      |
|------------|---|------|
| <b>CDH</b> | Darin hole correction factor on orifice diameter                          | [-]  |
| <b>dDH</b> | Drain hole diameter   | [mm] |
| <b>d0</b>  | Orifice diameter at reference temperature (i.e. input 'Orifice diameter') | [mm] |

## fxISO5167\_Venturi

### Description

The function calculates the mass flow rate for **classical Venturi** tube pressure differential flow devices according to the ISO-5167 standard.

### Compliance

ISO-5167 - 1991 Measurement of fluid flow by means of pressure differential devices, 1st edition, 1991  
 ISO-5167 Amd.1 : 1998(E)  
 ISO-5167 - 2003 Measurement of fluid flow by means of pressure differential devices inserted in circular cross-section conduits running full, 2nd edition, 2003

### Function inputs

| Function inputs               | Remark   | EU          | Range | Default   |
|-------------------------------|--|-------------|-------|-----------|
| Name                          | Optional tag name, tag description and tag group   |             |       |           |
| Differential Pressure         | Differential pressure over the primary flow device measured at the up- and downstream pressure tapings, which need to be in the positions as specified in the standard   | mbar        |       | 0         |
| Pressure                      | Upstream pressure value of the fluid at metering conditions  | bar(a)      |       | 0         |
| Temperature                   | Down- or upstream temperature of the fluid at metering conditions  | °C          |       | 0         |
| Density                       | Down or upstream density of the fluid at metering conditions   | kg/m3       |       | 0         |
| Dynamic Viscosity             | Dynamic viscosity of the fluid   | Pa.s        |       | 0         |
| Isentropic Exponent           | Also referred to as $\kappa$ (kappa). For an ideal gas this coefficient is equal to the ratio of the specific heat capacity at constant pressure to the specific heat at constant volume. According to the ISO standard this ratio may be used, when the real value is unknown.  | -           |       | 0         |
| Pipe Diameter                 | Internal diameter of the pipe at reference temperature   | mm          |       | 0         |
| Pipe Expansion factor         | The thermal expansion coefficient of the pipe material   | 1/°C        |       | 0.0000108 |
| Pipe Reference temperature    | The reference temperature that corresponds to the 'Pipe diameter' input value  | °C          |       | 20        |
| Venturi Diameter              | Venturi diameter at reference temperature  | mm          |       | 0         |
| Venturi Expansion factor      | The thermal expansion coefficient of the Venturi material  | 1/°C        |       | 0.0000163 |
| Venturi Reference Temperature | The reference temperature that corresponds to the 'Venturi diameter' input value   | °C          |       | 20        |
| Configuration                 | The type of classical venturi tube.<br>Three configurations are permitted by the ISO5167 standard. Each configuration has a different calculation of the discharge coefficient and of the expansion factor<br>1: As cast convergent section<br>2: Rough welded<br>3: Machined<br>4: User-defined (not according to the standard!)<br>When 'User-defined' is selected then the input 'Discharge coefficient' will be used in the calculations instead.  | -           |       | 2         |
| Pressure Location             | 1: Upstream<br>Input 'Pressure' represents the pressure at the upstream pressure tapping ( $p_1$ ).<br>Since the absolute pressure is usually measured at the upstream tapping this is the most common setting.<br>2: Downstream<br>Input 'Pressure' represents the pressure at the downstream tapping ( $p_2$ ).  | -           |       | 1         |
| Temperature Location          | 1: Upstream<br>Input 'Temperature' represents the upstream temperature ( $t_1$ ).<br>2: Downstream<br>Input 'Temperature' represents the temperature at the downstream tapping ( $t_2$ ).<br>3: Recovered<br>Input 'Temperature' represents the downstream temperature at a location Where the pressure has fully recovered ( $t_3$ ).<br>Since temperature measurement is usually downstream of the flow device this is the most common setting.  | -           |       | 2         |
| Temperature Correction        | This parameter specifies how the temperature should be corrected from downstream to upstream conditions (or vice versa)<br>1: $(1-\kappa)/\kappa$<br>Isentropic expansion using $(1-\kappa)/\kappa$ as the temperature referral exponent<br>2: Constant<br>Isentropic expansion using input 'Temperature Exponent' as the temperature referral exponent [-].<br>Please note that this value must be < 0<br>3: Joule Thomson<br>Isenthalpic expansion using input 'Temperature Exponent' as the Joule Thomson coefficient [°C/bar].<br>This method is prescribed by ISO5167-1:2003. |             |       | 3         |
| Temperature Exponent          | Refer to input Temperature Correction<br>Unit depends on input Temperature Correction value  | -<br>°C/bar |       | 0         |
| Density Location              | This parameter specifies if and how the density should be corrected from downstream to upstream conditions (or vice versa).<br>1: Upstream<br>Input 'Density' represents the density at the upstream pressure tapping ( $\rho_1$ ).<br>2: Downstream   | -           |       | 1         |

| Function inputs       | Remark   | EU        | Range | Default |
|-----------------------|--|-----------|-------|---------|
|                       | Input 'Density' represents the density at the downstream tapping ( $\rho_2$ ).<br>3: Recovered<br>Input 'Density' represents the density downstream at a location Where the pressure has fully recovered ( $\rho_3$ ).   |           |       |         |
| Density Exponent.     | This factor is used when density correction is enabled. The formula $1/\kappa$ will be used when the input value is set to 0, else the input value will be used.<br>For more details refer to section 'Density correction'.  | -         |       | 0       |
| Fluid                 | The type of fluid being measured<br>1: Gas<br>2: Liquid  | -         |       | 1       |
| Pressure Loss Mode    | The method for determining the pressure loss<br>1: Absolute value in mbar<br>The value of input 'Pressure Loss Value' is taken as a value in mbar<br>2: Percentage of differential pressure<br>The value of input 'Pressure Loss Value' is taken as a percentage from input 'Differential Pressure'  | -         |       | 1       |
| Pressure Loss Value   | Value in mbar or %, depending on the 'Pressure Loss Mode'.<br>The pressure loss over the Venturi is used to calculate the downstream fully recovered pressure. %<br>The pressure loss equals the difference between the upstream pressure ( $p_1$ ) and the fully recovered downstream pressure ( $p_3$ )<br>The standard prescribes that only the pressure loss that is caused by the venturi tube should be included (so it should not include the pressure loss that occurred between the two pressure tappings before the venturi tube was installed). | mbar<br>% |       | 0       |
| Discharge coefficient | This value will used instead of the discharge coefficient as specified in the standard.<br>Only used when input 'Configuration' is set to 'User-defined'.  | -         |       | 0       |

## Function outputs

| Function outputs                  | Remark  | EU      | Fallback |
|-----------------------------------|---|---------|----------|
| Status                            | 0: Normal (No error condition)<br>1: Input argument out of range<br>2: No convergence   |         |          |
| Mass flow rate                    | The calculated mass flow rate   | tonne/h | 0        |
| Beta ratio                        | Venturi to pipe diameter ratio at upstream temperature  | -       | 0        |
| Venturi diameter                  | At the upstream temperature   | mm      | 0        |
| Pipe diameter                     | At the upstream temperature   | mm      | 0        |
| Upstream pressure                 | Pressure at upstream tapping ( $p_1$ )  | bar(a)  | 0        |
| Pressure at downstream tapping    | Pressure at downstream tapping ( $p_2$ )  | bar(a)  | 0        |
| Recovered downstream pressure     | Fully recovered downstream pressure ( $p_3$ )   | bar(a)  | 0        |
| Upstream temperature              | Temperature at upstream tapping ( $t_1$ )   | °C      | 0        |
| Temperature at downstream tapping | Temperature at downstream tapping ( $t_2$ )   | °C      | 0        |
| Downstream Temperature            | 'Fully recovered' downstream temperature ( $t_3$ )  | °C      | 0        |
| Upstream density                  | Density at upstream tapping ( $\rho_1$ )  | kg/m3   | 0        |
| Density at downstream tapping     | Pressure at downstream tapping ( $\rho_2$ )   | kg/m3   | 0        |
| Downstream density                | 'Fully recovered' downstream density ( $\rho_3$ )   | kg/m3   | 0        |
| Reynolds number                   | The pipe Reynolds number (this is the Reynolds number upstream of the Venturi and not the one within the device throat itself)      | -       | 0        |
| Discharge coefficient             |   | -       | 0        |
| Expansion Factor                  |   | -       | 0        |
| Velocity of Approach              |   |         | 0        |
| Pressure Range                    | 0: Pressure is in valid range<br>1: Pressure is out of valid range  | -       | 0        |
| Reynolds Range                    | 0: Reynolds number is in valid range<br>1: Reynolds number is out of valid range  | -       | 0        |
| Diameter Range                    | 0: Device and pipe diameter and Beta ratio in valid range<br>1: Device diameter, pipe diameter and/or Beta ratio out of valid range | -       | 0        |

## fxISO5167\_VenturiNozzle

### Description

The function calculates the mass flow rate for **Venturi Nozzle** pressure differential flow devices according to the ISO-5167 standard.

### Compliance

ISO-5167 - 1991 Measurement of fluid flow by means of pressure differential devices, 1st edition, 1991  
 ISO-5167 Amd.1 : 1998(E)  
 ISO-5167 - 2003 Measurement of fluid flow by means of pressure differential devices inserted in circular cross-section conduits running full, 2nd edition, 2003

### Function inputs

| Function inputs                      | Remark   | EU          | Default   |
|--------------------------------------|--|-------------|-----------|
| Name                                 | Optional tag name, tag description and tag group   |             |           |
| Differential Pressure                | Differential pressure over the primary flow device measured at the up- and downstream pressure tapings, which need to be in the positions as specified in the standard   | mbar        | 0         |
| Pressure                             | Upstream pressure value of the fluid at metering conditions  | bar(a)      | 0         |
| Temperature                          | Down- or upstream temperature of the fluid at metering conditions  | °C          | 0         |
| Density                              | Down or upstream density of the fluid at metering conditions   | kg/m3       | 0         |
| Dynamic Viscosity                    | Dynamic viscosity of the fluid   | Pa.s        | 0         |
| Isentropic Exponent                  | Also referred to as $\kappa$ (kappa). For an ideal gas this coefficient is equal to the ratio of the specific heat capacity at constant pressure to the specific heat at constant volume. According to the ISO standard this ratio may be used, when the real value is unknown.  |             | 0         |
| Pipe Diameter                        | Internal diameter of the pipe at reference temperature   | mm          | 0         |
| Pipe Expansion factor                | The thermal expansion coefficient of the pipe material   | 1/°C        | 0.0000108 |
| Pipe Reference temperature           | The reference temperature that corresponds to the 'Pipe diameter' input value  | °C          | 20        |
| Venturi Nozzle Diameter              | Venturi Nozzle diameter at reference temperature   | mm          | 0         |
| Venturi Nozzle Expansion factor      | The thermal expansion coefficient of the Venturi Nozzle material   | 1/°C        | 0.0000163 |
| Venturi Nozzle Reference Temperature | The reference temperature that corresponds to the 'Venturi Nozzle diameter' input value  | °C          | 20        |
| Pressure Location                    | 1 Input 'Pressure' represents the pressure at the upstream pressure tapping ( $p_1$ ).<br>Since the absolute pressure is usually measured at the upstream tapping this is the most common setting.   | -           | 1         |
|                                      | 2 Input 'Pressure' represents the pressure at the downstream tapping ( $p_2$ ).  |             |           |
| Temperature Location                 | 1 Input 'Temperature' represents the upstream temperature ( $t_1$ ).   | -           | 2         |
|                                      | 2 Input 'Temperature' represents the temperature at the downstream tapping ( $t_2$ ).  |             |           |
|                                      | 3 Input 'Temperature' represents the downstream temperature at a location Where the pressure has fully recovered ( $t_3$ ).<br>Since temperature measurement is usually downstream of the flow device this is the most common setting.   |             |           |
| Temperature Correction               | 1 Isentropic expansion using $(1-\kappa)/\kappa$ as the temperature referral exponent  |             | 3         |
|                                      | 2 Isentropic expansion using input 'Temperature Exponent' as the temperature referral exponent [-]   |             |           |
|                                      | 3 Isenthalpic expansion using input 'Temperature Exponent' as the Joule Thomson coefficient [°C/bar].<br>This method is prescribed by ISO5167-1:2003.  |             |           |
| Temperature Exponent                 | Refer to input Temperature Correction  | -<br>°C/bar | 0         |
| Density Location                     | This parameter specifies if and how the density should be corrected from downstream to upstream conditions.  | -           | 1         |
|                                      | 1 Input 'Density' represents the density at the upstream pressure tapping ( $\rho_1$ ).  |             |           |
|                                      | 2 Input 'Density' represents the density at the downstream tapping ( $\rho_2$ ).   |             |           |
|                                      | 3 Input 'Density' represents the density downstream at a location Where the pressure has fully recovered ( $\rho_3$ ).   |             |           |
| Density Exponent.                    | This factor is used when density correction is enabled. The formula $1/\kappa$ will be used when the input value is set to 0, else the input value will be used.<br>For more details refer to function 'ISO5167 - Orifice' section 'Density correction'  | -           | 0         |
| Fluid                                | The type of fluid being measured<br>1: Gas<br>2: Liquid  | -           | 1         |
| Pressure Loss Mode                   | The method for determining the pressure loss   | -           | 1         |
|                                      | 1 Absolute value in mbar<br>The value of input 'Pressure Loss Value' is taken as a value in mbar   |             |           |
|                                      | 2 Percentage of differential pressure<br>The value of input 'Pressure Loss Value' is taken as a percentage from input 'Differential Pressure'  |             |           |
| Pressure Loss Value                  | Value in mbar or %, depending on the 'Pressure Loss Mode'.<br>The pressure loss over the Venturi nozzle is used to calculate the downstream fully recovered pressure. The pressure loss equals the difference between the upstream pressure ( $p_1$ ) and the fully recovered downstream pressure ( $p_3$ )<br>The standard prescribes that only the pressure loss that is caused by the venturi nozzle should be included (so it should not include the pressure loss that occurred between the two pressure tapings) | mbar<br>%   | 0         |



| Function inputs | Remark                                    | EU | Default |
|-----------------|---|----|---------|
|                 | before the venturi nozzle was installed). |    |         |

### Function outputs

| Function outputs                  | Remark  | EU      | Fallback |
|-----------------------------------|---|---------|----------|
| Status                            | 0: Normal (No error condition)<br>1: Input argument out of range<br>2: No convergence   |         |          |
| Mass flow rate                    | The calculated mass flow rate   | tonne/h | 0        |
| Beta ratio                        | Venturi nozzle to pipe diameter ratio at upstream temperature   |         | 0        |
| Venturi Nozzle diameter           | At the upstream temperature   |         | 0        |
| Pipe diameter                     | At the upstream temperature   |         | 0        |
| Upstream pressure                 | Pressure at upstream tapping ( $p_1$ )  | bar(a)  | 0        |
| Pressure at downstream tapping    | Pressure at downstream tapping ( $p_2$ )  | bar(a)  | 0        |
| Recovered downstream pressure     | Fully recovered downstream pressure ( $p_3$ )   | bar(a)  | 0        |
| Upstream temperature              | Temperature at upstream tapping ( $t_1$ )   | °C      | 0        |
| Temperature at downstream tapping | Temperature at downstream tapping ( $t_2$ )   | °C      | 0        |
| Downstream Temperature            | 'Fully recovered' downstream temperature ( $t_3$ )  | °C      | 0        |
| Upstream density                  | Density at upstream tapping ( $\rho_1$ )  | kg/m3   | 0        |
| Density at downstream tapping     | Pressure at downstream tapping ( $p_2$ )  | kg/m3   | 0        |
| Downstream density                | 'Fully recovered' downstream density ( $\rho_3$ )   | kg/m3   | 0        |
| Reynolds number                   | The pipe Reynolds number (this is the Reynolds number upstream of the Venturi nozzle and not the one within the device throat itself) | -       | 0        |
| Discharge coefficient             |   | -       | 0        |
| Expansion Factor                  |   | -       | 0        |
| Velocity of Approach              |   |         | 0        |
| Pressure Range                    | 0: Pressure is in valid range<br>1: Pressure is out of valid range  | -       | 0        |
| Reynolds Range                    | 0: Reynolds number is in valid range<br>1: Reynolds number is out of valid range  | -       | 0        |
| Diameter Range                    | 0: Device and pipe diameter and Beta ratio in valid range<br>1: Device diameter, pipe diameter and/or Beta ratio out of valid range   | -       | 0        |

### Temperature correction

When input 'Temperature exponent' = 0, then an isentropic expansion is applied:

$$t_1 = (t_3 + 273.15) \cdot \left( \frac{p_3}{p_1} \right)^{\frac{1-\kappa}{\kappa}} - 273.15$$

Else the value of input 'Temperature exponent' is used:

$$t_1 = (t_3 + 273.15) \cdot \left( \frac{p_3}{p_1} \right)^{K_{TE}} - 273.15$$

Where:

|                       |                                     |          |
|-----------------------|-------------------------------------|----------|
| <b>t<sub>1</sub></b>  | Upstream temperature                | [°C]     |
| <b>t<sub>3</sub></b>  | Downstream temperature              | [°C]     |
| <b>p<sub>1</sub></b>  | Upstream pressure                   | [bar(a)] |
| <b>p<sub>3</sub></b>  | Fully recovered downstream pressure | [bar(a)] |
| <b>κ</b>              | Isentropic exponent                 | [-]      |
| <b>K<sub>TE</sub></b> | Temperature exponent                | [-]      |

## fxISO6976\_1983\_M

### Description

ISO standard 6976 defines component properties and calculations to determine the calorific value, density and relative density for a gas composition at the specified metering and combustion reference temperatures and 1.01325 bar(a).

### Compliance

- International standard, Natural Gas - Calculation of calorific values, density, relative density and Wobbe index (ISO 6976:1983)

### Boundaries

ISO6976:1983 does not define limits for its input data.

### Function inputs

| Function inputs                       | Remark  | EU      | Range | Default |
|---------------------------------------|---|---------|-------|---------|
| Name                                  | Optional tag name, tag description and tag group  |         |       |         |
| Composition                           | Standard composition as defined in section 'Standard gas composition.   | mol/mol | 0..1  | 0       |
| Metering reference temperature        | Temperature used for calculating the compressibility, the density and the real relative density values<br>1: 0 °C<br>2: 15 °C   | -       |       | 1       |
| Calorific value reference temperature | Temperatures used for calculating the calorific values.<br>1st value represents the combustion reference temperature and the 2nd value the Gas volume reference temperature<br>1: 25 °C / 0 °C<br>2: 0 °C / 0 °C<br>3: 15 °C / 0 °C<br>4: 15 °C / 15 °C<br>5: 60 °F / 60 °F | -       |       | 1       |

### Function outputs

| Function outputs         | Remark   | EU      | Fallback |
|--------------------------|--|---------|----------|
| Status                   | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: Mole fractions do not add up to 1.0 +/- 0.0001 |         |          |
| Superior calorific value | Real value at the reference conditions of temperature and pressure   | MJ/m3   | 0        |
| Density                  | At the reference conditions of temperature and pressure  | kg/m3   | 0        |
| Compressibility          |  | -       | 1        |
| Relative density         |  | -       | 0        |
| Molar mass               |  | kg/kmol | 0        |

### Calculations

Calculations are performed in accordance with the standard, using the values as listed in the tables of the standard.

## fxISO6976\_1995\_M

### Description

ISO standard 6976 edition 1995 defines component properties and calculations to determine the calorific value, density, relative density and Wobbe index for a gas composition at the specified metering and combustion reference temperatures and 1.01325 bar(a).

Both the definitive and alternative methods of calculating the calorific value on a mass and volumetric basis are included.

### Boundaries

- The valid ranges for molar fractions are as follows:

|                  |                   |
|------------------|-------------------|
| • Methane        | 0.5 <= .. <= 1.0  |
| • Nitrogen       | 0.0 <= .. <= 0.3  |
| • Ethane         | 0.0 <= .. <= 0.15 |
| • Carbon dioxide | 0.0 <= .. <= 0.15 |
| • All others     | 0.0 <= .. <= 0.05 |

### Compliance

- International standard, Natural Gas - Calculation of calorific values, density, relative density and Wobbe index (ISO 6976:1995/BS7589)

### Function inputs and outputs

| Function inputs                    | Remark   | EU      | Range | Default |
|------------------------------------|--|---------|-------|---------|
| Name                               | Optional tag name, tag description and tag group   |         |       |         |
| Composition                        | Standard composition as defined in section 'Standard gas composition.'   | mol/mol | 0..1  | 0       |
| Reference conditions               | The reference temperature for combustion / metering:<br>1: 15°C / 15°C<br>2: 0°C / 0°C<br>3: 15°C / 0°C<br>4: 25°C / 0°C<br>5: 20°C / 20°C<br>6: 25°C / 20°C   |         |       | 1       |
| Molar mass table method            | 1: Calculate<br>Calculates the molar mass from the atomic masses as defined in the note of Table 1 of the standard<br>2: Table<br>Uses the values from Table 1 of the standard   | -       |       | 1       |
| Calorific value calculation method | Refer to paragraph 6.1 and 7.1 of the standard<br>1: Definitive method<br>Calculates the mass based calorific value from the molar based calorific values from table 3 and from the calculated molar mass values.<br>Calculates the volume based calorific value by multiplying the molar based calorific values from table 3 by p2/R.T2<br>2: Alternative method<br>Uses the values from tables 3, 4 and 5 as listed in the standard. | -       |       | 1       |

| Function outputs         | Remark   | EU      | Fallback |
|--------------------------|--|---------|----------|
| Status                   | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: Mole fractions do not add up to 1.0 +/- 0.0001 |         |          |
| Superior calorific value | Real superior calorific value on volume basis at the reference conditions of temperature and pressure                    | MJ/m3   | 0        |
| Density                  | At the reference conditions of temperature and pressure  | kg/m3   | 0        |
| Compressibility          |  | -       | 1        |
| Relative density         |  | -       | 0        |
| Molar mass               |  | kg/kmol | 0        |
| Superior calorific value | Real superior calorific value on mass basis at the reference conditions of temperature and pressure                      | MJ/kg   | 0        |
| Superior calorific value | Real superior calorific value on mole basis at the reference conditions of temperature and pressure                      | MJ/kmol | 0        |
| Inferior calorific value | Real inferior calorific value on volume basis at the reference conditions of temperature and pressure                    | MJ/m3   | 0        |
| Inferior calorific value | Real inferior calorific value on mass basis at the reference conditions of temperature and pressure                      | MJ/kg   | 0        |
| Inferior calorific value | Real superior calorific value on mole basis at the reference conditions of temperature and pressure                      | MJ/kmol | 0        |
| Wobbe index              |  | MJ/m3   | 0        |
| Data range               | With respect to the ISO6976-1995 standard the combination of input values is:<br>0: In Range<br>1: Out of Range          |         | -        |

### Calculations

Calculations are performed in accordance with the standard.

## fxISO6976ex\_1995\_M

### Description

Extended version that takes the first 55 components as used in the standard plus an additional set of user-definable components.

ISO standard 6976 edition 1995 defines component properties and calculations to determine the calorific value, density, relative density and Wobbe index for a gas composition at the specified metering and combustion reference temperatures and 1.01325 bar(a).

Both the definitive and alternative methods of calculating the calorific value on a mass and volumetric basis are included.

### Boundaries

The valid ranges for molar fractions are as follows:

- Methane 0.5 ≤ .. ≤ 1.0
- Nitrogen 0.0 ≤ .. ≤ 0.3
- Ethane 0.0 ≤ .. ≤ 0.15
- Carbon dioxide 0.0 ≤ .. ≤ 0.15
- All others 0.0 ≤ .. ≤ 0.05

### Compliance

- International standard, Natural Gas - Calculation of calorific values, density, relative density and Wobbe index (ISO 6976:1995/BS7589)

### Function inputs

| Function inputs | Remark   | EU      | Default |
|-----------------|--|---------|---------|
| Name            | Optional tag name, tag description and tag group   |         |         |
| Composition     | <p>Array of mole fractions of the first 55 components as used in the standard.</p> <p>1: Methane<br/>2: Ethane<br/>3: Propane<br/>4: n-Butane<br/>5: 2-Methylpropane<br/>6: n-Pentane<br/>7: 2-Methylbutane<br/>8: 2,2-Dimethylpropane<br/>9: n-Hexane<br/>10: 2-Methylpentane<br/>11: 3-Methylpentane<br/>12: 2,2-Dimethylbutane<br/>13: 2,3-Dimethylbutane<br/>14: n-Heptane<br/>15: n-Octane<br/>16: n-Nonane<br/>17: n-Decane<br/>18: Ethylene<br/>19: Propylene<br/>20: 1-Butene<br/>21: cis-2-Butene<br/>22: trans-2-Butene<br/>23: 2-Methylpropene<br/>24: 1-Pentene<br/>25: Propadiene<br/>26: 1,2-Butadiene<br/>27: 1,3-Butadiene<br/>28: Acetylene<br/>29: Cyclopentane<br/>30: Methylcyclopentane<br/>31: Ethylcyclopentane<br/>32: Cyclohexane<br/>33: Methylcyclohexane<br/>34: Ethylcyclohexane<br/>35: Benzene<br/>36: Toluene<br/>37: Ethylbenzene<br/>38: o-Xylene<br/>39: Methanol<br/>40: Methanethiol<br/>41: Hydrogen<br/>42: Water<br/>43: Hydrogen sulfide<br/>44: Ammonia<br/>45: Hydrogen cyanide<br/>46: Carbon monoxide<br/>47: Carbonyl sulfide<br/>48: Carbon disulfide<br/>49: Helium<br/>50: Neon<br/>51: Argon<br/>52: Nitrogen<br/>53: Oxygen</p> | mol/mol | 0       |

| Function inputs                             | Remark   | EU      | Default |
|---|--|---------|---------|
|   | 54: Carbon dioxide<br>55: Sulfur dioxide   |         |         |
| Reference conditions                        | The reference temperature for combustion / metering:<br>1: 15°C / 15°C<br>2: 0°C / 0°C<br>3: 15°C / 0°C<br>4: 25°C / 0°C<br>5: 20°C / 20°C<br>6: 25°C / 20°C   |         | 1       |
| Molar mass table method                     | 1: Calculate<br>Calculates the molar mass from the atomic masses as defined in the note of Table 1 of the standard<br>2: Table<br>Uses the values from Table 1 of the standard   | -       | 1       |
| Calorific value calculation method          | Refer to paragraph 6.1 and 7.1 of the standard<br>1: Definitive method<br>Calculates the mass based calorific value from the molar based calorific values from table 3 and from the calculated molar mass values.<br>Calculates the volume based calorific value by multiplying the molar based calorific values from table 3 by p2/R.T2<br>2: Alternative method<br>Uses the values from tables 3, 4 and 5 as listed in the standard. | -       | 1       |
| User-defined composition                    | Array of mole fractions of the additional user-definable components.<br>Note: The inputs for the additional components are optional inputs.  | mol/mol | 0       |
| User-defined molar mass                     | Array of molar masses of the additional user-definable components. This should be the molar mass corresponding to the current 'Molar mass table method'.<br>Note: This array should be exactly as long as the user-defined composition array.  | kg/kmol | 0       |
| User-defined summation factor               | Array of summation factor values of the additional user-definable components.<br>Note: The input values have to correspond with the metering conditions of input 'Reference conditions'. This array should be exactly as long as the user-defined composition array.   | -       | 0       |
| User-defined superior calorific value (SCV) | Array of Superior Calorific Values of the additional user-definable components. This should be the SCV corresponding to the current reference conditions.<br>Note: the input values have to correspond with the conditions as defined by input 'Reference conditions'. This array should be exactly as long as the user-definable composition array.   | KJ/mol  | 0       |
| User-defined inferior calorific value (ICV) | Array of Inferior Calorific Values of the additional user-definable components. This should be the ICV corresponding to the current reference conditions.<br>Note: the input values have to correspond with the conditions as defined by input 'Reference conditions'. This array should be exactly as long as the user-definable composition array.   | KJ/mol  | 0       |

## Function outputs

| Function outputs         | Remark   | EU      | Fallback |
|--------------------------|--|---------|----------|
| Status                   | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: Mole fractions do not add up to 1.0 +/- 0.0001 |         |          |
| Superior calorific value | Real superior calorific value on volume basis at the reference conditions of temperature and pressure                    | MJ/m3   | 0        |
| Density                  | At the reference conditions of temperature and pressure  | kg/m3   | 0        |
| Compressibility          |  | -       | 1        |
| Relative density         |  | -       | 0        |
| Molar mass               |  | kg/kmol | 0        |
| Superior calorific value | Real superior calorific value on mass basis at the reference conditions of temperature and pressure                      | MJ/kg   | 0        |
| Superior calorific value | Real superior calorific value on mole basis at the reference conditions of temperature and pressure                      | MJ/kmol | 0        |
| Inferior calorific value | Real inferior calorific value on volume basis at the reference conditions of temperature and pressure                    | MJ/m3   | 0        |
| Inferior calorific value | Real inferior calorific value on mass basis at the reference conditions of temperature and pressure                      | MJ/kg   | 0        |
| Inferior calorific value | Real superior calorific value on mole basis at the reference conditions of temperature and pressure                      | MJ/kmol | 0        |
| Wobbe index              |  | MJ/m3   | 0        |
| Data range               | With respect to the ISO6976-1995 standard the combination of input values is:<br>0: In Range<br>1: Out of Range          |         | -        |

## Calculations

Calculations are performed in accordance with the standard with the addition of the user-definable components.

based heating values that are calculated from these input properties. Only the Definitive Method for calculating the calorific value is supported in this case.

The properties of the user-definable components are specified by the corresponding inputs, except for the volume and mass

## fxISO6976\_2016\_M

### Description

ISO standard 6976 edition 2016 defines component properties and calculations to determine the calorific value, density, relative density and Wobbe index for a gas composition at the specified metering and combustion reference temperatures and metering pressure.

### Boundaries

The standard defines the following validity ranges

- 0.9 < Pressure < 1.1 bar
- Compressibility > 0.9

### Compliance

- International standard, Natural Gas - Calculation of calorific values, density, relative density and Wobbe indices from composition (ISO 6976:2016(e))

### Function inputs and outputs

| Function inputs             | Remark   | EU      | Range | Default |
|-----------------------------|--|---------|-------|---------|
| Name                        | Optional tag name, tag description and tag group   |         |       |         |
| Composition                 | Standard composition as defined in section 'Standard gas composition.'   | mol/mol | 0..1  | 0       |
| Reference conditions        | The reference temperature for combustion / metering:<br>1: 15°C / 15°C<br>2: 0°C / 0°C<br>3: 15°C / 0°C<br>4: 25°C / 0°C<br>5: 20°C / 20°C<br>6: 25°C / 20°C<br>7: 60°F / 60°F |         |       | 1       |
| Molar mass table method     | 1: Calculate<br>Calculates the molar mass from the atomic masses as defined in the note of Table 1 of the standard<br>2: Table<br>Uses the values from Table 1 of the standard | -       | 1..2  | 1       |
| Metering reference pressure | Metering reference pressure p2. The default value is 1.01325 bar (101.325 kPa).  | bar     | 0..2  | 1.01325 |

| Function outputs      | Remark   | EU      | Fallback |
|-----------------------|--|---------|----------|
| Status                | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: Mole fractions do not add up to 1.0 +/- 0.0001 |         |          |
| Gross calorific value | Real gas gross calorific value on volume basis at the reference conditions of temperature and pressure                   | MJ/m3   | 0        |
| Density               | At the reference conditions of temperature and pressure  | kg/m3   | 0        |
| Compressibility       |  | -       | 1        |
| Relative density      |  | -       | 0        |
| Molar mass            |  | kg/kmol | 0        |
| Gross calorific value | Real gas gross calorific value on mass basis at the reference conditions of temperature and pressure                     | MJ/kg   | 0        |
| Gross calorific value | Real gas gross calorific value on mole basis at the reference conditions of temperature and pressure                     | MJ/kmol | 0        |
| Net calorific value   | Real gas net calorific value on volume basis at the reference conditions of temperature and pressure                     | MJ/m3   | 0        |
| Net calorific value   | Real gas net calorific value on mass basis at the reference conditions of temperature and pressure                       | MJ/kg   | 0        |
| Net calorific value   | Real gas net calorific value on mole basis at the reference conditions of temperature and pressure                       | MJ/kmol | 0        |
| (Gross) Wobbe index   |  | MJ/m3   | 0        |
| Data range            | With respect to the ISO6976-2016 standard the combination of input values is:<br>0: In Range<br>1: Out of Range          |         | -        |

### Calculations

Calculations are performed in accordance with the standard.

## fxISO6976ex\_2016\_M

## Description

Extended version that takes the first 60 components as used in the standard plus an additional set of user-definable components.

ISO standard 6976 edition 2016 defines component properties and calculations to determine the calorific value, density, relative density and Wobbe index for a gas composition at the specified metering and combustion reference temperatures and metering pressure.

## Boundaries

The standard defines the following validity ranges

- 0.9 < Pressure < 1.1 bar
- Compressibility > 0.9

## Compliance

- International standard, Natural Gas - Calculation of calorific values, density, relative density and (Gross) Wobbe index (ISO 6976:2016/BS7589)

## Function inputs

| Function inputs | Remark   | EU      | Default |
|-----------------|--|---------|---------|
| Name            | Optional tag name, tag description and tag group   |         |         |
| Composition     | <p>Array of mole fractions of the first 55 components as used in the standard.</p> <p>1: Methane<br/> 2: Ethane<br/> 3: Propane<br/> 4: n-Butane<br/> 5: 2-Methylpropane<br/> 6: n-Pentane<br/> 7: 2-Methylbutane<br/> 8: 2,2-Dimethylpropane<br/> 9: n-Hexane<br/> 10: 2-Methylpentane<br/> 11: 3-Methylpentane<br/> 12: 2,2-Dimethylbutane<br/> 13: 2,3-Dimethylbutane<br/> 14: n-Heptane<br/> 15: n-Octane<br/> 16: n-Nonane<br/> 17: n-Decane<br/> 18: Ethylene<br/> 19: Propylene<br/> 20: 1-Butene<br/> 21: cis-2-Butene<br/> 22: trans-2-Butene<br/> 23: 2-Methylpropene<br/> 24: 1-Pentene<br/> 25: Propadiene<br/> 26: 1,2-Butadiene<br/> 27: 1,3-Butadiene<br/> 28: Acetylene<br/> 29: Cyclopentane<br/> 30: Methylcyclopentane<br/> 31: Ethylcyclopentane<br/> 32: Cyclohexane<br/> 33: Methylcyclohexane<br/> 34: Ethylcyclohexane<br/> 35: Benzene<br/> 36: Toluene<br/> 37: Ethylbenzene<br/> 38: o-Xylene<br/> 39: Methanol<br/> 40: Methanethiol<br/> 41: Hydrogen<br/> 42: Water<br/> 43: Hydrogen sulfide<br/> 44: Ammonia<br/> 45: Hydrogen cyanide<br/> 46: Carbon monoxide<br/> 47: Carbonyl sulfide<br/> 48: Carbon disulfide<br/> 49: Helium<br/> 50: Neon<br/> 51: Argon<br/> 52: Nitrogen<br/> 53: Oxygen<br/> 54: Carbon dioxide<br/> 55: Sulfur dioxide<br/> 56: N_undecane<br/> 57: N_Dodecane</p> | mol/mol | 0       |

| Function inputs                    | Remark  | EU      | Default |
|------------------------------------|---|---------|---------|
| Reference conditions               | 58: N_tridecane   |         |         |
|                                    | 59: N_pentadecane   |         |         |
|                                    | 60: N_pentadecane   |         |         |
|                                    | The reference temperature for combustion / metering:  |         | 1       |
|                                    | 1: 15°C / 15°C  |         |         |
|                                    | 2: 0°C / 0°C  |         |         |
|                                    | 3: 15°C / 0°C   |         |         |
|                                    | 4: 25°C / 0°C   |         |         |
| Molar mass table method            | 5: 20°C / 20°C  |         |         |
|                                    | 6: 25°C / 20°C  |         |         |
|                                    | 7: 60°F / 60°F  |         |         |
| Molar mass table method            | 1: Calculate  | -       | 1       |
|                                    | Calculates the molar mass from the atomic masses as defined in the note of Table 1 of the standard  |         |         |
| Metering reference pressure        | 2: Table  |         |         |
|                                    | Uses the values from Table 1 of the standard  |         |         |
| Metering reference pressure        | Metering reference pressure p2.   | bar     | 1.01325 |
| User-defined composition           | Array of mole fractions of the additional user-definable components.<br>Note: The inputs for the additional components are optional inputs.   | mol/mol | 0       |
| User-defined molar mass            | Array of molar masses of the additional user-definable components. This should be the molar mass corresponding to the current 'Molar mass table method'.<br>Note: This array should be exactly as long as the user-defined composition array.   | kg/kmol | 0       |
| User-defined summation factor      | Array of summation factor values of the additional user-definable components.<br>Note: The input values have to correspond with the metering conditions of input 'Reference conditions'.<br>This array should be exactly as long as the user-defined composition array.   | -       | 0       |
| User-defined gross calorific value | Array of Gross Calorific Values of the additional user-definable components. This should be the CV corresponding to the current reference conditions.<br>Note: the input values have to correspond with the conditions as defined by input 'Reference conditions'.<br>This array should be exactly as long as the user-definable composition array. | KJ/mol  | 0       |

## Function outputs

| Function outputs      | Remark  | EU      | Fallback |
|-----------------------|---|---------|----------|
| Status                | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: Mole fractions do not add up to 1.0 +- 0.0001 |         |          |
| Gross calorific value | Real gross calorific value on volume basis at the reference conditions of temperature and pressure                      | MJ/m3   | 0        |
| Density               | At the reference conditions of temperature and pressure   | kg/m3   | 0        |
| Compressibility       |   | -       | 1        |
| Relative density      |   | -       | 0        |
| Molar mass            |   | kg/kmol | 0        |
| Gross calorific value | Real gas gross calorific value on mass basis at the reference conditions of temperature and pressure                    | MJ/kg   | 0        |
| Gross calorific value | Real gas gross calorific value on mole basis at the reference conditions of temperature and pressure                    | MJ/kmol | 0        |
| Net calorific value   | Real gas net calorific value on volume basis at the reference conditions of temperature and pressure                    | MJ/m3   | 0        |
| Net calorific value   | Real gas net calorific value on mass basis at the reference conditions of temperature and pressure                      | MJ/kg   | 0        |
| Net calorific value   | Real gas net calorific value on mole basis at the reference conditions of temperature and pressure                      | MJ/kmol | 0        |
| (Gross) Wobbe index   |   | MJ/m3   | 0        |
| Data range            | With respect to the ISO6976-2016 standard the combination of input values is:<br>0: In Range<br>1: Out of Range         |         | -        |

## Calculations

Calculations are performed in accordance with the standard with the addition of the user-definable components. The properties of the user-definable components are specified by the corresponding inputs, except for the volume and mass based heating values that are calculated from these input properties. Only the Definitive Method for calculating the calorific value is supported in this case.



## fxMR113

### Description

The relative humidity, compressibility, density, speed of sound, isentropic coefficient and optionally the dynamic viscosity of a gas are calculated from its composition, absolute humidity, temperature and pressure in accordance with the GOST MR113 standard. The CPU-intensive calculation of viscosity can be optionally enabled if the (flow computer) CPU capacity allows for this.

### Compliance

- The GSSSD method MR 113-03. Kozlov, Mamonov, Rogovin, Rybakov, (10/06/2003).

### Boundaries

The standard defines a valid range for pressure and temperature. The function will not accept input values outside this range

The valid range is as follows

- Pressure: 1 .. 150 bar(a)
- Temperature: 263..500 K (-10 ..+226 °C)

Note: the standard does not specify a range limitation for the components.

### Function inputs

| Function inputs       | Remark   | EU      | Range      | Default |
|-----------------------|--|---------|------------|---------|
| Name                  | Optional tag name, tag description and tag group   |         |            |         |
| Pressure              | Flowing pressure   | bar(a)  | 1..150     | 1.01325 |
| Temperature           | Flowing temperature  | °C      | -10..+226  | 0       |
| Composition           | Standard composition as defined in section 'Standard gas composition. Unused components must be set to 0.                        | mol/mol | 0..1       | 0       |
| neo-Pentane mode      | Determines what to do when component neo-Pentane is larger than zero<br>1: Add to i-Pentane<br>2: Add to n-Pentane<br>3: Neglect | -       | 1 .. 3     | 1       |
| Absolute humidity     | Absolute humidity at the humidity meter  | kg/m3   | 0 .. 1     | 0       |
| Humidity pressure     | Pressure value at the humidity meter   | bar(a)  | 0..3500    | 1.01325 |
| Humidity temperature  | Temperature value at the humidity meter  | °C      | -250..+450 | 0       |
| Reference pressure    | Reference pressure (base conditions)   | bar(a)  | 0..3500    | 1.01325 |
| Reference temperature | Reference temperature (base conditions)  | °C      | -250..+450 | 0       |
| Rounding              | 0: Disabled, full precision<br>1: Enabled, results are rounded   |         | 0 .. 1     | 0       |
| Viscosity calculation | 0: Disabled<br>1: Enabled<br>Note: the viscosity calculation is relative CPU-intensive.  |         | 0 .. 1     | 0       |

### Function outputs

| Function outputs     | Remark  | EU      | Fallback |
|----------------------|---|---------|----------|
| Status               | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence                        |         |          |
| Base Compressibility | At reference conditions   | -       | 1        |
| Flow Compressibility | At flowing conditions   | -       | 1        |
| Base Density         | At reference conditions   | kg/m3   | 0        |
| Flow Density         | At flowing conditions   | kg/m3   | 0        |
| Kappa                | Isotropic exponent  | -       | 0        |
| Molar Mass           |   | kg/kmol | 0        |
| Speed of Sound       | At flowing conditions   | m/s     | 0        |
| Dew point            | Water dew point, the temperature at which the water in the gas starts to condensate.                            | K       | 0        |
| Viscosity            | The dynamic viscosity of the gas. The calculation is disabled by default.                                       | Pa.s    | 0        |
| Max water fraction   | Maximum water fraction at flowing conditions  | %mole   | 0        |
| Water fraction       | Actual water fraction at flowing conditions   | %mole   | 0        |
| Relative humidity    | At flow conditions  | %       | 0        |
| Range                | 0: All input values are within the 'Normal Range'<br>1: One or more input values are outside the 'Normal Range' |         | 0        |

### Calculations

The calculations are as documented in the reference.

## fxNX19\_1962

### Description

The AGA NX-19 standard describes a method to calculate the super-compressibility for natural gases and was developed in 1962.

The 1962 standard describes a standard method for calculating the super-compressibility factor that is based on the actual pressure and temperature, the specific gravity and the mole fractions of the carbon dioxide and nitrogen.

The 1962 standard also specifies 3 alternate methods, which are based on a full compositional analysis (1st alternate method), the relationship between methane and specific gravity (2nd alternate method) and the relationship between the heating value and the specific gravity

The function only performs the standard method as specified by the standard and none of the alternate methods.

Note: the definition of the specific gravity as used in the standard is that of the ratio of the density of the gas to that of air at base conditions, so the real specific gravity or real relative density.

### Compliance

- AGA Par Research Project NX-19 - Manual for the Determination. of the Supercompressibility Factors for Natural Gas, 1962
- Flow Measurement Engineering Handbook, Third edition, Richard W. Miller, 1996, ISBN-0-07-042366-0

### Boundaries

The following boundaries apply for the input values. Using the standard for conditions that lie outside this range will yield to a higher uncertainty and is not recommended.

|                  |                 |         |
|------------------|-----------------|---------|
| Temperature      | -40..240        | °F      |
| Pressure         | 0..5000         | psig    |
| Relative density | 0.554 .. 01.000 | -       |
| Nitrogen         | 0.00 .. 0.15    | mol/mol |
| Carbon dioxide   | 0.00 .. 0.15    | mol/mol |

### Function inputs

| Function inputs  | Remark   | EU      | Range     | Default |
|------------------|--|---------|-----------|---------|
| Name             | Optional tag name, tag description and tag group   |         |           |         |
| Pressure         | Observed pressure  | psig    | 0..40000  | 0       |
| Temperature      | Observed temperature   | °F      | -250..800 | 60      |
| Specific gravity | Ratio of density of gas and density of air at the applicable reference conditions of pressure and temperature, i.e. the <u>real</u> specific gravity (real relative density).at 60°F and 14.73 psia. | -       | 0..2      | 0       |
| Nitrogen         | Mole fraction of nitrogen  | mol/mol | 0..1      | 0       |
| Carbon dioxide   | Mole fraction of carbon dioxide  | mol/mol | 0..1      | 0       |

### Function outputs

| Function outputs             | Remark  | EU | Fallback |
|------------------------------|---|----|----------|
| Status                       | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>Note: value 1 is also reported when one of the intermediate results is out of limit. |    |          |
| Compressibility factor       | Compressibility factor at the observed temperature and pressure (Zf)  | -  | 1        |
| Base compressibility factor  | Compressibility factor at 60 °F and 14.7 psia (Zb)  | -  | 1        |
| Super-compressibility factor | Super-compressibility Fpv. Refer to section Calculations for ist definition.  | -  | 1        |
| Range                        | 0: All input values are within the 'Normal Range'<br>1: One or more input values are outside the 'Normal Range'   | -  | 0        |

### Calculations

The AGA-NX-19 standard specifies the calculations of the super-compressibility Fpv, which is defined as follows:

$$F_{pv} = \sqrt{\frac{Z_b}{Z_f}}$$

Where:

|                       |   |
|-----------------------|---|
| <b>F<sub>pv</sub></b> | Supercompressibility  |
| <b>Z<sub>b</sub></b>  | Compressibility at base conditions of 60 °F and 14.7 psia                         |
| <b>Z<sub>f</sub></b>  | Compressibility at flowing conditions, i.e. at the input temperature and pressure |

The definition of the base compressibility factor when applying the AGA-NX19:1962 method for custody transfer is given in chapter 2 of [Miller:1996].

$$Z_b = \left[ \sqrt{1 + \frac{0.00132}{T^{3.25}}} \right]^{-2}$$

Where T = Tadj/500 with Tadj calculated in accordance with the AGA NX-19:1962 standard

## fxNX19\_M

### Description

The AGA NX-19 standard describes a method to calculate the super-compressibility for natural gases and was developed in 1962.

The 1962 standard describes a standard method for calculating the super-compressibility factor that is based on the actual pressure and temperature, the specific gravity and the mole fractions of the carbon dioxide and nitrogen.

The 1962 standard also specifies 3 alternate methods, which are based on a full compositional analysis (1st alternate method), the relationship between methane and specific gravity (2nd alternate method) and the relationship between the heating value and the specific gravity

The function only performs the standard method as specified by the standard and none of the alternate methods.

The function provides the option to perform the PTB G9 correction instead of the 1962 standard method. This consists of the modified NX-19 method (NX-19-mod) per Herning & Wolowsky and the additional 'BR.KORR.3H' correction for high-caloric gases (gross heating value  $\geq 39.8$  MJ/m<sup>3</sup>).

Note: the definition of the specific gravity as used in the standard is that of the ratio of the density of the gas to that of air at base conditions, so the real specific gravity or real relative density.

### Compliance

- AGA Par Research Project NX-19 - Manual for the Determination. of the Supercompressibility Factors for Natural Gas, 1962
- Berechnung von Realgasfaktoren und Kompressibilitätszahlen für Erdgas, Technische Richtlinie G9 der Physikalisch - Technische Bundesanstalt für meßgeräte für Gas (PTB), TRG 9 8/82

### Boundaries

The following bounds apply for the input values. Using the standard for conditions that lie outside this range will yield to a higher uncertainty and is not recommended.

| Input value         | AGA-NX-19 (1962) | AGA-NX-19-mod | AGA-NX-19-mod.BR.KORR.3H | EU                |
|---------------------|------------------|---------------|--------------------------|-------------------|
| Pressure            | 0 .. 350         | 0 .. 137.9    | 0..80                    | bar(a)            |
| Temperature         | -40..115.6       | -40..115.6    | 0..30                    | °C                |
| Relative density    | 0.554 .. 01.000  | 0.554..0.75   | 0.554..0.691             | -                 |
| Gross heating value | Not used         | 31.8..39.8    | 39.8..46.2               | MJ/m <sup>3</sup> |
| Nitrogen            | 0.00 .. 0.15     | 0.00 .. 0.15  | 0.00..0.025              | mol/mol           |
| Carbon dioxide      | 0.00 .. 0.15     | 0.00 .. 0.15  | 0.00..0.07               | mol/mol           |

### Function inputs

| Function inputs     | Remark  | EU                | Range     | Default |
|---------------------|---|-------------------|-----------|---------|
| Name                | Optional tag name, tag description and tag group  |                   |           |         |
| Pressure            | Observed pressure   | bar(a)            | 0..200    | 1.01325 |
| Temperature         | Observed temperature  | °C                | -100..300 | 0       |
| Specific gravity    | Ratio of density of gas and density of air at the applicable reference conditions of pressure and temperature, i.e. the <u>real</u> specific gravity (real relative density). If setting 'PTB G9 correction' is disabled the reference conditions are 60°F and 14.73 psia. Else the specific gravity value shall be at the applicable reference conditions of pressure and temperature. | -                 | 0..2      | 0       |
| Gross heating value | At the applicable reference conditions of pressure and temperature<br>Only required when the 'PTB G9 correction' is enabled.  | MJ/m <sup>3</sup> | 0..100    | 0       |
| Nitrogen            |   | mol/mol           | 0..1      | 0       |
| Carbon dioxide      |   | mol/mol           | 0..1      | 0       |
| PTB G9 correction   | Determines if the AGA-NX-19-mod / AGA-NX-19-mod.BR.KORR.3H is used instead of the AGA-NX-19-1962 standard calculation.<br>0: Disabled<br>1: Enabled   | -                 |           | 1       |

### Function outputs

| Function outputs       | Remark   | EU | Fallback |
|------------------------|--|----|----------|
| Status                 | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence<br>Note: value 1 is also reported when one of the intermediate results is out of limit. |    |          |
| Compressibility factor |  | -  | 1        |
| Range                  | 0: All input values are within the 'Normal Range'<br>1: One or more input values are outside the 'Normal Range'  | -  | 0        |

### Calculations

The calculations are as specified in the standards.

fxOIML\_R22\_1975

Description

This function calculates the density, mass and volume based alcoholic strength of ethanol and water mixtures.

Compliance

- International Organisation of Legal metrology: International alcoholometric tables.

Function input

| Function inputs                       | Remark  | EU    | Range          | Default |
|---------------------------------------|---|-------|----------------|---------|
| Observed temperature                  |   | °C    | -25..45        | 7       |
| Standard temperature for the mixture. |   | °C    | -25..45        | 20      |
| Standard temperature for ethanol      |   | °C    | -25..45        | 20      |
| Input density                         |   | kg/m3 | 771.93..999.97 | 829.110 |
| Conversion method                     | 1: From observed to standard conditions<br>2: From standard to observed conditions.   |       | 1..2           | 1       |
| Density margin.                       | Allow the input density to go out of the limits of the standard by this margin. E.g. Now the function allows an Input density of 769. | kg/m3 |                | 3       |

Function output

| Function outputs | Remark   | EU    | Fallback |
|------------------|--|-------|----------|
| Status           | 0: Normal (No error condition)<br>1: Input argument out of range<br>2: No convergence  |       |          |
| Density          |  | kg/m3 | 1        |
| Ctl              | Volume correction factor for temperature.  | 0..1  | 1        |
| Mass strength    | Mass based alcoholic strength.   | 0..1  | 1        |
| Volume strength  | Volume based alcoholic strength.   | 0..1  | 1        |
| CBSW             | Correction factor to calculate the volume of ethanol at the ethanol standard temperature from the volume of the mixture at the mixture standard temperature. | 0..1  | 1        |
| Range status     | 0: Input values are in the range of the standard<br>1: Input values are outside the range of the standard  |       |          |

## fxSarasota\_C

### Description

The function calculates the density from a frequency input signal provided by a Sarasota densitometer and corrects it for temperature and pressure effects in **US customary** units.

Note: The calibration constants also need to be in US customary units (°F, psi and lbm/ft<sup>3</sup>).

### Function inputs

| Function inputs         | Remark   | EU                  | SW tag   | Range         | Default |
|-------------------------|--|---------------------|----------|---------------|---------|
| Name                    | Optional tag name, tag description and tag group                                     |                     |          |               |         |
| Periodic time           | In microseconds<br>Equals 1000 divided by the frequency in [Hz]                      | μs                  |          | 0..1e6        | 0       |
| Line temperature        | Used when temperature correction is enabled  | °F                  |          | -273.15..+500 | 20      |
| Line pressure           | Used when pressure correction is enabled   | psig                |          | 0..200        | 0       |
| Temperature correction  | 0: Disabled<br>1: Enabled  | -                   | TEMPCOR  |               | 1       |
| Pressure correction     | 0: Disabled<br>1: Enabled  | -                   | PRESCOR  |               | 1       |
| Reference temperature   | Used when temperature correction is enabled  | °F                  | REFTEMP  | 0..100        | 20      |
| Reference pressure      | Used when pressure correction is enabled   | psig                | REFPRES  | 0..100        | 0       |
| d <sub>0</sub>          | Constant from calibration certificate<br>Note: value required in lbm/ft <sup>3</sup> | lbm/ft <sup>3</sup> | D0       | 0..2000       | 0       |
| τ <sub>0</sub>          | Constant from calibration certificate  | μs                  | T0       | 0..1e6        | 0       |
| K                       | Spool calibration constant from calibration certificate                              | -                   | K        | 0..3e3        | 0       |
| Temperature coefficient | Constant from calibration certificate  | μs/°F               | TEMPCOEF | -1e6..1e6     | 0       |
| Pressure coefficient    | Constant from calibration certificate  | μs/psi              | PRESOEF  | -1e6..1e6     | 0       |

### Function outputs

| Function outputs  | Remark  | EU                  | SW tag  | Alarm         | Fallback |
|-------------------|---|---------------------|---------|---------------|----------|
| Status            | 0: Normal<br>1: Input argument out of range<br>2: Calculation error |                     | STS     | FLOOR<br>CALC |          |
| Corrected density | Density corrected for temperature and pressure                      | lbm/ft <sup>3</sup> | CORDENS |               | 0        |

### Calculations

The corrected density ρ<sub>C</sub> is calculated by

$$\rho_C = d_0 \cdot \frac{\tau - \tau_C}{\tau_C} \cdot \left( 2 + K \cdot \frac{\tau - \tau_C}{\tau_C} \right)$$

$$\tau_C = \tau_0 + t_{COEF} \cdot (t - t_{CAL}) + p_{COEF} \cdot (p - p_{CAL})$$

Where:

|                   |  |                     |
|-------------------|--|---------------------|
| ρ <sub>C</sub>    | The corrected density                                      | lbm/ft <sup>3</sup> |
| d <sub>0</sub>    | Obtained from the calibration certificate                  | lbm/ft <sup>3</sup> |
| τ <sub>0</sub>    | Obtained from the calibration certificate                  | μs                  |
| K                 | Obtained from the calibration certificate                  | -                   |
| p <sub>COEF</sub> | Obtained from the calibration certificate                  | μs/psi              |
| t <sub>COEF</sub> | Obtained from the calibration certificate                  | μs/°F               |
| t                 | Line temperature   | °F                  |
| t <sub>CAL</sub>  | Reference temperature                                      | °F                  |
| p                 | Line pressure  | psig                |
| p <sub>CAL</sub>  | Reference pressure   | psig                |
| τ <sub>C</sub>    | Time periodic input corrected for temperature and pressure | μs                  |
| τ                 | Measured time period                                       | μs                  |

## fxSarasota\_M

### Description

The function calculates the density from a frequency input signal provided by a Sarasota densitometer and corrects it for temperature and pressure effects in **metric** units.

Note: Calibration constants also need to be in metric units (°C, bar and kg/m3).

### Function inputs

| Function inputs         | Remark   | EU     | Range         | Default |
|-------------------------|--|--------|---------------|---------|
| Name                    | Optional tag name, tag description and tag group                         |        |               |         |
| Periodic time           | In microseconds. Equals 1000 divided by the frequency in [Hz]            | µs     | 0..1e6        | 0       |
| Line temperature        | Used when temperature correction is enabled                              | °C     | -273.15..+500 | 20      |
| Line pressure           | Used when pressure correction is enabled                                 | bar(g) | 0..200        | 0       |
| Temperature correction  | 0: Disabled<br>1: Enabled  | -      |               | 1       |
| Pressure correction     | 0: Disabled<br>1: Enabled  | -      |               | 1       |
| Reference temperature   | Used when temperature correction is enabled                              | °C     | 0..100        | 20      |
| Reference pressure      | Used when pressure correction is enabled                                 | bar(g) | 0..100        | 0       |
| d <sub>0</sub>          | Constant from calibration certificate                                    | kg/m3  | 0..3000       | 0       |
| τ <sub>0</sub>          | Constant from calibration certificate                                    | µs     | 0..1e6        | 0       |
| K                       | Spool calibration constant from calibration certificate                  | -      | 0..3e3        | 0       |
| Temperature coefficient | Constant from calibration certificate                                    | µs/°C  | -1e6..1e6     | 0       |
| Pressure coefficient    | Constant from calibration certificate.<br>Note: value required in µs/bar | µs/bar | -1e6..1e6     | 0       |

### Function outputs

| Function outputs  | Remark  | EU    | SW tag            | Fallback |
|-------------------|---|-------|-------------------|----------|
| Status            | 0: Normal<br>1: Input argument out of range<br>Outputs will be set to fallback values<br>2: Calculation error<br>Outputs will be set to fallback values | STS   | FLOOR<br><br>CALC |          |
| Corrected density | Density corrected for temperature and pressure  | kg/m3 | CORDENS           | 0        |

### Calculations

The corrected density ρ<sub>C</sub> is calculated by

$$\rho_C = d_0 \cdot \frac{\tau - \tau_C}{\tau_C} \cdot \left( 2 + K \cdot \frac{\tau - \tau_C}{\tau_C} \right)$$

$$\tau_C = \tau_0 + t_{COEF} \cdot (t - t_{CAL}) + p_{COEF} \cdot (p - p_{CAL})$$

Where:

|                   |  |        |
|-------------------|--|--------|
| ρ <sub>C</sub>    | The corrected density                                      | kg/m3  |
| d <sub>0</sub>    | Obtained from the calibration certificate                  | kg/m3  |
| τ <sub>0</sub>    | Obtained from the calibration certificate                  | µs     |
| K                 | Obtained from the calibration certificate                  | -      |
| d <sub>0</sub>    | Obtained from the calibration certificate                  | -      |
| p <sub>COEF</sub> | Obtained from the calibration certificate                  | µs/bar |
| t <sub>COEF</sub> | Obtained from the calibration certificate                  | µs/°C  |
| t                 | Line temperature   | °C     |
| t <sub>CAL</sub>  | Reference temperature                                      | °C     |
| p                 | Line pressure  | bar(g) |
| p <sub>CAL</sub>  | Reference pressure   | bar(g) |
| τ <sub>C</sub>    | Time periodic input corrected for temperature and pressure | µs     |
| τ                 | The time period in µs                                      | µs     |

## fxSGERG\_C

### Description

This function performs the SGERG calculation in **USC** units.

The Standard (or Simplified) GERG TM5 1991 Virial Equation (SGERG or SGERG-88) has defines a method to calculate the Compressibility Factor (Z) for Natural Gases. The SGERG calculation is equivalent to the AGA8 Gross Characterisation Method, however the results are slightly different

Instead of the full compositional analysis (as used by the AGA 8 Detailed Characterization method), the Gross Characterisation Method (SGERG) uses a restricted set of input variables for its equation, comprising Relative Density, Superior Calorific Value, Carbon Dioxide and Nitrogen together with pressure and temperature.

### Compliance

- GERG Technical Monograph 5, Standard GERG Virial Equation, 1991

### Boundaries

The standard specifies a maximum uncertainty of the compressibility factor of 0.1% provided the inputs lie in the following range.

|                     |              |         |
|---------------------|--------------|---------|
| Pressure            | 0 .. 1740    | psi(a)  |
| Temperature         | 17 .. 143    | °F      |
| Gross heating value | 509 .. 1288  | Btu/ft3 |
| Relative density    | 0.55 .. 0.90 | -       |
| Carbon dioxide      | 0.00 .. 0.30 | mol/mol |
| Nitrogen            | 0.00 .. 0.50 | mol/mol |
| Hydrogen            | 0.00 .. 0.10 | mol/mol |

### Function inputs

| Function inputs      | Remark  | EU      | Range       | Default |
|----------------------|---|---------|-------------|---------|
| Name                 | Optional tag name, tag description and tag group  |         |             |         |
| Pressure             | Observed pressure   | psia    | 0..30000    |         |
| Temperature          | Observed temperature  | °F      | -250 .. 500 | 0       |
| Relative density     | At the reference conditions according to input 'Reference conditions'   | -       | 0..2        | 0       |
| Gross heating value  | At the combustion and reference conditions according to input 'Reference conditions'  | Btu/ft3 | 0..2500     | 0       |
| Nitrogen             |   | mol/mol | 0..1        | 0       |
| Carbon dioxide       |   | mol/mol | 0..1        | 0       |
| Hydrogen             |   | mol/mol | 0..1        | 0       |
| Method               | Calculation method:<br>1: All inputs are known<br>2: Unknown Nitrogen mole fraction<br>3: Unknown Carbon Dioxide mole fraction<br>4: Unknown Gross Heating Value<br>5: Unknown Relative Density   | -       |             | 0       |
| Reference conditions | Reference conditions that correspond with the values of inputs 'Relative density' and 'Gross heating value'.<br>Combustion temp. / metering temp. / pressure<br>1: 60°F / 60 °F / 14.73 psia<br>2: 60 °F / 60 °F / 1.01592 bar<br>Note: the calculations are based on 25°C / 0°C / 1.01325 bar(a). For the other conditions conversion factors are applied as specified in GERG Technical Monograph 5, Standard GERG Virial Equation, 1991.<br>Refer to section 'Calculations' for more details |         |             | 1       |

### Function outputs

| Function outputs       | Remark   | EU       | SW tag | Alarm                      | Fallback |
|------------------------|--|----------|--------|----------------------------|----------|
| Status                 | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence   |          | STS    | FIOOR<br>CALCERR<br>NOCONV |          |
| Compressibility factor |  | -        |        |                            | 1        |
| Molar mass             |  | lb/lbmol |        |                            | 0        |
| Range                  | 0: In Normal Range<br>All components are within the 'Normal Range'<br>1: In Extended Range<br>One or more components within the 'Extended Range', but none of the components outside the Extended rang (outputs values have higher uncertainty)<br>2: Out of Range<br>One or more components outside the 'Extended Range' (using the AGA8 calculation is not recommended in this case) |          | RANGE  | OOR                        | 0        |

Calculations

The calculations are in accordance with the standard.

As specified in the standard and depending on the selected reference conditions (input 'Reference conditions') one of the following set of conversions is carried out to obtain the input values of the relative density (RD) at 0°C and 1.01325 bar(a) and the gross heating value (GHV) at 25°C and 1.01325 bar(a) combustion and 0°C and 1.01325 bar(a) metering conditions.

| Input 'Reference Conditions'  | Multiply input GHV with | Multiply input RD with |
|-------------------------------|-------------------------|------------------------|
| 60 °F, 60 °F @ 14.73 psia     | 1.0543/26.85            | 1.0002                 |
| 60 °F, 60 °F @ 1.01592 bar(a) | 1.0543/26.86            | 1.0002                 |



## fxSGERG\_M

### Description

This function performs the SGERG calculation in **metric** units. The Standard (or Simplified) GERG TM5 1991 Virial Equation (SGERG or SGERG-88) has defines a method to calculate the Compressibility Factor (Z) for Natural Gases. The SGERG calculation is equivalent to the AGA8 Gross Characterisation Method, however .the results are slightly different. Instead of the full compositional analysis (as used by the AGA 8 Detailed Characterization method), the Gross Characterisation Method (SGERG) uses a restricted set of input variables for its equation, comprising Relative Density, Superior Calorific Value, Carbon Dioxide and Nitrogen together with pressure and temperature.

### Function inputs

| Function inputs      | Remark  | EU      | Range     | Default |
|----------------------|---|---------|-----------|---------|
| Name                 | Optional tag name, tag description and tag group  |         |           |         |
| Pressure             | Observed pressure   | bar(a)  | 0..2000   | 1.01325 |
| Temperature          | Observed temperature  | °C      | -200..300 | 0       |
| Relative density     | At the reference conditions according to input 'Reference conditions'   | -       | 0..2      | 0       |
| Gross heating value  | At the combustion and reference conditions according to input 'Reference conditions'  | MJ/m3   | 0..100    | 0       |
| Nitrogen             |   | mol/mol | 0..1      | 0       |
| Carbon dioxide       |   | mol/mol | 0..1      | 0       |
| Hydrogen             |   | mol/mol | 0..1      | 0       |
| Method               | Calculation method:<br>1: All inputs are known<br>2: Unknown Nitrogen mole fraction<br>3: Unknown Carbon Dioxide mole fraction<br>4: Unknown Gross Heating Value<br>5: Unknown Relative Density   | -       |           | 0       |
| Reference conditions | Reference conditions that correspond with the values of inputs 'Relative density' and 'Gross heating value'.<br>Combustion temp. / metering temp. / pressure<br>1: 25°C / 0 °C / 1.01325 bar(a)<br>2: 0 °C / 0 °C / 1.01325 bar(a)<br>3: 15 °C / 15 °C / 1.01325 bar(a)<br>Note: the calculations are based on 25°C / 0 °C / 1.01325 bar(a). For the other conditions conversion factors are applied as specified in GERG Technical Monograph 5, Standard GERG Virial Equation, 1991.<br>Refer to section 'Calculations' for more details |         |           | 1       |

### Function outputs

| Function outputs       | Remark  | EU      | SW tag | Alarm                      | Fallback |
|------------------------|---|---------|--------|----------------------------|----------|
| Status                 | 0: Normal<br>1: Input argument out of range<br>2: Calculation error<br>3: No convergence  |         | STS    | FLOOR<br>CALCERR<br>NOCONV |          |
| Compressibility factor |   | -       |        |                            | 1        |
| Molar mass             |   | kg/kmol |        |                            | 0        |
| Range                  | 0: In Normal Range<br>All components are within the 'Normal Range'<br>1: In Extended Range<br>One or more components within the 'Extended Range, but none of the components outside the Extended rang (outputs values have higher uncertainty)<br>2: Out of Range<br>One or more components outside the 'Extended Range' (using the AGA8 calculation is not recommended in this case) |         | RANGE  |                            | 0        |
|                        |   |         |        | OOOR                       |          |

### Calculations

The calculations are in accordance with the standard. As specified in the standard and depending on the selected reference conditions (input 'Reference conditions') one of the following set of conversions is carried out to obtain the input values of the relative density (RD) at 0 °C and 1.01325 bar(a) and the gross heating value (GHV) at 25 °C and 1.01325 bar(a)

### Compliance

- GERG Technical Monograph 5, Standard GERG Virial Equation, 1991

### Boundaries

The standard specifies a maximum uncertainty of the compressibility factor of 0.1% provided the inputs lie in the following range.

|                     |              |         |
|---------------------|--------------|---------|
| Pressure            | 0 .. 120     | bar(a)  |
| Temperature         | 265..335     | K       |
| Gross heating value | 19 .. 48     | MJ/m3   |
| Relative density    | 0.55 .. 0.90 | -       |
| Carbon dioxide      | 0.00 .. 0.30 | mol/mol |
| Nitrogen            | 0.00 .. 0.50 | mol/mol |
| Hydrogen            | 0.00 .. 0.10 | mol/mol |

combustion and 0 °C and 1.01325 bar(a) metering conditions.

| Input 'Reference Conditions'  | Multiply input GHV with | Multiply input RD with |
|-------------------------------|-------------------------|------------------------|
| 25 °C / 0 °C / 1.01325 bar(a) | Not applicable          | Not applicable         |
| 0 °C, 0 °C @ 1.01325 bar(a)   | 0.9974                  | Not applicable         |
| 15 °C, 15 °C @ 1.01325 bar(a) | 1.0543                  | 1.0002                 |

## fxSolartron\_Gas\_C

### Description

The function calculates the density from a frequency input signal provided by a Solartron 7810, 7811 or 7812 gas densitometer and corrects it for temperature and velocity of sound effects in **US customary** units.

The function requires that the calibration constants are based on the following units:

- Temperature °F
- Pressure psi
- Density g/cc

### Function inputs

| Function inputs          | Remark  | EU | SW tag  | Range          | Default |
|--------------------------|---|----|---------|----------------|---------|
| Name                     | Optional tag name, tag description and tag group  |    |         |                |         |
| Periodic time            | In microseconds<br>Equals 1000 divided by the frequency in [Hz]   | μs |         | 0..1e6         | 0       |
| Line temperature         | Used when temperature correction is enabled   | °F |         | -459.67..+1000 | 20      |
| Temperature correction   | 0: Disabled<br>1: Enabled   | -  | TEMPCOR |                | 1       |
| VOS correction           | 0: Disabled<br>1: Enabled   | -  | VOSCOR  |                | 1       |
| Reference temperature    | Used when temperature correction is enabled   | °F | REFTEMP | 0..200         | 60      |
| K0                       | Constant K0 from calibration certificate  | -  | K0      | -1e9..1e9      |         |
| K1                       | Constant K1 from calibration certificate  | -  | K1      | -1e9..1e9      |         |
| K2                       | Constant K2 from calibration certificate  | -  | K2      | -1e9..1e9      |         |
| K18                      | Constant K18 from calibration certificate   | -  | K18     | -1e9..1e9      |         |
| K19                      | Constant K19 from calibration certificate   | -  | K19     | -1e9..1e9      |         |
| K3                       | Constant K3 from calibration certificate  | -  | K3      | -1e9..1e9      |         |
| K4                       | Constant K4 from calibration certificate  | -  | K4      | -1e9..1e9      |         |
| Calibration gas constant | Constant Kc from calibration certificate  | -  | KC      | -1e9..1e9      |         |
| G value method           | Method of determining value G, which is the ratio of Gas Specific Gravity and the Ratio of Specific Heats<br>1: Use input 'G value'<br>2: Uses ratio of inputs<br>Uses the ratio of inputs 'Specific Gravity' and 'Ratio of Specific Heats' | -  | GMETHOD |                | 1       |
| G value                  | Value will be used when VOS correction is enabled and the G value method is 'Use input G value'   | -  | GVAL    |                |         |
| Specific gravity         | Value will be used when VOS correction is enabled and the G value method is 'Use ratio of inputs'   | -  | SG      | 0..2           | 0       |
| Ratio of specific heats  | Value will be used when VOS correction is enabled and the G value method is 'Use ratio of inputs'   | -  | CP_CV   | 0.01..10       | 0       |

### Function outputs

| Function outputs                  | Remark  | EU      | SW tag   | Alarm            | Fallback |
|-----------------------------------|---|---------|----------|------------------|----------|
| Status                            | 0: Normal<br>1: Input argument out of range<br>2: Calculation error |         | STS      | FLOOR<br>CALCERR |          |
| Corrected density                 | Density corrected for temperature and VOS                           | lbm/ft3 | CORDENS  |                  | 0        |
| Density corrected for temperature | Density corrected for temperature                                   | lbm/ft3 | TCORDENS |                  | 0        |
| Uncorrected density               | Uncorrected (indicated density)                                     | lbm/ft3 | UNCDEN   |                  | 0        |

### Calculations

Density calculations are performed in g/cc, while the function outputs are in lbm/ft3

The uncorrected density  $\rho_i$  is calculated by

$$\rho_i = K0 + K1 \cdot \tau + K2 \cdot \tau^2$$

### Compliance

The calculations are in accordance with documents:

- 78125010 'Solartron 7812 Gas Density Transducer Manual', 2001.
- 78125040 Rev. C, 'Micro Motion 7812 Gas Density Meter', October 2007.

Where:

|          |   |      |
|----------|---|------|
| $\rho_i$ | The uncorrected density                   | g/cc |
| K0       | Obtained from the calibration certificate | -    |
| K1       | Obtained from the calibration certificate | -    |
| K2       | Obtained from the calibration certificate | -    |
| $\tau$   | The time period in μs                     | μs   |

The temperature corrected density  $\rho_t$  is calculated by

$$\rho_t = \rho_i \cdot [1 + K18 \cdot (t - t_R)] + K19 \cdot (t - t_R)$$

Where:

|                            |   |      |
|----------------------------|---|------|
| <b><math>\rho_t</math></b> | The density corrected for temperature     | g/cc |
| <b>K18</b>                 | Obtained from the calibration certificate | -    |
| <b>K19</b>                 | Obtained from the calibration certificate | -    |
| <b>t</b>                   | The line temperature                      | °F   |
| <b>t<sub>R</sub></b>       | The reference temperature                 | °F   |

The density value corrected for Velocity of Sound is calculated as follows:

$$\rho_{VOS} = \rho_t \left[ 1 + \frac{K_3}{(\rho_t + K_4)} \cdot \left( Kc - \frac{G}{t + 273} \right) \right]$$

$$Kc = \frac{Cc}{t_c + 273}$$

Where:

|                                |  |      |
|--------------------------------|--|------|
| <b><math>\rho_{VOS}</math></b> | The density corrected for temperature and VOS  | g/cc |
| <b>K3</b>                      | Obtained from the calibration certificate  | -    |
| <b>K4</b>                      | Obtained from the calibration certificate  | -    |
| <b>Kc</b>                      | Calibration gas constant from the calibration certificate  | -    |
| <b>G</b>                       | G value.<br>Equals either input 'G value' or the ratio of inputs 'Specific gravity' and 'Ratio of specific heats', depending on input 'G value method' | -    |
| <b>t</b>                       | The line temperature   | °F   |
| <b>Cc</b>                      | Specific Gravity/Ratio of specific heats of calibration gas  | -    |
| <b>tc</b>                      | Calibration temperature  | °F   |

## fxSolartron\_Gas\_M

### Description

The function calculates the density from a frequency input signal provided by a Solartron 7810, 7811 or 7812 gas densitometer and corrects it for temperature and velocity of sound effects in **metric** units.

The function requires that the calibration constants are based on the following units:

- Temperature °C
- Pressure bar
- Density kg/m<sup>3</sup>

### Function inputs

| Function inputs          | Remark  | EU | SW tag  | Range      | Default      |
|--------------------------|---|----|---------|------------|--------------|
| Name                     | Optional tag name, tag description and tag group  |    |         |            |              |
| Periodic time            | In microseconds<br>Equals 1000 divided by the frequency in [Hz]   | μs |         | 0..1e6     | 0            |
| Line temperature         | Used when temperature correction is enabled   | °C |         | -273..+500 | 20           |
| Temperature correction   | 0: Disabled<br>1: Enabled   | -  | TEMPCOR |            | 1            |
| VOS correction           | 0: Disabled<br>1: Enabled   | -  | VOSCOR  |            | 1            |
| Reference temperature    | Used when temperature correction is enabled   | °C | REFTEMP | 0..100     | 20           |
| K0                       | Constant K0 from calibration certificate  | -  | K0      | -1e9..1e9  | -1.104252E+2 |
| K1                       | Constant K1 from calibration certificate  | -  | K1      | -1e9..1e9  | -1.882012E-2 |
| K2                       | Constant K2 from calibration certificate  | -  | K2      | -1e9..1e9  | 4.749797E-4  |
| K18                      | Constant K18 from calibration certificate   | -  | K18     | -1e9..1e9  | -1.360E-5    |
| K19                      | Constant K19 from calibration certificate   | -  | K19     | -1e9..1e9  | 8.440E-4     |
| K3                       | Constant K3 from calibration certificate  | -  | K3      | -1e9..1e9  | 354          |
| K4                       | Constant K4 from calibration certificate  | -  | K4      | -1e9..1e9  | 57.4         |
| Calibration gas constant | Constant Kc from calibration certificate  | -  | KC      | -1e9..1e9  | 0.00236      |
| G value method           | Method of determining value G, which is the ratio of Gas Specific Gravity and the Ratio of Specific Heats<br>1: Use input 'G value'<br>2: Uses ratio of inputs<br>Uses the ratio of inputs 'Specific Gravity' and 'Ratio of Specific Heats' | -  | GMETHOD |            | 1            |
| G value                  | Value will be used when VOS correction is enabled and the G value method is 'Use input G value'   | -  | GVAL    | 0..100     | 0            |
| Specific gravity         | Value will be used when VOS correction is enabled and the G value method is 'Use ratio of inputs'   | -  | SG      | 0..2       | 0            |
| Ratio of specific heats  | Value will be used when VOS correction is enabled and the G value method is 'Use ratio of inputs'   | -  | CP_CV   | 0..10      | 0            |

### Function outputs

| Function outputs                  | Remark  | EU                | SW tag   | Alarm            | Fallback |
|-----------------------------------|---|-------------------|----------|------------------|----------|
| Status                            | 0: Normal<br>1: Input argument out of range<br>2: Calculation error |                   | STS      | FLOOR<br>CALCERR |          |
| Corrected density                 | Density corrected for temperature and VOS                           | kg/m <sup>3</sup> | CORDENS  |                  | 0        |
| Density corrected for temperature | Density corrected for temperature                                   | kg/m <sup>3</sup> | TCORDENS |                  | 0        |
| Uncorrected density               | Uncorrected (indicated density)                                     | kg/m <sup>3</sup> | UNCDENS  |                  | 0        |

### Calculations

The uncorrected density  $\rho_i$  is calculated by

$$\rho_i = K0 + K1 \cdot \tau + K2 \cdot \tau^2$$

Where:

|          |   |                   |
|----------|---|-------------------|
| $\rho_i$ | The uncorrected density                   | kg/m <sup>3</sup> |
| K0       | Obtained from the calibration certificate | -                 |
| K1       | Obtained from the calibration certificate | -                 |
| K2       | Obtained from the calibration certificate | -                 |
| $\tau$   | The time period in μs                     | μs                |

### Compliance

The calculations are in accordance with documents:

- 78125010 'Solartron 7812 Gas Density Transducer Manual', 2001.
- 78125040 Rev. C, 'Micro Motion 7812 Gas Density Meter', October 2007.

The temperature corrected density  $\rho_t$  is calculated by

$$\rho_t = \rho_i \cdot [1 + K18 \cdot (t - t_R)] + K19 \cdot (t - t_R)$$

Where:

|                |   |                   |
|----------------|---|-------------------|
| $\rho_t$       | The density corrected for temperature     | kg/m <sup>3</sup> |
| K18            | Obtained from the calibration certificate | -                 |
| K19            | Obtained from the calibration certificate | -                 |
| t              | The line temperature                      | °C                |
| t <sub>R</sub> | The reference temperature                 | °C                |

The density value corrected for Velocity of Sound is calculated as follows:

$$\rho_{VOS} = \rho_t \left[ 1 + \frac{K_3}{(\rho_t + K_4)} \cdot \left( Kc - \frac{G}{t + 273} \right) \right]$$

$$Kc = \frac{Cc}{t_c + 273}$$

Where:

|                                |  |       |
|--------------------------------|--|-------|
| <b><math>\rho_{VOS}</math></b> | The density corrected for temperature and VOS  | kg/m3 |
| <b>K3</b>                      | Obtained from the calibration certificate  | -     |
| <b>K4</b>                      | Obtained from the calibration certificate  | -     |
| <b>Kc</b>                      | Calibration gas constant from the calibration certificate  | -     |
| <b>G</b>                       | G value.<br>Equals either input 'G value' or the ratio of inputs 'Specific gravity' and 'Ratio of specific heats', depending on input 'G value method' | -     |
| <b>t</b>                       | The line temperature   | °C    |
| <b>Cc</b>                      | Specific Gravity/Ratio of specific heats of calibration gas  | -     |
| <b>tc</b>                      | Calibration temperature  | °C    |

## fxSolartron\_Liquid\_C

### Description

The function calculates the density from a frequency input signal provided by a Solartron 7835, 7845, 7846 or 7847 liquid densitometer and corrects it for temperature, pressure and velocity of sound effects using **US Customary** units.

The function requires that the calibration constants are based on the following units:

- Temperature °F
- Pressure psi
- Density g/cc

### Function inputs

| Function inputs        | Remark  | EU      | Range         | Default |
|------------------------|---|---------|---------------|---------|
| Name                   | Optional tag name, tag description and tag group  |         |               |         |
| Periodic time          | In microseconds<br>Equals 1000 divided by the frequency in [Hz]   | μs      | 0..1e6        | 0       |
| Line temperature       | Used when temperature correction is enabled   | °F      | -459.67..+100 | 0       |
| Line pressure          | Used when pressure correction is enabled  | psig    | 0..3000       | 0       |
| Temperature correction | 0: Disabled<br>1: Enabled   | -       |               | 1       |
| Pressure correction    | 0: Disabled<br>1: Enabled   | -       |               | 1       |
| VOS correction         | 0: Disabled<br>1: Based on Kr / Kj Constants<br>Solartron manual edition 1985<br>2: Based on VOS value<br>Solartron manual edition 1996 and later | -       |               | 2       |
| Reference temperature  | Used when temperature correction is enabled   | °F      | 0..200        | 60      |
| Reference pressure     | Used when pressure correction is enabled  | psig    | 0..1500       | 0       |
| K0                     | Constant from calibration certificate   | -       | -1e9..1e9     |         |
| K1                     | Constant from calibration certificate   | -       | -1e9..1e9     |         |
| K2                     | Constant from calibration certificate   | -       | -1e9..1e9     |         |
| K18                    | Constant from calibration certificate   | -       | -1e9..1e9     |         |
| K19                    | Constant from calibration certificate   | -       | -1e9..1e9     |         |
| K20A                   | Constant from calibration certificate   | -       | -1e9..1e9     |         |
| K20B                   | Constant from calibration certificate   | -       | -1e9..1e9     |         |
| K21A                   | Constant from calibration certificate   | -       | -1e9..1e9     |         |
| K21B                   | Constant from calibration certificate   | -       | -1e9..1e9     |         |
| Kr                     | Used when VOS method is set to 'Based on Kr / Kj Constants'.<br>Constant needs to be obtained from Solartron                                      | -       |               |         |
| Kj                     | Used when VOS method is set to 'Based on Kr / Kj Constants'.<br>Constant needs to be obtained from Solartron                                      | lbm/ft3 |               |         |
| Liquid VOS             | Velocity of sound of liquid<br>Used when VOS method is set to 'Based on VOS value'  | ft/s    |               |         |

### Function outputs

| Function outputs                               | Remark  | EU      | SW tag    | Alarm            | Fallback |
|--|---|---------|-----------|------------------|----------|
| Status   | 0: Normal<br>1: Input argument out of range<br>2: Calculation error |         | STS       | FLOOR<br>CALCERR |          |
| Corrected density                              | Density corrected for temperature, pressure and VOS                 | lbm/ft3 | CORDENS   |                  | 0        |
| Density corrected for temperature              |   | lbm/ft3 | TCORDENS  |                  | 0        |
| Density corrected for temperature and pressure |   | lbm/ft3 | PTCORDENS |                  | 0        |
| Uncorrected density                            |   | lbm/ft3 | UNCORDENS |                  | 0        |

### Calculations

Density calculations are performed in g/cc and m/s, while the function inputs and outputs are in lbm/ft3 and ft/s

The indicated density  $\rho_i$  is calculated by

$$\rho_i = K0 + K1 \cdot \tau + K2 \cdot \tau^2$$

### Compliance

The calculations are in accordance with documents:

- 78355010 'Solartron 7835, 7845, 7846 & 7847 Advanced Liquid Density Transducer Manual', 2001
- 78355080, Rev. C, 'Micro Motion 7835, 7845, 7846 & 7847 Liquid Density Transducer', October 2007

Where:

|          |   |      |
|----------|---|------|
| $\rho_i$ | The indicated density                     | g/cc |
| K0       | Obtained from the calibration certificate | -    |
| K1       | Obtained from the calibration certificate | -    |
| K2       | Obtained from the calibration certificate | -    |
| $\tau$   | The time period in μs                     | μs   |

The temperature corrected density  $\rho_t$  is calculated by

$$\rho_t = [\rho_i \cdot [1 + K18 \cdot (t - t_R)]] + K19 \cdot (t - t_R)$$

Where:

|          |   |      |
|----------|---|------|
| $\rho_t$ | The density corrected for temperature     | g/cc |
| K18      | Obtained from the calibration certificate | -    |
| K19      | Obtained from the calibration certificate | -    |
| t        | The line temperature                      | °F   |
| $t_R$    | The reference temperature                 | °F   |

The pressure and temperature corrected density  $\rho_{pt}$  is calculated by

$$\rho_{pt} = [\rho_t \cdot [1 + K20 \cdot (p - p_{REF})]] + K21 \cdot (p - p_{REF})$$

$$K20 = K20A + K20B \cdot (p - p_{REF})$$

$$K21 = K21A + K21B \cdot (p - p_{REF})$$

Where:

|             |  |      |
|-------------|--|------|
| $\rho_{pt}$ | The density corrected for pressure and temperature | g/cc |
| K20A        | Obtained from the calibration certificate          | -    |
| K20B        | Obtained from the calibration certificate          | -    |
| K21A        | Obtained from the calibration certificate          | -    |
| K21B        | Obtained from the calibration certificate          | -    |
| p           | The line pressure                                  | psig |
| $p_R$       | The reference pressure                             | psig |

When 'VOS Correction' is set to 'Based on Kr and Kj Constants' the following correction for velocity of sound is applied:

$$\rho_{VOS} = \rho_{pt} + K_r \cdot (\rho_{pt} - K_j)^3$$

When 'VOS Correction' is set to 'Based on VOS value', the following correction for velocity of sound is applied:

$$\rho_{VOS} = \rho_{pt} \cdot \left[ 1 + \frac{1.4e^6}{1000 \cdot \rho_{pt} + 1.4} \cdot \left( \frac{1}{V_C^2} + \frac{1}{V_A^2} \right) \right]$$

When  $0.3 \leq \rho_{pt} \leq 1.1$ :

$$V_C = (100 + 1455 \cdot \rho_{pt})$$

When  $1.1 < \rho_{pt} \leq 1.6$ :

$$V_C = 2690 - 900 \cdot \rho_{pt}$$

Else ( $\rho_{pt} < 0.3$  or  $\rho_{pt} > 1.4$ ) the VOS of sound correction is not performed.

Where:

|              |                                       |      |
|--------------|---------------------------------------|------|
| $\rho_{vos}$ | The density corrected for temperature | g/cc |
| $K_r$        | Constant obtained from Solartron      | -    |
| $K_j$        | Constant obtained from Solartron      | g/cc |
| $V_C$        | Calibration VOS                       | m/s  |
| $V_A$        | Liquid VOS                            | m/s  |

## fxSolartron\_Liquid\_M

The function calculates the density from a frequency input signal provided by a Solartron 7835, 7845, 7846 or 7847 liquid densitometer and corrects it for temperature, pressure and velocity of sound effects using **metric** units.

The function requires that the calibration constants are based on the following units:

- Temperature °C
- Pressure bar
- Density kg/m<sup>3</sup>

### Function inputs

| Function inputs        | Remark  | EU                | Range         | Default     |
|------------------------|---|-------------------|---------------|-------------|
| Name                   | Optional tag name, tag description and tag group  |                   |               |             |
| Periodic time          | In microseconds<br>Equals 1000 divided by the frequency in [Hz]   | µs                | 0..1e6        | 0           |
| Line temperature       | Used when temperature correction is enabled   | °C                | -273.15..+500 | 0           |
| Line pressure          | Used when pressure correction is enabled  | bar(g)            | 0..200        | 0           |
| Temperature correction | 0: Disabled<br>1: Enabled   | -                 |               | 1           |
| Pressure correction    | 0: Disabled<br>1: Enabled   | -                 |               | 1           |
| VOS correction         | 0: Disabled<br>1: Based on Kr / Kj Constants<br>Solartron manual edition 1985<br>2: Based on VOS value<br>Solartron manual edition 1996 and later | -                 |               | 2           |
| Reference temperature  | Used when temperature correction is enabled   | °C                | 0..100        | 20          |
| Reference pressure     | Used when pressure correction is enabled  | bar(g)            | 0..100        | 0           |
| K0                     | Constant from calibration certificate   | -                 | -1e9..1e9     | 1.7418E2    |
| K1                     | Constant from calibration certificate   | -                 | -1e9..1e9     | -1.10493e0  |
| K2                     | Constant from calibration certificate   | -                 | -1e9..1e9     | 3.703268e-4 |
| K18                    | Constant from calibration certificate   | -                 | -1e9..1e9     | -6.415e-4   |
| K19                    | Constant from calibration certificate   | -                 | -1e9..1e9     | -5.674e-1   |
| K20A                   | Constant from calibration certificate   | -                 | -1e9..1e9     | 2.888e-4    |
| K20B                   | Constant from calibration certificate   | -                 | -1e9..1e9     | -5.581e-6   |
| K21A                   | Constant from calibration certificate   | -                 | -1e9..1e9     | -4.467e-1   |
| K21B                   | Constant from calibration certificate   | -                 | -1e9..1e9     | -8.633e-3   |
| Kr                     | Used when VOS method is set to 'Based on Kr / Kj Constants'.<br>Constant needs to be obtained from Solartron                                      | -                 | -1..+1        | 0.0         |
| Kj                     | Used when VOS method is set to 'Based on Kr / Kj Constants'.<br>Constant needs to be obtained from Solartron                                      | kg/m <sup>3</sup> | 0..2000       | 0.0         |
| Liquid VOS             | Velocity of sound of liquid<br>Used when VOS method is set to 'Based on VOS value'  | m/s               | 0..2000       | 0.0         |

### Function outputs

| Function outputs                               | Remark  | EU                | SW tag    | Alarm            | Fallback |
|--|---|-------------------|-----------|------------------|----------|
| Status   | 0: Normal<br>1: Input argument out of range<br>2: Calculation error                                     |                   | STS       | FLOOR<br>CALCERR |          |
| Corrected density                              | Density corrected for temperature, pressure and VOS<br>(provided that particular correction is enabled) | kg/m <sup>3</sup> | CORDENS   |                  | 0        |
| Density corrected for temperature              |   | kg/m <sup>3</sup> | TCORDENS  |                  | 0        |
| Density corrected for temperature and pressure |   | kg/m <sup>3</sup> | PTCORDENS |                  | 0        |
| Uncorrected density                            |   | kg/m <sup>3</sup> | UNCDENS   |                  | 0        |

### Calculations

The indicated density  $\rho_i$  is calculated by

$$\rho_i = K0 + K1 \cdot \tau + K2 \cdot \tau^2$$

### Compliance

The calculations are in accordance with documents:

- 78355010 'Solartron 7835, 7845, 7846 & 7847 Advanced Liquid Density Transducer Manual', 2001
- 78355080, Rev. C, 'Micro Motion 7835, 7845, 7846 & 7847 Liquid Density Transducer', October 2007

Where:

|          |   |                   |
|----------|---|-------------------|
| $\rho_i$ | The indicated density                     | kg/m <sup>3</sup> |
| K0       | Obtained from the calibration certificate | -                 |
| K1       | Obtained from the calibration certificate | -                 |
| K2       | Obtained from the calibration certificate | -                 |
| $\tau$   | The time period in µs                     | µs                |



The temperature corrected density  $\rho_t$  is calculated by

$$\rho_t = [\rho_i \cdot [1 + K18 \cdot (t - t_R)]] + K19 \cdot (t - t_R)$$

Where:

|                      |   |       |
|----------------------|---|-------|
| $\rho_t$             | The density corrected for temperature     | kg/m3 |
| <b>K18</b>           | Obtained from the calibration certificate | -     |
| <b>K19</b>           | Obtained from the calibration certificate | -     |
| <b>t</b>             | The line temperature                      | °C    |
| <b>t<sub>R</sub></b> | The reference temperature                 | °C    |

The pressure and temperature corrected density  $\rho_{pt}$  is calculated by

$$\rho_{pt} = [\rho_t \cdot [1 + K20 \cdot (p - p_{REF})]] + K21 \cdot (p - p_{REF})$$

$$K20 = K20A + K20B \cdot (p - p_{REF})$$

$$K21 = K21A + K21B \cdot (p - p_{REF})$$

Where:

|                      |  |        |
|----------------------|--|--------|
| $\rho_{pt}$          | The density corrected for pressure and temperature | kg/m3  |
| <b>K20A</b>          | Obtained from the calibration certificate          | -      |
| <b>K20B</b>          | Obtained from the calibration certificate          | -      |
| <b>K21A</b>          | Obtained from the calibration certificate          | -      |
| <b>K21B</b>          | Obtained from the calibration certificate          | -      |
| <b>p</b>             | The line pressure                                  | bar(g) |
| <b>p<sub>R</sub></b> | The reference pressure                             | bar(g) |

When 'VOS Correction' is set to 'Based on Kr and Kj Constants' the following correction for velocity of sound is applied:

$$\rho_{VOS} = \rho_{pt} + K_r \cdot (\rho_{pt} - K_j)^3$$

When 'VOS Correction' is set to 'Based on VOS value', the following correction for velocity of sound is applied:

$$\rho_{VOS} = \rho_{pt} \cdot \left[ 1 + \frac{1.4e^6}{\rho_{pt} + 1400} \cdot \left( \frac{1}{V_C^2} - \frac{1}{V_A^2} \right) \right]$$

When  $300 \leq \rho_{pt} \leq 1100$ :

$$V_C = 100 + 1.455 \cdot \rho_{pt}$$

When  $1100 < \rho_{pt} \leq 1600$ :

$$V_C = 2690 - 0.9 \cdot \rho_{pt}$$

Else ( $\rho_{pt} < 300$  or  $\rho_{pt} > 1600$ ) the VOS of sound correction is not performed.

Where:

|                      |                                       |       |
|----------------------|---------------------------------------|-------|
| $\rho_{vos}$         | The density corrected for temperature | kg/m3 |
| <b>K<sub>r</sub></b> | Constant obtained from Solartron      | -     |
| <b>K<sub>j</sub></b> | Constant obtained from Solartron      | kg/m3 |
| <b>V<sub>C</sub></b> | Calibration VOS                       | m/s   |
| <b>V<sub>A</sub></b> | Liquid VOS                            | m/s   |

## fxSolartron\_SG

### Description

The function calculates the specific gravity from a frequency input signal provided by a Solartron 3096 or 3098 Specific Gravity transducer.

### Compliance

The calculations are in accordance with documents:

- 30985020 'Solartron 3098 Gas Specific Gravity Transducer Manual', 2001
- 30985020, Rev. B, 'Micro Motion 3098 Gas Specific Gravity Meter', October 2007

### Function input

| Function inputs | Remark  | EU | SW tag | Range     | Default     |
|-----------------|---|----|--------|-----------|-------------|
| Name            | Optional tag name, tag description and tag group                |    |        |           |             |
| Periodic time   | In microseconds<br>Equals 1000 divided by the frequency in [Hz] | μs |        | 0..1e6    | 0           |
| K0              | Constant from calibration certificate                           | -  | K0     | -10000..0 | -11.952     |
| K2              | Constant from calibration certificate                           | -  | K2     | 0..1      | 4.719593e-5 |

### Function output

| Function outputs | Remark   | EU | SW tag | Alarm            | Fallback |
|------------------|--|----|--------|------------------|----------|
| Status           | 0: Normal<br>1: Input argument out of range<br>2: Calculation error  |    | STS    | FLOOR<br>CALCERR |          |
| Specific Gravity | Ratio of the molecular weight of the gas (mixture) to that of the molecular weight of dry air (i.e. the ideal Specific Gravity). | -  | SG     |                  | 0        |

### Calculations

The specific gravity is calculated by

$$SG = K0 + K2 \cdot \tau^2$$

Where:

|           |   |    |
|-----------|---|----|
| <b>SG</b> | Specific gravity                          | -  |
| <b>τ</b>  | Periodic time                             | μs |
| <b>K0</b> | Obtained from the calibration certificate | -  |
| <b>K2</b> | Obtained from the calibration certificate | -  |

If the calibration certificate contains factors Gx, Gy, tx and ty then K2 must be calculated as follows:

$$K2 = \frac{Gx - Gy}{t_x^2 - t_y^2}$$

Where:

|           |                                       |    |
|-----------|---------------------------------------|----|
| <b>Gx</b> | Specific gravity of calibration gas x | -  |
| <b>Gy</b> | Specific gravity of calibration gas y | -  |
| <b>tx</b> | Periodic time of calibration gas x    | μs |
| <b>ty</b> | Periodic time of calibration gas y    | μs |

## fxUGC\_C

### Description

The function calculates the density from a frequency input signal provided by a UGC densitometer and corrects it for temperature and pressure effects in **US customary** units.

Note: Calibration constants also need to be in US customary units.

### Function input

| Function inputs        | Remark  | EU   | SW tag  | Range          | Default |
|------------------------|---|------|---------|----------------|---------|
| Name                   | Optional tag name, tag description and tag group                |      |         |                |         |
| Periodic time          | In microseconds<br>Equals 1000 divided by the frequency in [Hz] | μs   |         | 0..1e6         |         |
| Line temperature       | Used when temperature correction is enabled                     | °F   |         | -459.67..+1000 |         |
| Line pressure          | Used when pressure correction is enabled                        | psig |         | 0..3000        |         |
| Temperature correction | 0: Disabled<br>1: Enabled                                       | -    | TEMPCOR |                | 1       |
| Pressure correction    | 0: Disabled<br>1: Enabled                                       | -    | PRESCOR |                | 1       |
| Reference temperature  | Used when temperature correction is enabled                     | °F   | REFTEMP | 0..200         | 60      |
| Reference pressure     | Used when pressure correction is enabled                        | psig | REFPRES | 0..1500        | 0       |
| K0                     | Constant K0 from calibration certificate                        | -    | K0      | -1e9..1e9      |         |
| K1                     | Constant K1 from calibration certificate                        | -    | K1      | -1e9..1e9      |         |
| K2                     | Constant K2 from calibration certificate                        | -    | K2      | -1e9..1e9      |         |
| KT1                    | Constant KT1 from calibration certificate                       |      | KT1     | -1e9..1e9      |         |
| KT2                    | Constant KT2 from calibration certificate                       |      | KT2     | -1e9..1e9      |         |
| KT3                    | Constant KT3 from calibration certificate                       |      | KT3     | -1e9..1e9      |         |
| KP1                    | Constant KP1 from calibration certificate                       |      | KP1     | -1e9..1e9      |         |
| KP2                    | Constant KP2 from calibration certificate                       |      | KP2     | -1e9..1e9      |         |
| KP3                    | Constant KP3 from calibration certificate                       |      | KP3     | -1e9..1e9      |         |

### Function output

| Function outputs    | Remark   | EU      | SW tag  | Alarm         | Fallback |
|---------------------|--|---------|---------|---------------|----------|
| Status              | 0: Normal (No error condition)<br>1: Input argument out of range<br>2: Calculation error |         | STS     | FLOOR<br>CALC |          |
| Corrected density   | Density corrected for temperature and pressure   | lbm/ft3 | CORDENS |               | 0        |
| Uncorrected density | Uncorrected (indicated) density  | lbm/ft3 | UNCDENS |               | 0        |

### Calculations

The uncorrected density  $\rho_i$  is calculated by

$$\rho_i = K0 + K1 \cdot \tau + K2 \cdot \tau^2$$

Where:

|          |   |         |
|----------|---|---------|
| $\rho_i$ | The uncorrected density                   | lbm/ft3 |
| K0       | Obtained from the calibration certificate | -       |
| K1       | Obtained from the calibration certificate | -       |
| K2       | Obtained from the calibration certificate | -       |
| $\tau$   | The time period in μs                     | μs      |

The temperature and pressure corrected density  $\rho_t$  is calculated by

$$\rho_t = \rho_i + [K_{P1} + K_{P2} \cdot \rho_i + K_{P3} \cdot \rho_i^2] \cdot (p - p_R) + [K_{T1} + K_{T2} \cdot \rho_i + K_{T3} \cdot \rho_i^2] \cdot (t - t_R)$$

Where:

|                 |  |         |
|-----------------|--|---------|
| $\rho_t$        | The density corrected for temperature and pressure | lbm/ft3 |
| K <sub>P1</sub> | Obtained from the calibration certificate          | -       |
| K <sub>P2</sub> | Obtained from the calibration certificate          | -       |
| K <sub>P3</sub> | Obtained from the calibration certificate          | -       |
| K <sub>T1</sub> | Obtained from the calibration certificate          | -       |
| K <sub>T2</sub> | Obtained from the calibration certificate          | -       |
| K <sub>T3</sub> | Obtained from the calibration certificate          | -       |
| t               | The line temperature                               | °F      |
| t <sub>R</sub>  | The reference temperature                          | °F      |
| p               | The line pressure                                  | psig    |
| p <sub>R</sub>  | The reference pressure                             | psig    |

## fxUGC\_M

### Description

The function calculates the density from a frequency input signal provided by a UGC densitometer and corrects it for temperature and pressure effects in **metric** units. Calibration constants also need to be in metric units.

### Function input

| Function inputs        | Remark  | EU     | SW tag  | Range         | Default |
|------------------------|---|--------|---------|---------------|---------|
| Name                   | Optional tag name, tag description and tag group                |        |         |               |         |
| Periodic time          | In microseconds<br>Equals 1000 divided by the frequency in [Hz] | μs     |         | 0..1e6        |         |
| Line temperature       | Used when temperature correction is enabled                     | °C     |         | -273.15..+500 |         |
| Line pressure          | Used when pressure correction is enabled                        | bar(g) |         | 0..200        |         |
| Temperature correction | 0: Disabled<br>1: Enabled                                       | -      | TEMPCOR |               | 1       |
| Pressure correction    | 0: Disabled<br>1: Enabled                                       | -      | PRESOR  |               | 1       |
| Reference temperature  | Used when temperature correction is enabled                     | °C     | REFTEMP | 0..100        | 20      |
| Reference pressure     | Used when pressure correction is enabled                        | bar(g) | REFPRES | 0..100        | 0       |
| K0                     | Constant K0 from calibration certificate                        | -      | K0      | -1e9..1e9     |         |
| K1                     | Constant K1 from calibration certificate                        | -      | K1      | -1e9..1e9     |         |
| K2                     | Constant K2 from calibration certificate                        | -      | K2      | -1e9..1e9     |         |
| KT1                    | Constant KT1 from calibration certificate                       |        | KT1     | -1e9..1e9     |         |
| KT2                    | Constant KT2 from calibration certificate                       |        | KT2     | -1e9..1e9     |         |
| KT3                    | Constant KT3 from calibration certificate                       |        | KT3     | -1e9..1e9     |         |
| KP1                    | Constant KP1 from calibration certificate                       |        | KP1     | -1e9..1e9     |         |
| KP2                    | Constant KP2 from calibration certificate                       |        | KP2     | -1e9..1e9     |         |
| KP3                    | Constant KP3 from calibration certificate                       |        | KP3     | -1e9..1e9     |         |

### Function output

| Function outputs    | Remark   | EU    | SW tag  | Alarm         | Fallback |
|---------------------|--|-------|---------|---------------|----------|
| Status              | 0: Normal (No error condition)<br>1: Input argument out of range<br>2: Calculation error |       | STS     | FIOOR<br>CALC |          |
| Corrected density   | Density corrected for temperature and pressure   | kg/m3 | CORDENS |               | 0        |
| Uncorrected density | Uncorrected (indicated) density  | kg/m3 | UNCDENS |               | 0        |

### Calculations

The uncorrected density  $\rho_i$  is calculated by

$$\rho_i = K0 + K1 \cdot \tau + K2 \cdot \tau^2$$

Where:

|          |   |       |
|----------|---|-------|
| $\rho_i$ | The uncorrected density                   | kg/m3 |
| K0       | Obtained from the calibration certificate | -     |
| K1       | Obtained from the calibration certificate | -     |
| K2       | Obtained from the calibration certificate | -     |
| $\tau$   | The time period in μS                     | μS    |

The temperature and pressure corrected density  $\rho_t$  is calculated by

$$\rho_t = \rho_i + [K_{P1} + K_{P2} \cdot \rho_i + K_{P3} \cdot \rho_i^2] \cdot (p - p_R) + [K_{T1} + K_{T2} \cdot \rho_i + K_{T3} \cdot \rho_i^2] \cdot (t - t_R)$$

Where:

|                 |  |        |
|-----------------|--|--------|
| $\rho_t$        | The density corrected for temperature and pressure | kg/m3  |
| K <sub>P1</sub> | Obtained from the calibration certificate          | -      |
| K <sub>P2</sub> | Obtained from the calibration certificate          | -      |
| K <sub>P3</sub> | Obtained from the calibration certificate          | -      |
| K <sub>T1</sub> | Obtained from the calibration certificate          | -      |
| K <sub>T2</sub> | Obtained from the calibration certificate          | -      |
| K <sub>T3</sub> | Obtained from the calibration certificate          | -      |
| t               | The line temperature                               | °C     |
| t <sub>R</sub>  | The reference temperature                          | °C     |
| p               | The line pressure                                  | bar(g) |
| p <sub>R</sub>  | The reference pressure                             | bar(g) |

## fxVCone\_C

### Description

This function calculates the mass flow rate for a measured differential pressure over a McCrometer V-Cone meter in U.S. customary units.

The calculation, as specified by the meter supplier, is essentially a modified ISO 5167 flow rate calculation. As opposed to ISO-5167 the discharge coefficient is a function input. Because the discharge coefficient is a function of Reynolds number an optional calibration correction needs to be applied outside this function.

### Function inputs

| Function inputs            | Remark  | EU           | Range               | Default |
|----------------------------|---|--------------|---------------------|---------|
| Name                       | Optional tag name, tag description and tag group  |              |                     |         |
| Differential Pressure      | Differential pressure over the V-Cone device measured at the up- and downstream pressure taps   | inH2O @ 60°F | 0..100              | 0       |
| Pressure                   | Upstream pressure value of the fluid at metering conditions   | psia         | 0..30000            | 0       |
| Temperature                | Down- or upstream temperature of the fluid at metering conditions   | °F           | -400 ..2000         | 0       |
| Density                    | Down or upstream density of the fluid at metering conditions  | lbm/ft3      | 0..200              | 0       |
| Dynamic Viscosity          | Dynamic viscosity of the fluid  | lbm/ft.s     | 0..10               | 6.9e-6  |
| Isentropic Exponent        | Also referred to as $\kappa$ (kappa). For an ideal gas this coefficient is equal to the ratio of the specific heat capacity at constant pressure to the specific heat at constant volume. According to the ISO standard this ratio may be used, when the real value is unknown.   | -            | 0..10               | 1.3     |
| Pipe Diameter              | Internal diameter of the pipe at reference temperature  | inches       | 0..100              | 0       |
| Pipe Expansion factor      | The thermal expansion coefficient of the pipe material  | 1/°F         | 0..1e-4             | 6.2e-6  |
| Pipe Reference temperature | The reference temperature that corresponds to the 'Pipe diameter' input value   | °F           | -400..2000          | 68      |
| Cone Diameter              | Cone diameter at reference temperature  | inches       | 0.. 'Pipe Diameter' | 0       |
| Cone Expansion factor      | The thermal expansion coefficient of the Cone material  | 1/°F         | 0..1e-4             | 9.25e-6 |
| Cone Reference Temperature | The reference temperature that corresponds to the 'Cone diameter' input value   | °F           | -400 ..2000         | 68      |
| Configuration              | The type of McCrometer V-Cone meter.<br>This setting is used to select the appropriate equation for determination of the gas expansion factor as specified by McCrometer<br>1: Standard V-Cone<br>2: Wafer-Cone<br>Note of input 'Fluid' is set to 'Liquid', then this input is not used (because the expansion factor is set to 1)   | -            |                     | 1       |
| Pressure Location          | 1: Upstream<br>Input 'Pressure' represents the pressure at the upstream pressure tapping ( $p_1$ ).<br>Since the absolute pressure is usually measured at the upstream tapping this is the most common setting.<br>2: Downstream<br>Input 'Pressure' represents the pressure at the downstream tapping ( $p_2$ ).   | -            |                     | 1       |
| Temperature Location       | 1: Upstream<br>Input 'Temperature' represents the upstream temperature ( $t_1$ ).<br>2: Downstream<br>Input 'Temperature' represents the temperature at the downstream tapping ( $t_2$ ).<br>3: Recovered<br>Input 'Temperature' represents the downstream temperature at a location where the pressure has fully recovered ( $t_3$ ).<br>Since temperature measurement is usually downstream of the flow device this is the most common setting.   | -            |                     | 2       |
| Temperature Correction     | This parameter specifies if and how the temperature should be corrected from downstream to upstream conditions (or vice versa)<br>1: $(1-\kappa)/\kappa$<br>Isentropic expansion using $(1-\kappa)/\kappa$ as the temperature referral exponent<br>2: Constant<br>Isentropic expansion using input 'Temperature Exponent' as the temperature referral exponent [-]<br>3: Joule Thomson<br>Isenthalpic expansion using input 'Temperature Exponent' as the Joule Thomson coefficient [°F/psi].<br>This method is prescribed by ISO5167-1:2003. |              |                     | 1       |
| Temperature Exponent       | Refer to input Temperature Correction<br>Unit depends on input Temperature Correction value   | -<br>°F/psi  |                     | 0       |
| Density Location           | This parameter specifies if and how the density should be corrected from downstream to upstream conditions (or vice versa).<br>1: Upstream  | -            |                     | 1       |

### Compliance

- McCrometer: Flow Calculations for the V-Cone Flow meter Literature part #24509-54 Rev 3.1/02-05 2005

| Function inputs       | Remark   | EU | Range | Default |
|-----------------------|--|----|-------|---------|
|                       | Input 'Density' represents the density at the upstream pressure tapping ( $\rho_1$ ).<br>2: Downstream<br>Input 'Density' represents the density at the downstream tapping ( $\rho_2$ ).<br>3: Recovered<br>Input 'Density' represents the density downstream at a location Where the pressure has fully recovered ( $\rho_3$ ). |    |       |         |
| Density Exponent.     | This factor is used when density correction is enabled. The formula $1/\kappa$ will be used when the input value is set to 0, else the input value will be used.<br>For more details refer to section 'Density correction'.  | -  |       | 0       |
| Fluid                 | The type of fluid being measured<br>1: Gas<br>2: Liquid  | -  |       | 1       |
| Discharge coefficient | The McCrometer reference document states that the discharge coefficient is a function of Reynolds number. A calibration correction needs to be implemented through an additional function and input 'Discharge coefficient' needs to be linked to the corresponding output of this additional function.                          | -  | 0..2  | 0.85    |

### Function outputs

| Function outputs                  | Remark  | EU      | Fallback                                     |
|-----------------------------------|---|---------|--|
| Status                            | 0: Normal (No error condition)<br>1: Input argument out of range<br>2: No convergence   |         |  |
| Mass flow rate                    | The calculated mass flow rate   | klbm/hr | 0  |
| Beta ratio                        | Cone to pipe diameter ratio at upstream temperature   | -       | Input Cone diameter /<br>Input Pipe diameter |
| Cone diameter                     | At the upstream temperature   | inches  | Input Cone diameter                          |
| Pipe diameter                     | At the upstream temperature   | inches  | Input Pipe diameter                          |
| Upstream pressure                 | Pressure at upstream tapping ( $p_1$ )  | psia    | Input Pressure                               |
| Pressure at downstream tapping    | Pressure at downstream tapping ( $p_2$ )  | psia    | Input Pressure                               |
| Recovered downstream pressure     | Fully recovered downstream pressure ( $p_3$ )   | psia    | Input Pressure                               |
| Upstream temperature              | Temperature at upstream tapping ( $t_1$ )   | °F      | Input Temperature                            |
| Temperature at downstream tapping | Temperature at downstream tapping ( $t_2$ )   | °F      | Input Temperature                            |
| Downstream Temperature            | 'Fully recovered' downstream temperature ( $t_3$ )  | °F      | Input Temperature                            |
| Upstream density                  | Density at upstream tapping ( $\rho_1$ )  | lbm/ft3 | Input Density                                |
| Density at downstream tapping     | Pressure at downstream tapping ( $\rho_2$ )   | lbm/ft3 | Input Density                                |
| Downstream density                | 'Fully recovered' downstream density ( $\rho_3$ )   | lbm/ft3 | Input Density                                |
| Reynolds number                   |   | -       | 0  |
| Discharge coefficient             | Same as input value   | -       |  |
| Expansion Factor                  |   | -       | 0  |
| Velocity                          | Pipeline velocity   | Ft/s    | 0  |
| Expansion Factor Range            | The McCrometer reference document states that for gas applications the expansion factor should not get below 0.84<br>0: Expansion factor is in valid range<br>1: Expansion factor is out of valid range | -       | 0  |

### Calculations

The flow calculation is as specified in the McCrometer reference document.

The downstream to upstream correction (and vice versa) for pressure, temperature and density are as specified for function 'ASME MFC-3M Orifice'.

## fxVCone\_M

### Description

This function calculates the mass flow rate for a measured differential pressure over a McCrometer V-Cone meter in metric units.

The calculation, as specified by the meter supplier, is essentially a modified ISO 5167 flow rate calculation. As opposed to ISO-5167 the discharge coefficient is a function input. Because the discharge coefficient is a function of Reynolds number an optional calibration correction needs to be applied outside this function.

### Compliance

- McCrometer: Flow Calculations for the V-Cone Flow meter Literature part #24509-54 Rev 3.1/02-05 2005

## Function inputs

| Function inputs            | Remark  | EU          | Range        | Default   |
|----------------------------|---|-------------|--------------|-----------|
| Name                       | Optional tag name, tag description and tag group  |             |              |           |
| Differential Pressure      | Differential pressure over the V-Cone device measured at the up- and downstream pressure taps   | mbar        | 0..2000      | 0         |
| Pressure                   | Upstream pressure value of the fluid at metering conditions   | bar(a)      | 0..2000      | 0         |
| Temperature                | Down- or upstream temperature of the fluid at metering conditions   | °C          | -240..1000   | 0         |
| Density                    | Down or upstream density of the fluid at metering conditions  | kg/m3       | 0..2000      | 0         |
| Dynamic Viscosity          | Dynamic viscosity of the fluid  | Pa.s        | 0..1         | 0.01115   |
| Isentropic Exponent        | Also referred to as $\kappa$ (kappa). For an ideal gas this coefficient is equal to the ratio of the specific heat capacity at constant pressure to the specific heat at constant volume. According to the ISO standard this ratio may be used, when the real value is unknown.   | -           | 0..2         | 0         |
| Pipe Diameter              | Internal diameter of the pipe at reference temperature  | mm          | 0..2000      | 0         |
| Pipe Expansion factor      | The thermal expansion coefficient of the pipe material  | 1/°C        | 0..1         | 0.0000108 |
| Pipe Reference temperature | The reference temperature that corresponds to the 'Pipe diameter' input value   | °C          | -240..1000   | 20        |
| Cone Diameter              | Cone diameter at reference temperature  | mm          | 0            | 0         |
| Cone Expansion factor      | The thermal expansion coefficient of the Cone material  | 1/°C        |              | 0.0000163 |
| Cone Reference Temperature | The reference temperature that corresponds to the 'Cone diameter' input value   | °C          | -240 .. 1000 | 20        |
| Configuration              | The type of McCrometer V-Cone meter.<br>This setting is used to select the appropriate equation for determination of the gas expansion factor as specified by McCrometer<br>1: Standard V-Cone<br>2: Wafer-Cone<br>Note of input 'Fluid' is set to 'Liquid', then this input is not used (because the expansion factor is set to 1)   | -           |              | 1         |
| Pressure Location          | 1: Upstream<br>Input 'Pressure' represents the pressure at the upstream pressure tapping ( $p_1$ ).<br>Since the absolute pressure is usually measured at the upstream tapping this is the most common setting.<br>2: Downstream<br>Input 'Pressure' represents the pressure at the downstream tapping ( $p_2$ ).   | -           |              | 1         |
| Temperature Location       | 1: Upstream<br>Input 'Temperature' represents the upstream temperature ( $t_1$ ).<br>2: Downstream<br>Input 'Temperature' represents the temperature at the downstream tapping ( $t_2$ ).<br>3: Recovered<br>Input 'Temperature' represents the downstream temperature at a location Where the pressure has fully recovered ( $t_3$ ).<br>Since temperature measurement is usually downstream of the flow device this is the most common setting.   | -           |              | 2         |
| Temperature Correction     | This parameter specifies if and how the temperature should be corrected from downstream to upstream conditions (or vice versa)<br>1: $(1-\kappa)/\kappa$<br>Isentropic expansion using $(1-\kappa)/\kappa$ as the temperature referral exponent<br>2: Constant<br>Isentropic expansion using input 'Temperature Exponent' as the temperature referral exponent [-]<br>3: Joule Thomson<br>Isenthalpic expansion using input 'Temperature Exponent' as the Joule Thomson coefficient [°C/bar].<br>This method is prescribed by ISO5167-1:2003. |             |              | 1         |
| Temperature Exponent       | Refer to input Temperature Correction<br>Unit depends on input Temperature Correction value   | -<br>°C/bar |              | 0         |
| Density Location           | This parameter specifies if and how the density should be corrected from downstream to upstream conditions (or vice versa).<br>1: Upstream<br>Input 'Density' represents the density at the upstream pressure tapping ( $\rho_1$ ).<br>2: Downstream<br>Input 'Density' represents the density at the downstream tapping ( $\rho_2$ ).<br>3: Recovered<br>Input 'Density' represents the density downstream at a location Where the pressure has fully recovered ( $\rho_3$ ).  | -           |              | 1         |
| Density Exponent.          | This factor is used when density correction is enabled. The formula $1/\kappa$ will be used when the input value is set to 0, else the input value will be used.<br>For more details refer to section 'Density correction'.   | -           |              | 0         |
| Fluid                      | The type of fluid being measured<br>1: Gas<br>2: Liquid   | -           |              | 1         |
| Discharge coefficient      | The discharge coefficient of the meter as specified by the manufacturer.<br>The McCrometer reference document states that the discharge coefficient is a function of Reynolds number. It is advised that the meter is calibrated across the range of Reynold numbers for which the meter is used.<br>The resulting correction curve can be implemented through function <code>fxInterpolationCurve</code> . Input 'Discharge coefficient' needs to be linked to the corresponding output of this additional function.                         | -           | 0..2         | 0.85      |



## Function outputs

| Function outputs                  | Remark  | EU      | Fallback                                     |
|-----------------------------------|---|---------|--|
| Status                            | 0: Normal (No error condition)<br>1: Input argument out of range<br>2: No convergence   |         |  |
| Mass flow rate                    | The calculated mass flow rate   | tonne/h | 0  |
| Beta ratio                        | Cone to pipe diameter ratio at upstream temperature   | -       | Input Cone diameter /<br>Input Pipe diameter |
| Cone diameter                     | At the upstream temperature   | mm      | Input Cone diameter                          |
| Pipe diameter                     | At the upstream temperature   | mm      | Input Pipe diameter                          |
| Upstream pressure                 | Pressure at upstream tapping ( $p_1$ )  | bar(a)  | Input Pressure                               |
| Pressure at downstream tapping    | Pressure at downstream tapping ( $p_2$ )  | bar(a)  | Input Pressure                               |
| Recovered downstream pressure     | Fully recovered downstream pressure ( $p_3$ )   | bar(a)  | Input Pressure                               |
| Upstream temperature              | Temperature at upstream tapping ( $t_1$ )   | °C      | Input Temperature                            |
| Temperature at downstream tapping | Temperature at downstream tapping ( $t_2$ )   | °C      | Input Temperature                            |
| Downstream Temperature            | 'Fully recovered' downstream temperature ( $t_3$ )  | °C      | Input Temperature                            |
| Upstream density                  | Density at upstream tapping ( $\rho_1$ )  | kg/m3   | Input Density                                |
| Density at downstream tapping     | Pressure at downstream tapping ( $\rho_2$ )   | kg/m3   | Input Density                                |
| Downstream density                | 'Fully recovered' downstream density ( $\rho_3$ )   | kg/m3   | Input Density                                |
| Reynolds number                   |   | -       | 0  |
| Discharge coefficient             | Same as input value   | -       |  |
| Expansion Factor                  |   | -       | 0  |
| Velocity                          | Pipeline velocity   | m/s     | 0  |
| Expansion Factor Range            | The McCrometer reference document states that for gas applications the expansion factor should not get below 0.84<br>0: Expansion factor is in valid range<br>1: Expansion factor is out of valid range | -       | 0  |

## Calculations

The flow calculation is as specified in the McCrometer reference document.

The downstream to upstream correction (and vice versa) for pressure, temperature and density are as specified for function 'ISO 5167 Orifice'.

### 3 Flow-X flow computer functions

This chapter lists all available general Spirit<sup>IT</sup> Flow-X functions. These functions are only available in the Flow-X flow computer software.

#### fx2CellSelection

##### Description

The function selects between 2 input cells (e.g. differential pressure cells) based on the actual measured value and the failure status of each cell.

The function can handle the following type of cell range configurations:

- Lo – Hi
- Hi – Hi

Where 'Lo' means low range, 'Mid' mid range and 'Hi' high range.

##### Function inputs

| Function inputs        | Remark  | EU | SW tag   | Range  | Default |
|------------------------|---|----|----------|--------|---------|
| Name                   |   |    |          |        |         |
| Cell A value           | Input value as percentage of span of cell A   |    |          |        |         |
| Cell A status          | Input status of cell A<br>0: Normal<br><> 0 : Failure   |    |          |        |         |
| Cell B value           | Input value as percentage of span of cell B   |    |          |        |         |
| Cell B status          | Input status of cell B<br>0: Normal<br><> 0 : Failure   |    |          |        |         |
| Range type             | For a description of the functionality refer to adjacent section 'Logic'<br>1: Lo Hi<br>Cell A at low range<br>Cell B at high range<br>2: Hi Hi<br>Cell A and B at same range |    | RNGTYP   |        |         |
| Auto switchback        | For a description of the functionality refer to adjacent section 'Logic'<br>0: Disabled<br>1: Enabled   |    |          |        |         |
| Switch-up percentage   | Switch-up value expressed as percentage of span of the lower range  | -  | SWUPPERC | 0..100 | 95      |
| Switch-down percentage | Switch-down value expressed as percentage of span of the lower range  | -  | SWDNPERC | 0..100 | 90      |

##### Function outputs

| Function outputs     | Remark                                      | EU | SW tag | Alarm | Fallback |
|----------------------|---|----|--------|-------|----------|
| Status               | 0: Normal<br>1: Input argument out of range |    | STS    | FLOOR |          |
| Selected cell number | 1: Cell 1<br>2: Cell 2                      |    | SELNR  |       | 1        |
| Selected cell status | 0: Normal<br>1: Failure                     |    | SELSTS |       | 0        |

##### Logic

The function will switch from one cell to another at the following conditions:

##### Range type = 'Lo Hi'

When cell A is currently selected

- Select cell B when cell A value is above or equal to the switch-up percentage of its range and cell B is healthy.
- Select cell B when cell A fails while cell B is healthy

When cell B is currently selected

- Select cell A when cell A value is below or equal to the switch-down percentage of its range and cell A is healthy
- Select cell A when cell B fails and cell A is healthy

##### Range type = 'Hi Hi'

When cell A is currently selected

- Select cell B when cell A value fails and cell B is healthy

When cell B is currently selected

- Select cell A when cell A is healthy and 'Auto switchback' is enabled
- Select cell A when cell B fails and cell A is healthy.

## fx3CellSelection

### Description

The function selects between 3 input cells (typically differential pressure cells) based on the actual measured value and the failure status of each cell.

The function can handle the following type of cell range configurations:

- Lo – Mid – Hi
- Lo – Hi – Hi
- Hi – Hi – Hi

Where 'Lo' means low range, 'Mid' mid range and 'Hi' high range.

### Function inputs

| Function inputs        | Remark   | EU | SW tag   | Range  | Default |
|------------------------|--|----|----------|--------|---------|
| Name                   |  |    |          |        |         |
| Cell A value           | Input value as percentage of span of cell A  |    |          |        |         |
| Cell A status          | Input status of cell A<br>0: Normal<br><> 0 : Failure  |    |          |        |         |
| Cell B value           | Input value as percentage of span of cell B  |    |          |        |         |
| Cell B status          | Input status of cell B<br>0: Normal<br><> 0 : Failure  |    |          |        |         |
| Cell C value           | Input value as percentage of span of cell C  |    |          |        |         |
| Cell C status          | Input status of cell C<br>0: Normal<br><> 0 : Failure  |    |          |        |         |
| Range type             | For a description of the functionality refer to adjacent section 'Logic'<br>1: Lo Mid Hi<br>Cell A at low range<br>Cell B at mid range<br>Cell C at high range<br>2: Lo Hi Hi<br>Cell A at low range<br>Cell B and C at high range<br>3: Hi Hi Hi<br>Cell A, B and C at same range |    | RNGTYP   |        |         |
| Auto switchback        | For a description of the functionality refer to adjacent section 'Logic'<br>0: Disabled<br>1: Enabled  |    |          |        |         |
| Switch-up percentage   | Switch-up value expressed as percentage of span of the lower range<br>Does not apply for selection type 'Hi Hi Hi'   | -  | SWUPPERC | 0..100 | 95      |
| Switch-down percentage | Switch-down value expressed as percentage of span of the lower range<br>Does not apply for selection type 'Hi Hi Hi'   | -  | SWDNPERC | 0..100 | 90      |

### Function outputs

| Function outputs     | Remark                                      | EU | SW tag | Alarm | Fallback |
|----------------------|---|----|--------|-------|----------|
| Status               | 0: Normal<br>1: Input argument out of range |    | STS    | FIOOR |          |
| Selected cell number | 1: Cell 1<br>2: Cell 2<br>3: Cell 3         |    | SELNR  |       | 1        |
| Selected cell status | 0: Normal<br>1: Failure                     |    | SELSTS |       | 0        |

## Logic

The function will switch from one cell to another at the following conditions:

### Range type = 'Lo Mid Hi'

When cell A is currently selected

- Select cell B when cell A value is above or equal to the switch-up percentage of its range and cell B is healthy.
- Select cell B when cell A fails while cell B is healthy
- Select cell C when cell A and cell B fail and cell C is healthy

When cell B is currently selected

- Select cell C when cell B value is above or equal to the switch-up percentage of its range and cell C is healthy
- Select cell A when cell A value is below or equal to the switch-down percentage of its range and cell A is healthy
- Select cell A when cell B fails while cell A is healthy
- Select cell C when cell B and cell A fail and cell C is healthy

When cell C is currently selected

- Select cell B when cell B value is below or equal to the switch-down percentage of its range and cell B is healthy
- Select cell B when cell C fails while cell B is healthy
- Select cell A when cell C and cell B fail and cell A is healthy

### Range type = 'Lo Hi Hi'

When cell A is currently selected

- Select cell B when cell A value is above or equal to the switch-up percentage of its range and cell B is healthy.
- Select cell C when cell A value is above or equal to the switch-up percentage of its range and cell B fails and cell C is healthy.
- Select cell B when cell A fails while cell B is healthy
- Select cell C when cell A and cell B fail and cell C is healthy

When cell B is currently selected

- Select cell A when cell A value is below or equal to the switch-down percentage of its range and cell A is healthy
- Select cell C when cell B fails while cell C is healthy
- Select cell A when cell B and cell C fail and cell A is healthy

When cell C is currently selected

- Select cell A when cell A value is below or equal to the switch-down percentage of its range and cell A is healthy
- Select cell B when cell B is healthy and 'Auto switchback' is enabled
- Select cell A when cell C and cell B fail and cell A is healthy

### Range type = 'Hi Hi Hi'

When cell A is currently selected

- Select cell B when cell A value fails and cell B is healthy
- Select cell C when cell A and cell B fail and cell C is healthy

When cell B is currently selected

- Select cell A when cell A is healthy and 'Auto switchback' is enabled
- Select cell A when cell B fails and cell A is healthy
- Select cell C when cell B and A fail and cell C is healthy

When cell C is currently selected

- Select cell A when cell A is healthy and 'Auto switchback' is enabled
- Select cell B when cell B is healthy and cell A fails and 'Auto switchback' is enabled
- Select cell A when cell C fails and cell A is healthy
- Select cell B when cell C and A fail and cell B is healthy

## fxBatchFWA

### Description

The function calculates a **flow-weighted average (FWA)** for a batch.

A batch can be any batch type of process, such as product loading, meter proving or transmitter validation.

The function weights the input value with a flow increment and updates the average accordingly. The flow increment is provided by either a 'fxTotalizerDelta' or a 'xTotalizerRate' function.

### Function inputs

| Function inputs | Remark  | EU                  | SW tag | Range       | Default |
|-----------------|---|---------------------|--------|-------------|---------|
| Name            | Name used for tag-prefix and retentive storage.   |                     |        |             |         |
| Input value     | Value to be averaged  | Same as linked cell |        | -1e11..1e11 |         |
| Enabled         | 0: Disabled<br>1: Enabled   |                     | EN     |             |         |
| Increment       | Flow increment with which the input value is weighed.<br>Must refer to the corresponding output from a 'TotalizerRate' or 'TotalizerDelta' function<br>Negative values will be ignored.   | Same as linked cell |        | 0..1e11     |         |
| Reset command   | Trigger to reset the batch.<br>At a batch reset the current average is stored in the previous value and the current value is reset to 0   |                     |        |             |         |
| Identification  | Batch identification.<br>Can be any string of maximum 255 characters long.<br>If multiple identifications need to be stored for future referral, e.g. the batch number, the ship name and the nomination number, then the individual strings should be concatenated with an "." character in-between. |                     | ID     |             |         |

### Function outputs

| Function outputs | Remark                                     | EU                          | SW tag | Alarm | Fallback |
|------------------|--|-----------------------------|--------|-------|----------|
| Current average  | Average calculated over the current batch. | Same as input 'Input value' | CB     |       | 0        |
| Previous average | Average of the previous batch.             | Same as input 'Input value' | PB     |       | 0        |

## fxBatchHistData

### Description

The function retrieves historical 'batch' data from the flow computer persistent memory.

A 'batch' can be any batch type of process, such as product loading, meter proving or transmitter validation.

The function retrieves one or more historical values for the specified function instance. The function instance must be one of the following function types:

- fxBatchFWA
- fxBatchLatch
- fxBatchStore
- fxBatchTotal
- fxBatchTWA
- fxBatchWatch

The function instance is referred to by its name (i.e. the 1st argument of the referred function).

### Function inputs

| Function inputs | Remark  | EU | SW tag  | Range | Default |
|-----------------|---|----|---------|-------|---------|
| Name            | Name used for tag-prefix and retentive storage.   |    |         |       |         |
| First ID        | Optional.<br>Batch identification of the first historical batch for which the value has to be retrieved.  |    | FIRSTID |       |         |
| Last ID         | Optional.<br>Batch identification of the last historical batch for which the value has to be retrieved.   |    | LASTID  |       |         |
| Sequence        | Sequence in which the retrieved values must be copied to the function outputs.<br>1: Ascending order (Value 1 contains oldest value)<br>2: Descending order (Value 1 contains newest value) |    |         |       | 1       |

### Function outputs

| Function outputs | Remark   | EU | SW tag  | Alarm | Fallback |
|------------------|--|----|---------|-------|----------|
| Number of values | Number of historical values that was retrieved from the flow computer memory according to the input criteria |    | ACTSIZE |       |          |
| Value 1          | The 1st retrieved historical data value  |    | 1       |       |          |
| Value 2          | The 2nd retrieved historical data value  |    | 2       |       |          |
| etc.             |  |    |         |       |          |

## fxBatchLatch

### Description

The function latches a value at every batch reset.

### Function inputs

| Function inputs | Remark   | EU                  | SW tag | Range | Default |
|-----------------|--|---------------------|--------|-------|---------|
| Name            | Name used for tag-prefix and retentive storage.  |                     |        |       |         |
| Input value     | Value to be latched  | Same as linked cell |        |       |         |
| Latch command * | Trigger to latch the value   |                     |        |       |         |
| Reset command * | Trigger to reset the batch.<br>At every batch reset the last latched value is stored in the previous latch output value and the current latch output value is reset to 0 |                     |        |       |         |
| Identification  | Batch identification.<br>Can be any string of maximum 255 characters long.   |                     | ID     |       |         |

Note: When the latch and reset commands are given at the same time, then the current value becomes the 'Previous latch' output value and the current latch is reset to 0.

### Function outputs

| Function outputs | Remark   | EU                          | SW tag | Alarm | Fallback |
|------------------|--|-----------------------------|--------|-------|----------|
| Current latch    | Value that is latched since the last batch reset.<br>Is reset to 0 at every batch reset.   | Same as input 'Input value' | CB     |       | 0        |
| Previous latch   | Value that was latched during the previous batch. If no value was latched during the previous batch, then the value is set to 0. | Same as input 'Input value' | PB     |       | 0        |

## fxBatchMax

### Description

The function determines the maximum for a particular input value over a batch.

A batch can be any batch type of process, such as product loading, meter proving or transmitter validation.

### Function inputs

| Function inputs | Remark  | EU                  | SW tag | Range       | Default |
|-----------------|---|---------------------|--------|-------------|---------|
| Name            | Name used for tag-prefix and retentive storage.   |                     |        |             |         |
| Input value     | Value for which the maximum has to be determined  | Same as linked cell |        | -1e11..1e11 |         |
| Enabled         | 0: Disabled<br>1: Enabled   |                     | EN     |             |         |
| Reset command   | Trigger to reset the batch.<br>At a batch reset the current average is stored in the previous value and the current value is reset to 0   |                     |        |             |         |
| Identification  | Batch identification.<br>Can be any string of maximum 255 characters long.<br>If multiple identifications need to be stored for future referral, e.g. the batch number, the ship name and the nomination number, then the individual strings should be concatenated with an "." character in-between. |                     | ID     |             |         |

### Function outputs

| Function outputs | Remark                           | EU                          | SW tag | Alarm | Fallback |
|------------------|----------------------------------|-----------------------------|--------|-------|----------|
| Current minimum  | Minimum over the current batch.  | Same as input 'Input value' | CB     |       | 0        |
| Previous minimum | Minimum over the previous batch. | Same as input 'Input value' | PB     |       | 0        |



## fxBatchMin

### Description

The function determines the minimum for a particular input value over a batch.

A batch can be any batch type of process, such as product loading, meter proving or transmitter validation.

### Function inputs

| Function inputs | Remark  | EU                  | SW tag | Range       | Default |
|-----------------|---|---------------------|--------|-------------|---------|
| Name            | Name used for tag-prefix and retentive storage.   |                     |        |             |         |
| Input value     | Value for which the minimum has to be determined  | Same as linked cell |        | -1e11..1e11 |         |
| Enabled         | 0: Disabled<br>1: Enabled   |                     | EN     |             |         |
| Reset command   | Trigger to reset the batch.<br>At a batch reset the current average is stored in the previous value and the current value is reset to 0   |                     |        |             |         |
| Identification  | Batch identification.<br>Can be any string of maximum 255 characters long.<br>If multiple identifications need to be stored for future referral, e.g. the batch number, the ship name and the nomination number, then the individual strings should be concatenated with an "." character in-between. |                     | ID     |             |         |

### Function outputs

| Function outputs | Remark                           | EU                          | SW tag | Alarm | Fallback |
|------------------|----------------------------------|-----------------------------|--------|-------|----------|
| Current minimum  | Minimum over the current batch.  | Same as input 'Input value' | CB     |       | 0        |
| Previous minimum | Minimum over the previous batch. | Same as input 'Input value' | PB     |       | 0        |

## fxBatchTotal

### Description

The function accumulates a flow increment into a batch total. At every batch reset the current batch total is stored into the previous value and the current value is reset to 0.

The flow increment originates from a 'TotalizerRate' or 'TotalizerDelta' function.

### Function inputs

| Function inputs | Remark  | EU                      | SW tag | Range   | Default |
|-----------------|---|-------------------------|--------|---------|---------|
| Name            | Name used for tag-prefix and retentive storage.   |                         |        |         |         |
| Increment       | Increment value to be added to the batch total.<br>Negative values will be ignored, so the batch total will not decrease.   | Same as linked cell     |        | 0..1e11 |         |
| Enabled         | 0: Disabled<br>1: Enabled   |                         | EN     |         |         |
| Identification  | Batch identification.<br>Can be any string of maximum 255 characters long.<br>If multiple identifications need to be stored for future referral, e.g. the batch number, the ship name and the nomination number, then the individual strings should be concatenated with an "." character in-between. |                         | ID     |         |         |
| Rollover value  | The batch total will be reset to 0 when it reaches the rollover value   | Same as input Increment | ROVAL  | 0..1e15 | 1e12    |
| Decimal places  | Defines the number of decimal places for the current and previous total output values.<br>-1 means full precision (no rounding applied)   |                         | DECPLS | -1..10  | -1      |

### Function outputs

| Function outputs | Remark  | EU                        | SW tag | Alarm | Fallback |
|------------------|---|---------------------------|--------|-------|----------|
| Current total    | Accumulated total for the current batch, so since the last batch reset.                                 | Same as input 'Increment' | CB     |       | 0        |
| Previous total   | Accumulated total for the previous batch  | Same as input 'Increment' | PB     |       | 0        |
| Rollover flag    | Flag indicating a rollover to 0.<br>0: Off<br>1: On<br>Note: stays 'On' for one calculation cycle only) | 0                         |        | ROALM |          |

## fxBatchTWA

### Description

The function calculates a **time-weighted average (TWA)** for a batch. At a batch reset the current average is stored in the previous value and the current value is reset to 0.

The function weights the input value with the time (in fact the actual calculation cycle time) and updates the average accordingly.

### Function inputs

| Function inputs | Remark  | EU                  | SW tag | Range       | Default |
|-----------------|---|---------------------|--------|-------------|---------|
| Name            | Name used for tag-prefix and retentive storage.   |                     |        |             |         |
| Input value     | Value to be averaged  | Same as linked cell |        | -1e11..1e11 |         |
| Enabled         | 0: Disabled<br>1: Enabled   |                     | EN     |             |         |
| Reset command   | Trigger to reset the batch.<br>At a batch reset the current latch is stored in the previous value and the current latch is reset to 0   |                     |        |             |         |
| Identification  | Batch identification.<br>Can be any string of maximum 255 characters long.<br>If multiple identifications need to be stored for future referral, e.g. the batch number, the ship name and the nomination number, then the individual strings should be concatenated with an "." character in-between. |                     | ID     |             |         |

### Function outputs

| Function outputs | Remark                                     | EU                          | SW tag | Alarm | Fallback |
|------------------|--|-----------------------------|--------|-------|----------|
| Current average  | Average calculated over the current batch. | Same as input 'Input value' | CB     |       | 0        |
| Previous average | Average of the previous batch.             | Same as input 'Input value' | PB     |       | 0        |

## fxBatchWatch

### Description

The function 'remembers' that a condition has been valid during a batch.

A typical example is a transmitter that was overridden with a keypad value.

### Function inputs

| Function inputs | Remark  | EU | SW tag | Range | Default |
|-----------------|---|----|--------|-------|---------|
| Name            | Name used for tag-prefix and retentive storage.   |    |        |       |         |
| Condition       | 0: Condition is not valid<br><>0: Condition is valid  |    |        |       |         |
| Enabled         | 0: Disabled<br>1: Enabled   | EN |        |       |         |
| Reset command   | Trigger to reset the batch.<br>At a batch reset the current watched value is stored in the previous value and the current watched value is reset to 0   |    |        |       |         |
| Identification  | Batch identification.<br>Can be any string of maximum 255 characters long.<br>If multiple identifications need to be stored for future referral, e.g. the batch number, the ship name and the nomination number, then the individual strings should be concatenated with an "." character in-between. |    | ID     |       |         |

### Function outputs

| Function outputs | Remark   | EU | SW tag | Alarm | Fallback |
|------------------|--|----|--------|-------|----------|
| Current watch    | Indicates whether or not the condition has been valid during the current batch:<br>0: Not valid<br>1: Valid  |    | CB     |       | 0        |
| Previous watch   | Indicates whether or not the condition has been valid during the previous batch:<br>0: Not valid<br>1: Valid |    | PB     |       | 0        |

## fxDeviationAlarm

### Description

The function watches the deviation, or the difference or discrepancy, between two values and generates an alarm when the deviation exceeds the specified limit.

### Function inputs

| Function inputs | Remark   | EU  | SW tag | Range         | Default |
|-----------------|--|---|--------|---------------|---------|
| Name            | Optional tag name, tag description and tag group   |   |        |               |         |
| Input value 1   | Must be linked to another cell   | Same as linked cell                             |        | -1e11..1e11   | 0       |
| Input value 2   | Must be linked to another cell   | Must be same as for input value 1               |        | -1e11..1e11   | 0       |
| Deviation type  | Determines whether the absolute or the relative difference needs to be checked. The unit of the deviation limit will be in accordance.<br>1: Absolute<br>2: Relative |   | DEVTYP |               | 1       |
| Deviation limit | The unit depends on the 'Deviation type'   | Absolute: Same as input value 1<br>Relative : % | DEVLIM | 0..1e11       | 0       |
| Enabled         | Enabled or disabled the alarm  |   |        | True or false | True    |
| Alarm type      | 1: Alarm<br>2: Warning   |   |        |               | 1       |

### Function outputs

| Function outputs | Remark                | EU | SW tag | Alarm  | Fallback |
|------------------|-----------------------|----|--------|--------|----------|
| Deviation alarm  | 0: Normal<br>1: Alarm | -  | DEVALM | DEVALM |          |

### Logic

Deviation type = 1 (Absolute)

- A deviation alarm is raised when the absolute difference between the two values is greater than the 'Discrepancy limit'.

Deviation type = 2 (Relative)

- A deviation alarm is raised when the absolute difference between the two values divided by the minimum of the two values times 100 % is greater than the 'Discrepancy limit'.

## fxGenerateReport

### Description

This function generates prints and stores a report.

### Function inputs

| Function inputs  | Remark   | EU | SW tag | Range | Default |
|------------------|--|----|--------|-------|---------|
| Name             | Report definition<br>Must be the name of the report definition (Flow-Xpress, section Reports).   |    |        |       |         |
| Event            | Event to generate the report.<br>Event occurs when value changes from zero to non-zero (or from FALSE to TRUE).  |    |        |       |         |
| Identifier       | Optional report file name, defined as a string<br>When defined the Identifier is used as the report file name .<br>When left empty, the UniqueMethod setting as defined for the report definition is used for the report file name ( <b>Flow-Xpress</b> , section Reports).  |    |        |       |         |
| Printer          | Optional printer.<br>Must be the name of one of the printers that are defined in <b>Flow-Xpress</b> .<br>When defined this printer is used instead of the printer that is assigned to the report template ( <b>Flow-Xpress</b> , section Reports).<br>When left empty the printer that is assigned to the report template is used. |    |        |       |         |
| Number of copies | Number of copies to print.<br>This setting is ignored when no printer is defined.  |    |        |       | 1       |

### Function outputs

| Function outputs | Remark  | EU | SW tag | Alarm           | Fallback |
|------------------|---|----|--------|-----------------|----------|
| Status           | 0: Normal<br>1: Input argument out of range or in conflict<br>2: Latest report could not be generated | -  | STS    | FIOOR<br>RPTERR |          |

## fxIndex

### Description

The 'fxIndex' provides the same functionality as the Excel Index function with the addition of the creation of tag names.

A spreadsheet cell that contains a 'fxIndex' function obtains the tag name as defined by its 'Name' input with the tag inheriting all properties including the value and units from the referred tag. When the referred cell contains a writable tag (i.e. a value and no function) than the cell with the 'fxIndex' function also represents a writable tag with the same properties.

When the referred cell contains a tag that represents one or more alarms, then the same alarms are created for the cell with the 'fxIndex' function.

The 'fxIndex' is especially useful for setting up generic (template) applications as illustrated by the following examples:

- For each of the 6 analog inputs the application contains one 'Analog input' function that generates tag names with prefix, "AIN1\_", "AIN2\_" etc. Also more meaningful tag names such as "..PT" (pressure transmitter), "..TT" are used in the application. When changing the high alarm limit for the pressure transmitter (e.g. through an OPC interface) it makes more sense to address the tag as "..PT\_HISCALE" instead of "..AIN3\_HISCALE" (assuming AIN 3 being used for the pressure transmitter). This can be achieved by using the 'fxIndex' function for the cell that represents the '..PT\_HISCALE' tag.
- In some cases one and the same input signal is used for multiple process variables that are defined in the generic application. E.g. when the generic application assumes a prover inlet temperature input signal as well as a prover outlet temperature signal (and has corresponding tag names), while there is only a temperature transmitter in the prover loop, then the input tags of both signals can refer to the same "AIN" signal by using the 'fxIndex' function.

### Function inputs

| Function inputs | Remark  | EU | SW tag | Range | Default |
|-----------------|---|----|--------|-------|---------|
| Name            | Tag name for the cell that contains the function  |    |        |       |         |
| Reference       | Reference to one or more cell ranges  |    |        |       | 1       |
| Row number      | Optional<br>Number of the row in reference from which to return a reference   |    |        |       | 1       |
| Column number   | Optional.<br>Number of the column in reference from which to return a reference   |    |        |       | 1       |
| Area number     | Optional<br>Selects a range in reference from which to return the intersection of 'Row number' and 'Column number'. The first area selected or entered is numbered 1, the second is 2, and so on. |    |        |       | 1       |

### Function outputs

| Function outputs | Remark   | EU                    | SW tag     | Alarm | Fallback |
|------------------|--|-----------------------|------------|-------|----------|
| Value            | The cell obtains a tag name that consist of the prefix as defined by input 'Name' with the addition of the suffix as was generated for the tag that is being referred to.<br>The same applies for an alarm if one has been defined for the referred tag. | Same as referred cell | See Remark |       |          |

## fxKeypadFallback

### Description

This function provides a generic interface to any input signal, such as a pressure, temperature, density or flow input. It provides the option to override the 'live' value with a keypad value and to fallback to a specific value when the input value is faulty.

When the input signal fails, the in-use value may fall back to the last good value, the keypad value or additionally a separate fallback value. The fallback value allows the user to define a fixed value (e.g. 0) that is independent from the current keypad value.

### Function inputs

| Function inputs | Remark  | EU            | SW tag | Range | Default |
|-----------------|---|---------------|--------|-------|---------|
| Name            | Optional tag name, tag description and tag group  |               |        |       |         |
| Input status    | Status of the input signal<br>0: Normal<br><> 0: Failure<br>Must be linked to the Status output of the related input function       |               | INPSTS |       |         |
| Input value     | Value of the input signal<br>Must be linked to the (scaled) value output of the related input function.                             |               | INPVAL |       |         |
| Fallback type   | Determines what to do when input fails<br>1: Use last good value<br>2: Use fallback value<br>3: Use keypad value<br>4: Use measured |               | FBTYP  |       |         |
| Fallback value  | Used when output 'Input status' becomes 'Faulty' and 'Fallback type' is set to 'Use fallback value'                                 | Same as input | FBVAL  |       |         |
| Keypad mode     | Forces the usage of the keypad value<br>0: Disabled<br>1: Enabled   |               | KPMOD  | -     | 0       |
| Keypad value    | Used when output 'Input status' becomes 'Faulty' and 'Fallback type' is set to 'Use fallback value'                                 | Same as input | KPVAL  |       | 0       |

### Function outputs

| Function outputs | Remark   | EU            | SW tag | Alarm   | Fallback |
|------------------|--|---------------|--------|---|----------|
| Status           | 0: Normal<br>1: Argument out of range<br>2: Keypad<br>3: Fail Last Good<br>4: Fail Keypad<br>5: Fail Fallback<br>6: Fail Measured<br>Only for status 'Function Input argument out of range' the output values will revert to the corresponding fallback value. |               | STS    | FIOOR<br>FAILLG<br>FAILKP<br>FAILFB<br>KEYPAD<br>FAILMS |          |
| In-use value     |  | Same as input | CUR    |   | 0        |



## fxKeypadFallbackArray

### Description

This function provides a generic interface to an array of input values, typically a gas composition. It provides the option to override the 'live' values with keypad values and to fallback to specific values when the set of input values is faulty.

When the input signals fail, the in-use values may fall back to the last good values, the keypad values or additionally separate fallback values. The fallback values allow the user to define a fixed values (e.g. 0) that is independent from the current keypad values.

### Function inputs

| Function inputs | Remark  | EU            | SW tag | Range | Default |
|-----------------|---|---------------|--------|-------|---------|
| Name            | Optional tag name, tag description and tag group  |               |        |       |         |
| Input status    | Status of the input signals<br>0: Normal<br><> 0: Failure   |               | INPSTS |       |         |
| Input values    | <b>Array</b> if input values  |               | INPVAL |       |         |
| Fallback type   | Determines what to do when input fails<br>1: Use last good value<br>2: Use fallback value<br>3: Use keypad value<br>4: Use measured |               | FBTYP  |       |         |
| Fallback value  | Array of fallback values.<br>Used when output 'Input status' becomes 'Faulty' and 'Fallback type' is set to 'Use fallback value'    | Same as input | FBVAL  |       |         |
| Keypad mode     | Forces the usage of the keypad value<br>0: Disabled<br>1: Enabled   |               | KPMOD  | -     | 0       |
| Keypad value    | Array of keypad values.<br>Used when output 'Input status' becomes 'Faulty' and 'Fallback type' is set to 'Use fallback value'      | Same as input | KPVAL  |       | 0       |

### Function outputs

| Function outputs | Remark  | EU            | SW tag | Alarm   | Fallback |
|------------------|---|---------------|--------|---|----------|
| Status           | 0: Normal<br>1: Argument out of range<br>2: Keypad<br>3: Fail Last Good<br>4: Fail Keypad<br>5: Fail Fallback<br>6: Fail Measured<br>Only for status 'Function Input argument out of range' the output vales will revert to the corresponding fallback value. |               | STS    | FIOOR<br>FAILLG<br>FAILKP<br>FAILFB<br>KEYPAD<br>FAILMS |          |
| In-use value     | Array of in-use values  | Same as input | CUR    |   | 0        |

# fxLatch

## Description

The 'fxLatch' function provides generic latching functionality.

## Function inputs

| Function inputs | Remark  | EU | SW tag | Range | Default |
|-----------------|---|----|--------|-------|---------|
| Name            | Tag name for the cell that contains the 'fxLatchValue' function.                        |    |        |       |         |
| Latch trigger   | Trigger to latch the input value  |    |        |       |         |
| Input value     | Value to be latched. May be a constant a formula or a reference to another cell or tag. |    |        |       |         |
| Reset trigger   | Optional<br>Trigger to resets the latched value to the reset value                      |    |        |       |         |
| Reset value     | Optional<br>Reset value (default 0). May be a constant or a formula.                    |    |        |       |         |

## Function outputs

| Function outputs | Remark  | EU                              | SW tag     | Alarm | Fallback |
|------------------|---|---------------------------------|------------|-------|----------|
| Latched value    | The most recent latched value<br>Note: this value is persistent and will be reloaded upon startup | Same as of input<br>Input Value | Input Name |       |          |

## fxLimitAlarm

### Description

The function applies alarm limits on any value.

### Function inputs

| Function inputs       | Remark  | EU                  | SW tag | Range                    | Default |
|-----------------------|---|---------------------|--------|--------------------------|---------|
| Name                  | Optional tag name   |                     |        |                          |         |
| Input value           | Must be linked to another cell  | Same as linked cell | INPVAL | -1e11..1e11              | 0       |
| Low limit value       |   | Same as Input value | LLIM   | -1e11..1e11              | -1e11   |
| High limit value      |   | Same as Input value | HLIM   | Low limit value .. 1e11  | -1e11   |
| Low low limit value   |   | Same as Input value | LLLIM  | -1e11.. Low limit value  | 1e11    |
| High high limit value |   | Same as Input value | HHLIM  | High limit value .. 1e11 | 1e11    |
| Deadband              |   | Same as Input value |        | 0..1e11                  | 0       |
| Enabled               | Enables or disables the alarm   |                     |        | True or false            | True    |
| Warning behavior      | Determines the warning behavior when the lo and hi limit are violated:<br>1: No warnings, just alarms<br>2: Warn on lo limit<br>3: Warn on hi limit<br>4: Warn on lo and hi limit |                     |        |                          | 1       |

### Function outputs

| Function outputs | Remark   | EU | SW tag | Alarm                          | Fallback |
|------------------|--|----|--------|--------------------------------|----------|
| Alarm status     | 0: Normal<br>1: Low alarm<br>2: High alarm<br>3: Low low alarm<br>4: High high alarm | -  | ALMSTS | LALM<br>HALM<br>LLALM<br>HHALM |          |

### Logic

The order of priority in setting the alarm status output is as follows:

- 1 If process value is below the 'Low low limit value' then the status becomes '3: Low low alarm'.
- 2 Else if process value is above the 'High high limit value' then the status becomes '4: High high alarm'.
- 3 Else if process value is below the 'Low limit value' then the status becomes '1: Low alarm'.
- 4 Else if process value is above the 'High limit value' then the status becomes '2: High alarm' and the 'High high alarm' is raised
- 5 Else the status becomes '0: Normal'.

fxName

Description

The 'fxName' function creates a string that defines the prefix, description and group for any function that generates tags, except for function fxTag.

Function outputs

| Function inputs | Remark   | EU | SW tag | Range | Default |
|-----------------|--|----|--------|-------|---------|
| Name            | Name for the tag   |    |        |       |         |
| Description     | Optional description for the tag   |    |        |       | <Empty> |
| Group           | Optional Group for the tag, including optional parent groups.<br>The parent group must proceed the child group and be separated by the '\' character.<br>E.g. "Meter setup\Meter data" defines that the tag belongs to group 'Meter data', which is a subgroup of group "Meter setup". |    |        |       | <Empty> |

Function outputs

| Function outputs | Remark  | EU | SW tag | Alarm | Fallback |
|------------------|---|----|--------|-------|----------|
|                  | String containing the name, description and group for the tag(s) to be created. |    |        |       |          |

## fxPeriodFWA

### Description

The function calculates a **flow-weighted average (FWA)** for a particular period.

The function weights the input value with a flow increment and updates the average accordingly. The flow increment is provided by a 'TotalizerDelta' or 'TotalizerRate' function.

At the end of the period the current average is stored in the previous value and the current value is reset to 0.

### Function inputs

| Function inputs | Remark   | EU                  | SW tag | Range      | Default |
|-----------------|--|---------------------|--------|------------|---------|
| Name            | Name used for tag prefix and retentive storage.  |                     |        |            |         |
| Input value     | Value to be averaged   | Same as linked cell |        |            |         |
| Enabled         | 0: Disabled<br><> 0: Enabled   |                     | EN     |            |         |
| Increment       | Flow increment with which the input value is weighed. Must refer to the corresponding output from a 'TotalizerRate' or 'TotalizerDelta' function. Negative values will be ignored.   | Same as linked cell |        |            |         |
| Period type     | Type of period:<br>1: Second<br>2: Minute<br>3: Hour<br>4: Day<br>5: Week<br>6: Month<br>7: Quarter<br>8: Year   |                     | TYP    |            |         |
| Period count    | Number of periods (e.g. 5 minutes, 8 hours)  |                     | CNT    | 1..1e11    |         |
| Period start    | Absolute start date and time of the period. This will be used as the reference point to calculate the next period rollover from. The value may be defined in the past or the future. The next rollover period will be calculated accordingly (so forwards or backwards in time). |                     | START  | <DATETIME> |         |

### Function outputs

| Function outputs     | Remark   | EU                          | SW tag | Alarm | Fallback |
|----------------------|--|-----------------------------|--------|-------|----------|
| Current average      | Average calculated over the current period.                                      | Same as input 'Input value' | CUR    |       | 0        |
| Previous average     | Average of the previous period.  | Same as input 'Input value' | PRV    |       | 0        |
| Pre-previous average | Average of the pre-previous period (i.e. the period before the previous period). | Same as input 'Input value' | PPRV   |       | 0        |

## fxPeriodLatch

### Description

The function latches a value at the end of a repeating period of time.

### Function inputs

| Function inputs | Remark  | EU                  | SW tag | Range       | Default |
|-----------------|---|---------------------|--------|-------------|---------|
| Name            | Name used for tag prefix and retentive storage.   |                     |        |             |         |
| Input value     | Value to be latched   | Same as linked cell |        | Not applied |         |
| Period type     | Type of period:<br>1: Second<br>2: Minute<br>3: Hour<br>4: Day<br>5: Week<br>6: Month<br>7: Quarter<br>8: Year  |                     | TYP    |             |         |
| Period count    | Number of periods (e.g. 5 minutes, 8 hours)   |                     | CNT    | 1..1e11     |         |
| Period start    | Absolute start date and time of the period. This will be used as the reference point to calculate the next period rollover from.<br>The value may be defined in the past or the future. The next rollover period will be calculated accordingly (so forwards or backwards in time). |                     | START  | <DATETIME>  |         |

### Function outputs

| Function outputs | Remark  | EU                          | SW tag | Alarm | Fallback |
|------------------|---|-----------------------------|--------|-------|----------|
| Current latch    | Value that is latched at start of the current period (end of previous period) | Same as input 'Input value' | CUR    |       | 0        |
| Previous latch   | Value that is latched at the start of the previous period                     | Same as input 'Input value' | PRV    |       | 0        |

## fxPeriodMax

### Description

The function determines a maximum value over a particular period.

### Function inputs

| Function inputs | Remark  | EU                  | SW tag | Range      | Default |
|-----------------|---|---------------------|--------|------------|---------|
| Name            | Name used for tag prefix and retentive storage.   |                     |        |            |         |
| Input value     | Value for which the maximum has to be determined  | Same as linked cell |        |            |         |
| Enabled         | 0: Disabled<br><> 0: Enabled  |                     | EN     |            |         |
| Period type     | Type of period:<br>1: Second<br>2: Minute<br>3: Hour<br>4: Day<br>5: Week<br>6: Month<br>7: Quarter<br>8: Year  |                     | TYP    |            |         |
| Period count    | Number of periods (e.g. 5 minutes, 8 hours)   |                     | CNT    | 1..1e11    |         |
| Period start    | Absolute start date and time of the period. This will be used as the reference point to calculate the next period rollover from.<br>The value may be defined in the past or the future. The next rollover period will be calculated accordingly (so forwards or backwards in time). |                     | START  | <DATETIME> |         |

### Function outputs

| Function outputs     | Remark  | EU                          | SW tag | Alarm | Fallback |
|----------------------|---|-----------------------------|--------|-------|----------|
| Current maximum      | Maximum over the current period.  | Same as input 'Input value' | CUR    |       | 0        |
| Previous maximum     | Maximum over the previous period.   | Same as input 'Input value' | PRV    |       | 0        |
| Pre-previous maximum | Maximum over the pre-previous period (period before the previous period). | Same as input 'Input value' | PPRV   |       | 0        |

## fxPeriodMin

### Description

The function determines a minimum value over a particular period.

### Function inputs

| Function inputs | Remark  | EU                  | SW tag | Range      | Default |
|-----------------|---|---------------------|--------|------------|---------|
| Name            | Name used for tag prefix and retentive storage.   |                     |        |            |         |
| Input value     | Value for which the minimum has to be determined  | Same as linked cell |        |            |         |
| Enabled         | 0: Disabled<br><> 0: Enabled  |                     | EN     |            |         |
| Period type     | Type of period:<br>1: Second<br>2: Minute<br>3: Hour<br>4: Day<br>5: Week<br>6: Month<br>7: Quarter<br>8: Year  |                     | TYP    |            |         |
| Period count    | Number of periods (e.g. 5 minutes, 8 hours)   |                     | CNT    | 1..1e11    |         |
| Period start    | Absolute start date and time of the period. This will be used as the reference point to calculate the next period rollover from.<br>The value may be defined in the past or the future. The next rollover period will be calculated accordingly (so forwards or backwards in time). |                     | START  | <DATETIME> |         |

### Function outputs

| Function outputs     | Remark   | EU                          | SW tag | Alarm | Fallback |
|----------------------|--|-----------------------------|--------|-------|----------|
| Current minimum      | Minimum over the current period.   | Same as input 'Input value' | CUR    |       | 0        |
| Previous minimum     | Minimum over the previous period.  | Same as input 'Input value' | PRV    |       | 0        |
| Pre-previous maximum | Minimum over the pre-previous period (i.e. period before the previous period). | Same as input 'Input value' | PPRV   |       | 0        |



## fxPeriodTotal

### Description

The function accumulates a flow increment into a period total. At the end of the period the current total is stored into the previous value and the current value is reset to 0.

The flow increment originates from a 'TotalizerRate' or 'TotalizerDelta' function.

### Function inputs

| Function inputs | Remark  | EU                      | SW tag | Range      | Default |
|-----------------|---|-------------------------|--------|------------|---------|
| Name            | Name used for tag prefix and retentive storage.   |                         |        |            |         |
| Increment       | Increment value to be added to the period total.<br>Negative values will be ignored, so the period total will not decrease.   | Same as linked cell     |        | 0..1e11    |         |
| Enabled         | 0: Disabled<br>1: Enabled   |                         | EN     |            |         |
| Period type     | Type of period:<br>1: Second<br>2: Minute<br>3: Hour<br>4: Day<br>5: Week<br>6: Month<br>7: Quarter<br>8: Year  |                         | TYP    |            |         |
| Period count    | Number of periods (e.g. 5 minutes, 8 hours)   |                         | CNT    | 1..1e11    |         |
| Period start    | Absolute start date and time of the period. This will be used as the reference point to calculate the next period rollover from.<br>The value may be defined in the past or the future. The next rollover period will be calculated accordingly (so forwards or backwards in time). |                         | START  | <DATETIME> |         |
| Rollover value  | The period total will be reset to 0 when it reaches the rollover value  | Same as input Increment | ROVAL  | 0..1e15    | 1e12    |
| Decimal places  | Defines the number of decimal places for the current and previous total output values.<br>-1 means full precision (no rounding applied)   |                         | DECPLS | -1..10     | -1      |

### Function outputs

| Function outputs   | Remark   | EU                        | SW tag | Alarm | Fallback |
|--------------------|--|---------------------------|--------|-------|----------|
| Current total      | Accumulated total for the current period   | Same as input 'Increment' | CUR    |       | 0        |
| Previous total     | Accumulated total for the previous period  | Same as input 'Increment' | PRV    |       | 0        |
| Rollover flag      | Flag indicating a rollover to 0.<br>0: Off<br>1: On<br>Note: stays 'On' for one calculation cycle only). |                           |        | ROALM |          |
| Pre-previous total | Accumulated total for the pre-previous period (i.e. the period before the previous period)               | Same as input 'Increment' | PPRV   |       | 0        |

## fxPeriodTWA

### Description

The function calculates a **time-weighted average (TWA)** for a particular period. At the end of a period the current average is stored in the previous value and the current value is reset to 0. The function weights the input value with the time (in fact the actual calculation cycle time) and updates the average accordingly.

### Function inputs

| Function inputs | Remark   | EU                  | SW tag | Range       | Default |
|-----------------|--|---------------------|--------|-------------|---------|
| Name            | Name used for tag prefix and retentive storage.  |                     |        |             |         |
| Input value     | Value to be averaged   | Same as linked cell |        | -1e11..1e11 |         |
| Enabled         | 0: Disabled<br>1: Enabled  |                     | EN     |             |         |
| Period type     | Type of period:<br>1: Second<br>2: Minute<br>3: Hour<br>4: Day<br>5: Week<br>6: Month<br>7: Quarter<br>8: Year   |                     | TYP    |             |         |
| Period count    | Number of periods (e.g. 5 minutes, 8 hours)  |                     | CNT    | 1..1e11     |         |
| Period start    | Absolute start date and time of the period. This will be used as the reference point to calculate the next period rollover from. The value may be defined in the past or the future. The next rollover period will be calculated accordingly (so forwards or backwards in time). |                     | START  | <DATETIME>  |         |

### Function outputs

| Function outputs     | Remark  | EU                          | SW tag | Alarm | Fallback |
|----------------------|---|-----------------------------|--------|-------|----------|
| Current average      | Average calculated over the current period                                      | Same as input 'Input value' | CUR    |       | 0        |
| Previous average     | Average of the previous period  | Same as input 'Input value' | PRV    |       | 0        |
| Pre-previous average | Average of the pre-previous period (i.e. the period before the previous period) | Same as input 'Input value' | PPRV   |       | 0        |

## fxPeriodWatch

### Description

The function 'remembers' that a condition has been valid during a period of time.

A typical example is a transmitter that was overridden with a keypad value.

### Function inputs

| Function inputs | Remark  | EU | SW tag | Range      | Default |
|-----------------|---|----|--------|------------|---------|
| Name            | Name used for tag-prefix and retentive storage.   |    |        |            |         |
| Condition       | The condition to be watched<br>0: Condition is not valid<br><>0: Condition is valid   |    |        |            |         |
| Enabled         | 0: Disabled<br>1: Enabled   |    | EN     |            |         |
| Period type     | Type of period:<br>1: Second<br>2: Minute<br>3: Hour<br>4: Day<br>5: Week<br>6: Month<br>7: Quarter<br>8: Year  |    | TYP    |            |         |
| Period count    | Number of periods (e.g. 5 minutes, 8 hours)   |    | CNT    | 1..1e11    |         |
| Period start    | Absolute start date and time of the period. This will be used as the reference point to calculate the next period rollover from.<br>The value may be defined in the past or the future. The next rollover period will be calculated accordingly (so forwards or backwards in time). |    | START  | <DATETIME> |         |

### Function outputs

| Function outputs   | Remark  | EU | SW tag | Alarm | Fallback |
|--------------------|---|----|--------|-------|----------|
| Current watch      | Indicates whether or not the condition has been valid during the current period:<br>0: Not valid<br>1: Valid  |    | CUR    |       | 0        |
| Previous watch     | Indicates whether or not the condition has been valid during the previous period:<br>0: Not valid<br>1: Valid   |    | PRV    |       | 0        |
| Pre-previous watch | Indicates whether or not the condition has been valid during the pre-previous period (period before the previous period):<br>0: Not valid<br>1: Valid |    | PPRV   |       | 0        |

## fxPID

### Description

PID control is a generic method to control a process variable by means of a feedback control loop and is widely used in the industry.

A PID controller adjusts its control output by applying a Proportional, Integral and Derivative algorithm based on the error between the measured process variable and the desired setpoint.

The Proportional part of the algorithm determines the reaction to the current error. The Integral part reacts to the recent errors accumulated over a sliding time window, while the Derivative part reacts to the change rate of the error. The 3 actions are added up by applying individual weigh factors and the sum is used to adjust a control device, e.g. the position of a control valve.

Note: In flow measurement systems typically only PI control is applied, so the derivative action is disabled.

The Flow-X PID function provides several features for enhanced PID control such as:

- In cascade control there are two PID control loops arranged with one loop controlling the set point of the other loop. Within the outer loop the primary physical parameter is controlled, such as fluid level or velocity. The inner loop reads the output of the outer loop as its set point and usually controls a more rapid changing parameter such as flow rate or acceleration.

- For systems with a slow responsiveness to disturbances or setpoint changes feed forward control may be beneficial. Besides of the closed PID loop an open feed-forward loop is added that reacts immediately to a change in process or setpoint value.
- The function provides the option for bumpless transfers between auto and manual mode and vice versa. The actual process value is copied into the required setpoint value while manual mode is enabled (PV tracking). When reverting to auto mode the process will stay on the current process value. For the same reason the actual output % is copied to the manual output % while Auto mode is enabled.
- When the control output reaches its limit (e.g. control valve is fully opened) there is the risk for wind-up of the integral part, because the error will continue to be integrated. This results in the integral part to become very large, so the error must have the opposite value for a long time before the control loop returns to normal. In order to avoid this windup (i.e. achieve anti-windup) the function compensates the integral part when the control output has reached its limit.
- To avoid that a change in setpoint value will result in an impulse in the control signal the function provides the feature to define a maximum for the setpoint clamp rate and the control output slew rate. The setpoint clamp rate causes the setpoint to change gradually until it has caught up with the required value. The slew rate directly limits the rate of change of the control output.

### Function inputs

| Function inputs         | Remark  | EU   | SW tag | Range | Default |
|-------------------------|---|------|--------|-------|---------|
| Name                    | Optional tag name, tag description and tag group  |      |        |       |         |
| Process value           | This represents the actual process value that is being controlled   | EU   |        |       |         |
| Setpoint value          | The control loop will try to achieve this input value provided that both the 'Manual mode' and 'Cascade mode' are disabled.   | EU   |        |       |         |
| Proportional gain       | Proportional gain factor  | -    |        |       |         |
| Integral gain           | Integral gain factor<br>The value 0 disables the integral part of the PID algorithm   | s    |        |       |         |
| Derivative gain         | Derivative gain factor<br>The value 0 disables the derivative part of the PID algorithm   | s    |        |       |         |
| Low scale value         | Process / setpoint value that corresponds to 0% of the control output   | EU   |        |       |         |
| High scale value        | Process / setpoint value that corresponds to 100% of the control output   | EU   |        |       |         |
| Reverse                 | Selects the direct or reverse action of control<br>0: Forward -> Error = (PV - SP)<br>1: Reverse -> Error = (SP - PV)   |      |        |       | 0       |
| Manual mode             | 0: Disabled<br><> 0: Enabled<br>When this input is enabled the 'Control output %' is set to input 'Manual output %'.<br>When this input is disabled the PID algorithm is applied and either the 'Setpoint value' or Cascade value' is used depending on the 'Cascade mode'. |      |        |       | 0       |
| Manual output %         | The control output % will be set this value when 'Manual mode' is enabled   | %    |        |       | 0       |
| Upwards SP clamp rate   | The setpoint will not be allowed to increase faster than this limit<br>Enter 0 disable this feature   | EU/s |        |       | 0       |
| Downwards SP clamp rate | The setpoint will not be allowed to decrease faster than this limit   | EU/s |        |       | 0       |
| Upwards OP slew rate    | The control output % will not be allowed to increase faster than this limit   | %/s  |        |       | 0       |
| Downwards OP slew rate  | The control output % will not be allowed to decrease faster than this limit   | %/s  |        |       | 0       |
| Low limit value         | The control output % will not be allowed to go below this limit   | %    |        |       | 0       |
| High limit value        | The control output % will not be allowed to go above this limit   | %    |        |       | 100     |
| Manual at startup       | Forces manual mode at restart of flow computer<br>0: Disabled<br>1: Enabled   |      |        |       | 0       |
| Bumpless transfer       | When this input is enabled bump-less transfers between auto and manual mode and vice versa  |      |        |       | 1       |

| Function inputs | Remark  | EU | SW tag | Range | Default |
|-----------------|---|----|--------|-------|---------|
|                 | will be performed.<br>When enabled and when the mode changes from manual to auto, input 'Setpoint value' will be set to the scaled value that corresponds with the current control output %.<br>When the mode changes from auto to manual, then input 'Manual output %' will be set to the current output %.<br>0: Disabled<br><> 0: Enabled  |    |        |       |         |
| Permissive flag | When the Permissive flag is not set the output is forced to the 'Idle output %'<br>This input can be used for user-defined logic<br>0: Disabled<br><> 0: Enabled  |    |        |       | 1       |
| Idle output %   | Value used for control output when the PID permissive flag is not set   |    |        |       | 0       |
| Cascade mode    | 0: Disabled<br><> 0: Enabled<br>When this input is enabled while Manual mode is disabled, the PID algorithm is applied using the 'Cascade input %' (after scaling) as the set point value.  |    |        |       | 0       |
| Cascade input % | The control loop will try to achieve this input value (after scaling) provided that 'Manual mode' is disabled and 'Cascade mode' is enabled<br>Must be linked to the output 'Control output' of the primary PID controller.   | %  |        |       | 0       |
| Tracking mode   | 0: Disabled<br><> 0: Enabled<br>This output is meant for cascade control. If this function acts as the primary (Master) PID controller in a cascade configuration, this input needs to be connected to output 'Tracking mode' of the secondary (Slave) PID function.<br>This input tells this function that the secondary (Slave) PID function is not using its Cascade input, but its Manual output % or Setpoint value instead. This allows the primary PID function to track the secondary process or setpoint value enabling a bumpless transfer between modes.<br>0: Disabled<br><> 0: Enabled |    |        |       | 0       |
| Tracking value  | This output is meant for cascade control. If this function acts as the primary (Master) PID controller in a cascade configuration, this input needs to be connected to output 'Tracking value' of the secondary (Slave) PID function.<br>The value represents the process or setpoint value of the secondary (Slave) PID function as percentage of scale.   | %  |        |       | 0       |
| Feed forward    | Value is directly added to the control output<br>The advantage of feed forward control is that corrective action is taken for a change in a disturbance input before it affects the controlled parameter.   | %  |        |       | 0       |

## Function outputs

| Function outputs | Remark  | EU | SW tag | Alarm | Fallback |
|------------------|---|----|--------|-------|----------|
| Control output   | The actual output value as percentage of scale that shall be used for actual control.<br>Equals the required control output including the slew rate and min/max limitations.  | %  |        |       |          |
| Setpoint value   | The actual setpoint in-use (may differ from the required setpoint because of the SP clamp rate)   | EU |        |       |          |
| Tracking mode    | 0: Disabled<br><> 0: Enabled<br>This output is meant for cascade control. If this function acts as the secondary (Slave) PID controller in a cascade configuration, this input needs to be connected to output 'Tracking mode' of the primary (Master) PID function<br>This output tells the primary (Master) PID function that the Slave PID function is not using the Cascade input, but the Manual output % or Setpoint value instead. This allows the primary PID function to track the secondary process or setpoint value enabling a bumpless transfer between modes. |    |        |       |          |
| Tracking value   | This output is meant for cascade control. If this function acts as the secondary (Slave) PID controller in a cascade configuration, this input needs to be connected to output 'Tracking value' of the primary (Master) PID function<br>The value depends on the Manual and Cascade mode:<br>If Manual mode is enabled, this output equals the percentage of scale of input 'Process value', else this output equals the percentage of scale of input 'Setpoint value'.   | %  |        |       |          |
| Error            | Current error   |    |        |       |          |
| P                | Current proportional part   |    |        |       |          |
| I                | Current integral part   |    |        |       |          |
| D                | Current derivative part   |    |        |       |          |
| v                | Required control output as percentage of scale (refer to section calculations). This output is for information only and shall not be used for actual control  | %  |        |       |          |

|                   |                  |   |
|-------------------|------------------|---|
| <b>Logic</b>      | e <sub>PRV</sub> | error in previous cycle [EU]                        |
| <b>Symbols</b>    | Δu               | control output deviation value [%]                  |
| PV <sub>CUR</sub> | v <sub>CUR</sub> | required control output value in current cycle [%]  |
| PV <sub>PRV</sub> | v <sub>PRV</sub> | required control output value in previous cycle [%] |
| SP <sub>REQ</sub> | u <sub>CUR</sub> | actual control output value in current cycle [%]    |
| SP <sub>CUR</sub> | u <sub>PRV</sub> | actual control output value in previous cycle [%]   |
| SP <sub>PRV</sub> | u <sub>MIN</sub> | low limit for control output [%]                    |
| e <sub>CUR</sub>  | u <sub>MAX</sub> | high limit for control output [%]                   |

|            |                                    |
|------------|------------------------------------|
| $\Delta t$ | calculation cycle time [s]         |
| $K_P$      | Proportional gain factor           |
| $K_I$      | Integral gain factor               |
| $K_D$      | Derivation gain factor             |
| $P$        | Proportional part of current cycle |
| $I_{CUR}$  | Integral part of current cycle     |
| $I_{PRV}$  | Integral part of previous cycle    |
| $D$        | Derivative part of current cycle   |

### Control output logic

The logic for the control output depends on the current manual and tracking modes.

#### Manual mode = Enabled

- Set current output equal to manual input value  
 $V_{CUR} = \text{'Manual output \%'}$

#### Manual mode = Disabled AND Tracking mode = Enabled

- Set current output equal to tracking input value  
 $V_{CUR} = \text{'Tracking value' (input)}$

#### Manual mode = Disabled AND Tracking mode = Disabled

- Determine the current setpoint  
**If cascade mode enabled then**  
 $SP_{CUR} = \text{Cascade input value} * (\text{High scale value} - \text{Low scale value}) + \text{Low scale value}$   
**Else**  
 $SP_{CUR} = SP_{REQ}$
- Check if the current setpoint needs to be gradually ramped up or down to the required setpoint:  
**If**  $(SP_{CUR} - SP_{PRV}) > (\text{Upwards SP clamp rate} * \Delta t)$  **then**  
 $SP_{CUR} = SP_{PRV} + (\text{Upwards SP clamp rate} * \Delta t)$   
**Else if**  $(SP_{PRV} - SP_{CUR}) > (\text{Downwards SP clamp rate} * \Delta t)$  **then**  
 $SP_{CUR} = SP_{PRV} - (\text{Downwards SP clamp rate} * \Delta t)$
- Calculate the current error:  
**If Control direction = Forward then**  
 $e_{CUR} = SP_{CUR} - PV_{CUR}$   
**Else**  
 $e_{CUR} = PV_{CUR} - SP_{CUR}$
- Calculate the Proportional part:  
 $P = K_P * e_{CUR}$

- Calculate the Integral part:  
 $I_{CUR} = I_{PRV} + K_I * \Delta t * (e_{CUR} + (u_{PRV} - v_{PRV}) * (\text{High scale value} - \text{Low scale value}) / 100)$   
 Note: the latter part is required to avoid anti-windup.
- Calculate the Derivative part:  
 $D = K_D / \Delta t * (e_{CUR} - e_{PRV})$
- Calculate the required control output:  
 $V_{CUR} = [P + I_{CUR} + D - \text{Low scale value}] / [\text{High scale value} - \text{Low scale value}]$
- Check if change in control output is within the slew rate  
**If**  $v_{CUR} - u_{PRV} > \text{Upwards slew rate} * \Delta t$  **then**  
 $u_{CUR} = u_{PRV} + (\text{Upwards slew rate} * \Delta t)$   
**Else if**  $\Delta u < - (\text{Downwards slew rate} * \Delta t)$  **then**  
 $u_{CUR} = u_{PRV} - (\text{Downwards slew rate} * \Delta t)$   
**Else**  
 $u_{CUR} = v_{CUR}$
- Check if new control output is outside its limits  
**If**  $u_{CUR} > u_{MAX}$  **then**  
 $u_{CUR} = u_{MAX}$   
**Else If**  $u_{CUR} < u_{MIN}$  **then**  
 $u_{CUR} = u_{MIN}$

### Bumpless transfer logic

If bumpless transfer is enabled, then the following logic is applied.

#### **Setpoint tracking**

IF Manual mode = Enabled OR Tracking mode = Enabled

$$SP_{REQ} = PV_{CUR}$$

ELSE IF Cascade mode = Enabled

$$SP_{REQ} = SP_{CUR}$$

#### **Manual output tracking**

IF Manual mode = Disabled

$$\text{'Manual output \%'} = u_{CUR}$$

#### **Tracking mode and value**

Outputs 'Tracking mode' and 'Tracking value' are set as follows:

#### **Tracking mode**

'Tracking mode' = ('Manual mode' = Enabled) OR ('Cascade mode' = Disabled)

#### **Tracking value**

IF 'Manual mode' = Enabled

$$\text{'Tracking value'} = (PV_{CUR} * - \text{Low scale value}) / (\text{High scale value} - \text{Low scale value}) * 100$$

IF 'Manual mode' = Disabled

$$\text{'Tracking value'} = (SP_{CUR} * - \text{Low scale value}) / (\text{High scale value} - \text{Low scale value}) * 100$$

## fxROCArm

### Description

The function checks if a value does not change its value at a rate that is higher than a specific limit ('rate of change').

### Function inputs

| Function inputs      | Remark   | EU   | SW tag | Range         | Default |
|----------------------|--|--|--------|---------------|---------|
| Name                 | Optional tag name, tag description and tag group |  |        |               |         |
| Input value          | Must be linked to another cell                   | Same as linked cell                                    |        | -1e11..1e11   | 0       |
| Rate of change limit | The unit depends on the 'Deviation type'         | Absolute: Same as input value 1 / s<br>Relative : % /s | ROCLIM | 0..1e11       | 0       |
| Enabled              | Enables or disabled the alarm                    |  |        | True or false | True    |
| Alarm type           | 1: Alarm<br>2: Warning                           |  |        |               | 1       |

### Function outputs

| Function outputs     | Remark                | EU | SW tag | Alarm  | Fallback |
|----------------------|-----------------------|----|--------|--------|----------|
| Rate of change alarm | 0: Normal<br>1: Alarm | -  | ROCALM | ROCALM |          |

### Logic

A 'Rate of change alarm' is raised when the absolute difference between two consecutive values divided by the calculation cycle time in seconds is more than the limit.

## fxSetOnChange

### Description

The 'fxSetOnChange' function sets a tag or cell to a specific value whenever another value changes

### Function inputs

| Function inputs | Remark  | EU | SW tag | Range   | Default |
|-----------------|---|----|--------|---------|---------|
| Module          | Number of the Flow-X/M module.<br>-1 : local module<br>1..8 : module 1 through 8                    |    |        | -1 .. 8 |         |
| Target          | The cell or tag that has to be set. This must be a direct reference to a cell.                      |    |        |         |         |
| Value           | Value to be assigned. May be a constant a formula or a reference to another cell or tag.            |    |        |         |         |
| Change          | A change if this value will set the Target to the Value. This must be a direct reference to a cell. |    |        |         |         |

### Function outputs

| Function outputs | Remark   | EU | SW tag | Alarm | Fallback |
|------------------|--|----|--------|-------|----------|
| Date and time    | Date and time that the most recent change has occurred |    |        |       |          |



## fxSetOnCondition

### Description

The 'fxSetOnCondition' function sets a tag or cell to a specific value whenever a condition is true.

It is a generic function that is especially useful for implementing logic for controlling output signals (e.g. valve commands) and state machines (e.g. prove sequences).

### Function inputs

| Function inputs | Remark  | EU | SW tag | Range   | Default |
|-----------------|---|----|--------|---------|---------|
| Module          | Number of the Flow-X/M module.<br>-1 : local module<br>1..8 : module 1 through 8                        |    |        | -1 .. 8 |         |
| Target          | The cell or tag that has to be set. This must be a direct reference to a cell.                          |    |        |         |         |
| Value           | Value to be assigned. May be a constant a formula or a reference to another cell or tag.                |    |        |         |         |
| Condition       | Boolean expression.<br>When the expression outcome is TRUE (<> 0), then the target is set to the value. |    |        |         |         |

### Function outputs

| Function outputs | Remark  | EU | SW tag | Alarm | Fallback |
|------------------|---|----|--------|-------|----------|
| Date and time    | Date and time that the most recent event has occurred |    |        |       |          |

## fxSetOnEvent

### Description

The 'fxSetOnEvent' function sets a tag to a specific value whenever an event occurs.

It is a generic function that is especially useful for implementing logic for controlling output signals (e.g. valve commands) and state machines (e.g. prove sequences).

### Function inputs

| Function inputs | Remark  | EU | SW tag | Range   | Default |
|-----------------|---|----|--------|---------|---------|
| Module          | Number of the Flow-X/M module.<br>-1 : local module<br>1..8 : module 1 through 8  |    |        | -1 .. 8 | -1      |
| Target          | The cell or tag that has to be set. This must be a direct reference to a cell.  |    |        |         |         |
| Value           | Value to be assigned. May be a constant a formula or a reference to another cell or tag.  |    |        |         |         |
| Event           | Boolean expression.<br>When the expression outcome <u>changes</u> from FALSE to TRUE (or from 0 to <> 0), then the target is set to the value.    |    |        |         |         |
| Condition       | Optional condition that needs to be valid while the event occurs.<br>If the condition is not valid, then the target will not be set to the value. |    |        |         | TRUE    |

### Function outputs

| Function outputs | Remark  | EU | SW tag | Alarm | Fallback |
|------------------|---|----|--------|-------|----------|
| Date and time    | Date and time that the most recent event has occurred |    |        |       |          |

## fxSetIndexOnChange

### Description

The 'fxSetIndexOnChange' function sets one tag from an array of tags to a specific value whenever another value changes.

### Function inputs

| Function inputs | Remark  | EU | SW tag | Range   | Default |
|-----------------|---|----|--------|---------|---------|
| Module          | Number of the Flow-X/M module.<br>-1 : local module<br>1..8 : module 1 through 8                    |    |        | -1 .. 8 | -1      |
| Index           | The index number of the target tag to be set  |    |        |         |         |
| Value           | Value to be assigned. May be a constant a formula or a reference to another cell or tag.            |    |        |         |         |
| Change          | A change if this value will set the Target to the Value. This must be a direct reference to a cell. |    |        |         |         |
| Target 1        | The tag that has to be set when the index number is 1. This must be a direct reference to a cell.   |    |        |         |         |
| Target 2        | The tag that has to be set when the index number is 2. This must be a direct reference to a cell.   |    |        |         |         |
| etc.            |   |    |        |         |         |

### Function outputs

| Function outputs | Remark   | EU | SW tag | Alarm | Fallback |
|------------------|--|----|--------|-------|----------|
| Date and time    | Date and time that the most recent change has occurred |    |        |       |          |

## fxSetIndexOnCondition

### Description

The 'fxSetIndexOnCondition' function sets one tag from an array of tags to a specific value whenever a condition is true.

It is a generic function that is especially useful for implementing logic for controlling output signals (e.g. valve commands) and state machines (e.g. prove sequences).

### Function inputs

| Function inputs | Remark   | EU | SW tag | Range   | Default |
|-----------------|--|----|--------|---------|---------|
| Module          | Number of the Flow-X/M module.<br>-1 : local module<br>1..8 : module 1 through 8                               |    |        | -1 .. 8 | -1      |
| Index           | The index number of the target tag to be set   |    |        |         |         |
| Value           | Value to be assigned. May be a constant a formula or a reference to another cell or tag.                       |    |        |         |         |
| Condition       | Boolean expression.<br>When the expression outcome <u>is</u> TRUE (<> 0), then the target is set to the value. |    |        |         |         |
| Target 1        | The tag that has to be set when the index number is 1. This must be a direct reference to a cell.              |    |        |         |         |
| Target 2        | The tag that has to be set when the index number is 2. This must be a direct reference to a cell.              |    |        |         |         |
| etc.            |  |    |        |         |         |

### Function outputs

| Function outputs | Remark  | EU | SW tag | Alarm | Fallback |
|------------------|---|----|--------|-------|----------|
| Date and time    | Date and time that the most recent event has occurred |    |        |       |          |

## fxSetIndexOnEvent

### Description

The 'fxSetIndexOnEvent' function sets one tag from an array of tags to a specific value whenever an event occurs.

It is a generic function that is especially useful for implementing logic for controlling output signals (e.g. valve commands) and state machines (e.g. prove sequences).

### Function inputs

| Function inputs | Remark   | EU | SW tag | Range   | Default |
|-----------------|--|----|--------|---------|---------|
| Module          | Number of the Flow-X/M module.<br>-1 : local module<br>1..8 : module 1 through 8   |    |        | -1 .. 8 | -1      |
| Index           | The index number of the target tag to be set   |    |        |         |         |
| Value           | Value to be assigned. May be a constant a formula or a reference to another cell or tag.   |    |        |         |         |
| Event           | Boolean expression.<br>When the expression outcome <u>changes</u> from FALSE to TRUE (or from 0 to <> 0), then the target is set to the value. |    |        |         |         |
| Condition       | Condition that needs to be valid while the event occurs.<br>If the condition is not valid, then the target will not be set to the value.       |    |        |         |         |
| Target 1        | The tag that has to be set when the index number is 1. This must be a direct reference to a cell.  |    |        |         |         |
| Target 2        | The tag that has to be set when the index number is 2. This must be a direct reference to a cell.  |    |        |         |         |
| etc.            |  |    |        |         |         |

### Function outputs

| Function outputs | Remark  | EU | SW tag | Alarm | Fallback |
|------------------|---|----|--------|-------|----------|
| Date and time    | Date and time that the most recent event has occurred |    |        |       |          |

fxStatusAlarm

Description

The 'fxStatusAlarm' alarm function generates an alarm that can be triggered by a boolean condition.

Function input

| Function inputs | Remark   | EU | SW tag | Range         | Default |
|-----------------|--|----|--------|---------------|---------|
| Name            | Name for the tag   |    |        |               |         |
| Condition       | A boolean indicating whether the alarm should be triggered |    |        |               |         |
| Enable          | Enables or disables the alarm                              |    |        | True or false | True    |
| Alarm type      | 1: Alarm<br>2: Warning                                     |    |        |               | 1       |

## fxTag

### Description

The 'fxTag' function creates a tag for the cell that contains the 'fxTag' function.

### Function input

| Function inputs | Remark   | EU | SW tag | Range | Default |
|-----------------|--|----|--------|-------|---------|
| Name            | Name for the tag   |    |        |       |         |
| Description     | Description for the tag  |    |        |       |         |
| Value           | May contain a value or a formula.<br>In case of a formula or a reference to a cell or another tag, the tag becomes read-only.<br>On the other hand when it is a value the tag is writable and the specified value is considered at the initial value.  |    |        |       |         |
| Unit            | Defines an engineering unit, enumeration date/time, or a special data type, e.g. 'xt_bool', 'xu_kg_s' or 'xe_period'.  |    |        |       |         |
| Write level     | Applies for writeable tags only.<br>Security access level that is required to write a new value to the tag. Only applies when input 'Value' contains a value and not a formula.<br>When not defined (i.e. function argument is left empty) the tag is only internally writable by a spreadsheet function but not externally writable through the display or communications |    |        |       |         |
| Retentive       | Applies for writable tags only<br>Defines whether or not the value needs to be 'remembered' (retentive).<br>When not defined (i.e. function argument is left empty) the tag is retentive provided that the tag is writable and AutoReset is not enabled  |    |        |       |         |
| AutoReset       | Applies for writeable tags only.<br>Automatically resets the tag to its initial value after it has been written to.  |    |        |       |         |
| Minimum         | Minimum value that is accepted when the tag is externally writable.<br>May be left empty, in which case no minimum check is applied  |    |        |       |         |
| Maximum         | Maximum value that is accepted when the tag is externally writable<br>May be left empty, in which case no maximum check is applied   |    |        |       |         |

### Function output

| Function outputs | Remark  | EU         | SW tag     | Alarm | Fallback |
|------------------|---|------------|------------|-------|----------|
| Value            | Depends on setting 'Mode'<br>Mode = 'This Cell'<br>Cell shows the value or the result of the formula that is defined for input 'Value'<br>Mode = 'Referred Cell'<br>Cell returns TRUE when the 'fxTag' function evaluates successfully or FALSE otherwise | Input Unit | Input Name |       |          |

## fxTimer

### Description

The 'fxTimer' function provides generic timer functionality.

### Function input

| Function inputs | Remark  | EU  | SW tag | Range | Default |
|-----------------|---|-----|--------|-------|---------|
| Name            | Optional tag name, tag description and tag group  |     |        |       |         |
| Start           | Trigger to start the timer.<br>Sets output Running to 1 and starts accumulation of the actual waited time, provided that the Enable condition is true (<> 0)<br>If the timer is already running, then it will be restarted, i.e. the Wait Time will be set to 0 and Elapsed status will be reset to False (in case it was True)   |     | START  |       |         |
| Reset           | Trigger to resets the timer.<br>Sets outputs Elapsed, Running and Wait time to 0  |     | RST    |       |         |
| Limit           | Time-out period for the timer.<br>When the actual wait time is larger than the limit output Elapsed is set to 1.<br>The limit value is expressed in seconds and may contain a fractional part<br>The actual wait time however will be a multifold of the flow computer cycle time.<br>When the limit value does not match an exact number of cycles, then the actual limit value will be rounded upwards to match the 'next' number of cycles. E.g. when the flow computer cycle time is 250 ms and the Limit is set to 3.15 sec, the actual limit value being used will be 3.25 sec. | sec | LIM    |       |         |
| Enable          | Condition that controls the accumulation of actual waited time.<br>0: Disabled<br>1: Enabled<br>When disabled the actual wait time will be frozen until the timer is enabled again.   |     | EN     |       |         |

### Function output

| Function outputs | Remark   | EU  | SW tag | Alarm | Fallback |
|------------------|--|-----|--------|-------|----------|
| Elapsed          | Flag that indicates that timer has timed out, i.e. the actual wait time is larger than the limit   |     | ELAP   |       |          |
| Running          | Flag that indicates that the timer is running, i.e. has been started and not been reset yet, irrespective of the Enable condition  |     | RUN    |       |          |
| Wait time        | Time accumulated since the latest start and while being enabled. When this time reached the limit, the Elapsed output is set to 1. Time will remain accumulated even when the timer has elapsed. | sec | TIM    |       |          |



## fxTotalizerDelta

### Description

The function accumulates a **flow increment** into a cumulative (eternal) total.

Besides of the cumulative total the function also outputs the flow increment that represents the increase in flow quantity in the last calculation cycle. This increment value serves as an input for related batch and period flow-weighted averaging and totalization functions.

### Function input

| Function inputs | Remark   | EU                       | SW tag | Range   | Default |
|-----------------|--|--------------------------|--------|---------|---------|
| Name            | Optional tag name, tag description and tag group and retentive storage.  |                          |        |         |         |
| Flow increment  | Actual flow increment to be accumulated.<br>Negative values will be ignored, so the cumulative total will not decrease.  | Defined by 'Input unit'  |        | 0..1e11 |         |
| Enabled         | Dictates whether the flow accumulation is enabled or not. When disabled the cumulative total will not be updated and the increment will be set to 0.<br>0: Disabled<br>1: Enabled                  |                          | EN     |         |         |
| Input unit      | Unit of input 'Flow increment'.  |                          |        |         |         |
| Output unit     | Unit to be used for total and increment.<br>Refer to the next section 'Unit conversion' for more information.<br>Changing the unit will only be possible when the cumulative total value equals 0. |                          |        |         |         |
| Rollover value  | The cumulative total will be reset to 0 when it reaches the rollover value   | Defined by 'Output unit' | ROVAL  | 0..1e15 | 1e12    |
| Decimal places  | Defines the number of decimal places for the total and increment output values.<br>-1 means full precision (no rounding applied)   |                          | DECPLS | -1..10  | -1      |
| Reset           | This should be used with great care!<br>Command to reset the cumulative total to 0<br>0: No reset<br>1: Reset  |                          |        |         | 0       |

Note: As opposed to the flow increment input value, the flow increment output value is set to 0 when the totalization is disabled and has the proper units and is therefore better suited as input for other functions.

### Function output

| Function outputs         | Remark  | EU                      | SW tag | Alarm   | Fallback |
|--------------------------|---|-------------------------|--------|---------|----------|
| Cumulative total         | Total quantity accumulated so far since the last rollover or reset  | Defined by 'Input unit' | CUM    |         |          |
| Increment                | Increment in last calculation cycle   | Defined by 'Input unit' | INCR   |         |          |
| Rollover flag            | Flag indicating a rollover to 0.<br>0: Off<br>1: On<br>Note: stays 'On' for one cycle only.   |                         |        | ROALM   |          |
| Reset flag               | Flag indicating a reset to 0.<br>0: Off<br>1: On<br>Note: stays 'On' for one cycle only   |                         |        | RESET   |          |
| Recoverable reload error | Flag that indicates that at startup only 2 of the 3 copies were equal and that that value is used as the initial total.<br>0: Off<br>1: On<br>Note: stays 'On' for one cycle only |                         |        | RTOTERR |          |
| Fatal reload error       | Flag that indicates that at startup all 3 copies were different and the total was reset to 0<br>0: Off<br>1: On<br>Note: stays 'On' for one cycle only                            |                         |        | FTOTERR |          |

### Unit conversion

The function will automatically apply the required conversion based on the unit of the flow increment input value (Input unit) and the selected 'Output unit' for the flow quantity.

E.g. when flow rate input is in 'scf' the output unit is 'MMscf' then the following conversions are applied:

- 1 The flow increment input value is converted to the corresponding base unit, which is 'sm3' for a 'Volume' unit

- 2 The flow increment is converted from 'sm3' to 'MMscf' before the cumulative total and increment output values are updated.

Similar conversions are applied for flow increments that are expressed in mass, volume, normal volume and energy units.

## fxTotalizerRate

### Description

The function accumulates a **flow rate** into a cumulative (eternal) total.

Besides of the cumulative total the function also outputs the flow increment that represents the increase in flow quantity in the last calculation cycle. This increment value serves as an input for related batch and period flow-weighted averaging and totalization functions.

### Function inputs

| Function inputs | Remark   | EU                       | SW tag | Range   | Default |
|-----------------|--|--------------------------|--------|---------|---------|
| Name            | Optional tag name, tag description and tag group and retentive storage.  |                          |        |         |         |
| Flow rate       | Actual flow rate to be accumulated.<br>Negative values will be ignored, so the cumulative total will not decrease.   | Defined by 'Input unit'  |        | 0..1e11 |         |
| Enabled         | Dictates whether the flow accumulation is enabled or not. When disabled the cumulative total will not be updated and the increment will be set to 0.<br>0: Disabled<br>1: Enabled                  |                          | EN     |         |         |
| Input unit      | Unit of input 'Flow rate.'   |                          |        |         |         |
| Output unit     | Unit to be used for total and increment.<br>Refer to the next section 'Unit conversion' for more information.<br>Changing the unit will only be possible when the cumulative total value equals 0. |                          |        |         |         |
| Rollover value  | The cumulative total will be reset to 0 when it reaches the rollover value   | Defined by 'Output unit' | ROVAL  | 0..1e15 | 1e12    |
| Decimal places  | Defines the number of decimal places for the total and increment output values.<br>-1 means full precision (no rounding applied)   |                          | DECPLS | -1..10  | -1      |
| Reset           | This should be used with great care!<br>Command to reset the cumulative total to 0<br>0: No reset<br>1: Reset  |                          |        |         | 0       |

### Function output

| Function outputs | Remark  | EU                      | SW tag | Alarm  | Default |
|------------------|---|-------------------------|--------|--------|---------|
| Cumulative total | Total quantity accumulated so far since the last rollover or reset  | Defined by Input unit'  | CUM    |        |         |
| Increment        | Increment in last calculation cycle   | Defined by 'Input unit' | INCR   |        |         |
| Rollover flag    | Flag indicating a rollover to 0.<br>0: Off<br>1: On<br>Note: stays 'On' for one cycle only.   |                         |        | ROALM  |         |
| Reset flag       | Flag indicating a reset to 0.<br>0: Off<br>1: On<br>Note: stays 'On' for one cycle only   |                         |        | RESET  |         |
| Reload warning   | Flag that indicates that at startup only 2 of the 3 copies were equal and that that value is used as the initial total.<br>0: Off<br>1: On<br>Note: stays 'On' for one cycle only |                         |        | RLWARN |         |
| Reload error     | Flag that indicates that at startup all 3 copies were different and the total was reset to 0<br>0: Off<br>1: On<br>Note: stays 'On' for one cycle only                            |                         |        | RLERR  |         |

### Unit conversion

The function will automatically apply the required conversion based on the unit of the flow rate input value (Input unit) and the selected 'Output unit' for the flow quantity.

E.g. when flow rate input is in 'kg/hr' the selected unit is 'tonne' then the following conversions are applied:

1. The flow rate value is converted to the corresponding base unit, which is 'kg/s' for a 'Mass per Time' unit
2. The flow increment over the last calculation cycle is calculated from the 'kg/s' value and the actual calculation cycle time, resulting in a value expressed in 'kg' (i.e. the base unit for 'Mass').

3. The flow increment is converted from 'kg' to 'tonne' before the cumulative total and increment output values are updated.

Similar conversions are applied for flow rates that are expressed in volume, standard volume, normal volume and energy units.

## fxWatchUpdate

### Description

This function raises a flag whenever a value has been updated in the latest calculation cycle.

It is a generic function that can be used for any purpose, e.g. to report the number of times that a gas chromatograph has sent updates of the gas composition.

Use function fxTotalizerDelta to accumulate the number of times the flag has been raised.

### Function input

| Function inputs | Remark  | EU | SW tag  | Range | Default |
|-----------------|---|----|---------|-------|---------|
| Name            | Optional tag name, tag description and tag group  |    |         |       | <Empty> |
| Value           | The value that needs to be checked for updates  |    | VAL     |       | 0       |
| Neglect zeros   | Controls if the value 0 has to be considered as an update or not.<br>0: Disabled<br>The value 0 is also an update<br>1: Enabled<br>The value 0 is not considered as an update |    | NGLZERO |       | 0       |

### Function output

| Function outputs | Remark  | EU | SW tag     | Alarm | Fallback |
|------------------|---|----|------------|-------|----------|
| UpdateFlag       | Update flag<br>0: Value has not changed<br>1: Value has not changed<br>Flag is automatically cleared (set to 0) at next cycle |    | UPDATEFLAG |       | 0        |



## 4 Flow-X IO Functions

This chapter lists all available Flow-X IO functions. Please refer to the pinouts for your specific model of flow computer in the installation manual provided with the Spirit Flow Suite software.

### fxAnalogInput

#### Description

Each flow module supports a maximum of 6 analog input signals. The first 2 signals can be used as either a mA/VDC input or as a RTD input.

The Analog input function is used for mA and VDC inputs. For RTD inputs refer to function 'RTD Input'.

Analog signals are sampled at a rate of about 15 Hz. Every calculation cycle the samples are averaged and the average is scaled to a value in engineering units.

The output value can be equal to either the last sample or the average of the samples of the last calculation cycle. The average is either the arithmetic mean or the Root of the Mean of the Squares (RMS), Where the latter is meant for a differential pressure signal of a primary flow device (e.g. an orifice plate)

The input signal is considered to be faulty when the input circuitry has an open or a short circuit or when the measured value is outside a configurable range.

Note: Function fxKeypadfallback provides the option to force the analog input value to a specific fallback value in case it should fail. It also provides the option to force the input value to a keypad value e.g. upon user request.

#### Function inputs

| Function inputs | Remark   | EU | SW tag | Range | Default |
|-----------------|--|----|--------|-------|---------|
| Name            | Optional tag name, tag description and tag group     |    |        |       |         |
| Channel number  |  |    | CHAN   | 1..6  | 1       |
| Input type      | 1: 4-20 mA<br>2: 0-20 mA<br>3: 1-5 VDC<br>4: 0-5 VDC |    | INPTYP |       | 2       |
| Averaging type  | 1: Arithmetic mean<br>2: Root Mean Square            |    | AVGTYP |       | 1       |

#### Function outputs

| Function outputs | Remark   | EU | SW tag | Alarm | Fallback |
|------------------|--|----|--------|-------|----------|
| Status           | 0: Normal<br>1: Function Input argument out of range |    | STS    | FLOOR |          |
| Percentage value | Actual percentage of scale value                     | %  | PERC   |       | 0        |

## fxAnalogOutput

### Description

This function configures a single 4-20 mA output channel on the local Flow-X module. Use function 'fxSetAnalogOutput' to control the actual output signal.

The output current is either set directly or gradually changed to the required set point based on the specified filter method.

### Function inputs

| Function inputs | Remark  | EU   | SW tag | Range | Default |
|-----------------|---|------|--------|-------|---------|
| Name            | Optional Optional tag name, tag description and tag group                   |      |        |       | <Empty> |
| Channel number  |   | 1..4 | CHAN   |       | 0       |
| Filter setpoint | 0 .. 15<br>0: No filtering<br>1: Fastest filter<br>..<br>15: Slowest filter |      | FILSP  |       | 0       |

### Function outputs

| Function outputs | Remark   | EU | SW tag | Alarm | Fallback |
|------------------|--|----|--------|-------|----------|
| Status           | 0: Normal<br>1: Function Input argument out of range             |    | STS    | FIOOR |          |
| Percentage value | The actual (and filtered) output value expressed as a percentage | %  | PERC   |       | 0        |

## fxSetAnalogOutput

### Description

This function writes an analog value to an output. Make sure that the analog output has been set up by calling fxAnalogOutput first.

### Function inputs

| Function inputs | Remark  | EU   | SW tag | Range  | Default |
|-----------------|---|------|--------|--------|---------|
| Name            | Optional Optional tag name, tag description and tag group                   |      |        |        | <Empty> |
| Module          | Not used, set to -1   |      |        | -1..16 | -1      |
| Channel number  |   | 1..4 | CHAN   |        | 0       |
| Filter setpoint | 0 .. 15<br>0: No filtering<br>1: Fastest filter<br>..<br>15: Slowest filter |      | FILSP  |        | 0       |

### Function outputs

| Function outputs | Remark   | EU | SW tag | Alarm | Fallback |
|------------------|--|----|--------|-------|----------|
| Status           | 0: Normal<br>1: Function Input argument out of range |    | STS    | FIOOR |          |

## fxDigitalInput

### Description

The Digital Input function processes a single digital input and outputs either the actual input signal or the latched input signal.

### Function inputs

| Function inputs | Remark   | EU | SW tag    | Default |
|-----------------|--|----|-----------|---------|
| Name            | Optional tag name, tag description and tag group   |    |           |         |
| Channel number  | 1..16  |    | CHAN      | 1       |
| Logic           | 1: Positive<br>2: Negative   |    | LOGIC     | 1       |
| Mode            | 1: Actual<br>2: Latched  |    | MODE      | 1       |
| Threshold       | Each digital input has 2 threshold levels that determine whether the signal is considered to be either high (above the threshold) or low (below the threshold).<br>The threshold levels are as follows (all relative to signal ground):<br><br>Channels 1 through 8:<br>1: + 1.25 Volts<br>2: + 12 Volts<br><br>Channels 9 through 16:<br>1: + 3.75 Volts<br>2: + 12 Volts |    | THRESHOLD | 1       |

### Function outputs

| Function outputs | Remark  | SW tag   | Alarm | EU |
|------------------|---|----------|-------|----|
| Status           | 0: Normal<br>1: Input argument out of range   | STS      | FLOOR | -  |
| Signal State     | 0: Off<br>1: On<br>Meaning depends on the input Logic and Mode, refer to the table below. | SIGSTATE |       | -  |

### Calculations

The following table summarizes the relationship between the input signal and the output 'State', depending on the inputs 'Logic and 'Mode'.

| Logic    | Mode    | Signal state = Off                                     | Signal State = On                                  |
|----------|---------|--|--|
| Positive | Actual  | Actual signal is low                                   | Actual signal is high                              |
| Positive | Latched | Signal has not been high during last calculation cycle | Signal has been high during last calculation cycle |
| Negative | Actual  | Actual signal is high                                  | Actual signal is low                               |
| Negative | Latched | Signal has not been low during last calculation cycle  | Signal has been low during last calculation cycle  |



## fxDigitalOutput

### Description

The Digital Output function configures a single digital output on the local module. Use function 'fxSetDigitalOutput' to control the actual output signal.

### Function inputs

| Function inputs         | Remark   | EU | SW tag    | Range | Default |
|-------------------------|--|----|-----------|-------|---------|
| Name                    | Name for output 'Signal State'   |    |           |       |         |
| Channel number          | One of the 16 digital I/O channels.  |    | CHAN      | 1..16 | 1       |
| Logic                   | 1: Positive<br>2: Negative   |    | LOGIC     |       | 1       |
| Delay                   | Period of time that the control signal must be high (> 0) without interruption before the output will be activated.<br>The value 0 disables the delay function<br>If the control signal becomes 0 before the time has elapsed, then the output signal will not be activated. | ms | DELAY     | >= 0  | 0       |
| Minimum activation time | Minimum period of time that the signal will remain activated.<br>After the minimum activation time has elapsed the output signal will remain activated until the control value becomes 0.  | ms | MINACTITM | >= 0  | 0       |

### Function outputs

| Function outputs | Remark  | SW tag   | Alarm | EU | Fallback |
|------------------|---|----------|-------|----|----------|
| Status           | 0: Normal<br>1: Input argument out of range or conflict | STS      | FLOOR | -  | 0        |
| Signal State     | 0: Not activated<br>1: Activated                        | SIGSTATE |       | -  | 0        |

### Calculations

The following table summarizes the relationship between the output signal, the input 'Logic and the control value as set by function 'fxSetDigitalOutput'.

## fxSetDigitalOutput

### Description

This function writes a value to a configured digital output.

### Function inputs

| Function inputs | Remark   | EU | SW tag | Range  | Default |
|-----------------|--|----|--------|--------|---------|
| Name            | Name for output 'Signal State'   |    |        |        |         |
| Module          | Unused, set to -1  |    |        | -1..16 | -1      |
| Channel number  | One of the 16 digital i/o channels.  |    |        | 1..16  |         |
| Setpoint        | Logic is positive:<br>0: Output is activated<br><>0: Output is not activated<br>Logic is negative:<br>0: Output is not activated<br><>0: Output is activated |    |        |        |         |

### Function outputs

| Function outputs | Remark  | SW tag | Alarm | EU | Fallback |
|------------------|---|--------|-------|----|----------|
| Status           | 0: Normal<br>1: Input argument out of range or conflict | STS    | FLOOR | -  | 0        |

fxFrequencyOutput

Description

This function provides a programmable output frequency on one of the digital pins. The frequency as well as the duty cycle are user programmable. When using the frequency output to configure a dual pulse system, channel 2 can be configured.

Function inputs

| Function inputs  | Remark  | EU | SW tag | Range | Default |
|------------------|---|----|--------|-------|---------|
| Name             |   |    |        |       |         |
| Index            | Index of the frequency output                           |    |        | 1..4  |         |
| Channel number   | Output channel number, the digital IO pin that is used. |    |        | 0..16 |         |
| Channel number 2 | Output channel number, the digital IO pin that is used. |    |        | 0..16 | 0       |

Function outputs

| Function outputs | Remark  | SW tag | Alarm | EU | Fallback |
|------------------|---|--------|-------|----|----------|
| Status           | 0: Normal<br>1: Input argument out of range or conflict | STS    | FLOOR | -  | 1        |

## fxSetFrequencyOutput

### Description

This function starts a programmed frequency on the digital pin, set by fxFrequencyOutput. In case of a dual pulse via frequency out, here the phase shift between the pins can be configured.

### Function inputs

| Function inputs | Remark   | EU | SW tag | Range        | Default |
|-----------------|--|----|--------|--------------|---------|
| Name            |  |    |        |              |         |
| Module          | Not used, set to -1  |    |        | -1..16       | -1      |
| Index           | Index of the frequency output  |    |        | 1..4         |         |
| Frequency       | Output frequency (Hz)  | Hz |        | 0.01.. 10000 |         |
| Duty cycle      | Duty cycle   | %  |        | 0..100       |         |
| Enabled         | Enables (<>0) or disables (0) the output signal.   |    |        |              |         |
| Phase shift     | Phase shift between dual pulse channel A and B expressed as the ratio of the time delay between the last A and B and the time between two A pulses. A typical phase difference is 90° corresponding to a value of 0.25.<br>The shift is limited to [0°..180°]. |    |        | 0..0.5       | 0       |

### Function outputs

| Function outputs  | Remark   | SW tag  | Alarm | EU | Fallback |
|-------------------|--|---------|-------|----|----------|
| Status            | 0: Normal<br>1: Input argument out of range or conflict  | STS     | FIOOR | -  | 1        |
| Actual frequency  | Actual frequency, which can deviate from the programmed frequency because of hardware limitations. | ACTFREQ |       | Hz | 0        |
| Actual duty cycle |  | ACTDC   |       | %  | 0        |

## fxDoubleChronometry

### Description

The function provides double chronometry measurement for meter proving and calibration purposes with a resolution of 100 nanoseconds.

The function monitors a (dual) pulse input signal provided by the meter under test and by one or more digital signals that represent the start and stop of the measurement.

The digital inputs used for start and stop of the measurement are typically connected to the sphere detector switches of a pipe prover or the piston detectors of a compact prover.

The start / stop signal may also be any other type of signal, e.g. a digital output from another flow computer. This allows for flexible master meter configurations in which a single prove measurement is performed by two separate flow computers, one that monitors the meter under test and one that monitors the reference or master meter.

By using multiple Double Chronometry functions multiple prove measurements can be performed at the same time by one and the same flow module.


Some examples of simultaneous prove measurements are:

- For a prover with 2 begin and 2 end detector switches the flow meter can be proved against all 4 the calibrated prover volumes at the same time.

- With 2 detectors at one end of the prover (A and B) and 2 at the other end (C and D) there are 4 possible detector combinations A-C, A-D, B-C and B-D, resulting in four available prover volumes. By defining 4 Prove measurement functions all 4 prove volumes can be used to prove the meter by a single prove sequence. The operator selects the primary detector combination that will be used for calculating the new K factor or meter factor. The result of the 4 detector combinations are compared to each other and an alarm is raised in case of discrepancy.
- Meters that operate in series can all be proved at the same time.
- For meters that provide more than flow signal all signals can be proved at the same time
- For provers with a range of calibrated prover volumes to accommodate proving of meters of different capacities, multiple prover volumes can be processed at the same time.

Combinations of these scenarios are possible as well.

The double chronometry method comprises the measurement of the time between the start and stop signals and the time between the two meter pulses that immediately follow the start and stop signals. The flow module then determines the interpolated number of meter pulses that correspond to the measurement start and stop signals as follows:

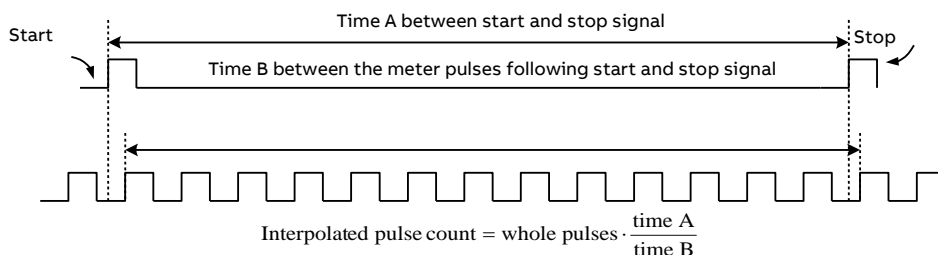

### Function inputs and outputs

| Function inputs            | Remark   | EU  | SW tag     | Range  | Default |
|----------------------------|--|-----|------------|--------|---------|
| Name                       | Optional tag name, tag description and tag group   |     |            |        |         |
| Index                      | Index number   |     | INDEX      | 1..4   | 1       |
| Flow input channel number  | Number of the digital input channel  |     | FLOWCHAN   |        |         |
| Start DI channel number    | Channel number of the digital input that is to be used as the Start signal   |     | STRTCHAN   |        | 0       |
| Start DI logic             | 1: Positive<br>2: Negative   |     | STRTLOGIC  | 1..2   |         |
| Stop DI channel number     | Channel number of the digital input that is to be used as the Stop signal.<br>Note: the same digital input may be used for both Start and Stop of measurement  |     | STOPCHAN   |        | 0       |
| Stop DI logic              | 1: Positive<br>2: Negative   |     | STOPLOGIC  | 1..2   |         |
| Start minimum delay time * | After the Reset command has been given the function will wait for at least this delay time before considering the activation of the Start digital input  | sec | STRTMINDLY | 0..1e9 | 0       |
| Start maximum delay time * | After the Reset command has been given the function will wait for no longer than this delay time before the Start digital input must have been activated<br>0 disables this delay check  | sec | STRTMAXDLY | 0..1e9 | 0       |
| Stop minimum delay time *  | After the Reset command has been given the function will wait for at least this delay time before considering the activation of the Stop digital input.<br>0 disables this delay check<br>Note: The stop minimum delay time must be defined when a common digital input is used as both the Start and Stop signals | sec | STOPMINDLY | 0..1e9 | 0       |

| Function inputs                 | Remark  | EU  | SW tag     | Range  | Default |
|---------------------------------|---|-----|------------|--------|---------|
| Stop maximum delay time *       | After the Reset command has been given the function will wait for no longer than this delay time before the Stop digital input must have been activated.<br>0 disables this delay check   | sec | STOPMAXDLY | 0..1e9 | 0       |
| Number of pulses per revolution | Applies for flow meter that provide a direct pulse signal (typically turbine and Positive Displacement (PD) meters)<br>To exclude the influence of geometrical imperfections of the primary metering device the function may be forced to accumulate a number of pulses that corresponds to a whole number of flow meter revolutions.<br>E.g. suppose that at the stop signal 6754 pulses have been accumulated and that corresponding turbine meter provides 20 pulses for each turbine revolution, the function will accumulate another 6 pulses before the measurement is stopped. |     | PLSPERREV  | 1..1e9 | 1       |
| Start                           | 0 No action<br><> 0 Starts the double chronometry<br>If the double chronometry function is already running, then it will be restarted.  |     | START      |        | 0       |
| Reset                           | 0 No action<br><> 0 Resets all outputs to 0 or, where applicable, FALSE.  |     | RST        |        |         |

### Function outputs

| Function outputs            | Remark   | SW tag   | Alarm | EU  |
|-----------------------------|--|----------|-------|-----|
| Status                      | 0: Normal<br>1: Input argument out of range or conflict  | STS      | FLOOR | -   |
| Interpolated pulse count    | Equals :<br>Whole pulse count * Time A / Time B<br>According to API requirements the interpolated pulse count should be used when less than 10000 pulses are acquired  | INPOLCNT |       |     |
| Whole pulse count           | The number of meter pulses that were acquired within the measurement period (time B).<br>Could be used instead of interpolated pulses when more than 10000 pulses are acquired<br>Note: Whole pulse count = the decimal part of Interpolated pulse count | WHOLECNT |       |     |
| Time between start and stop | Time period between start and stop signal  | INPOLTIM |       | sec |
| Time between pulses         | Time between the meter pulses immediately following the start and stop signals   | WHOLETIM |       | sec |
| In Progress                 | Status bit that indicates that the measurement is in progress  | INPRG    |       |     |
| Completed                   | Prove measurement has been completed   | COMPL    |       |     |
| Start time-out              | Prove measurement has been aborted - Start signal time-out   | STRTTO   |       |     |
| Stop time-out               | Aborted - Stop signal time-out   | STOPTO   |       |     |

## fxPulseInput

### Description


The 'fxPulseInput' function is meant for a flow meter that provides a single or a dual pulse output signal. Each flow module supports either 1 single or 1 dual pulse input.

A dual pulse signal is a set of two pulse signals ('pulse trains') A and B that originate from the same flow meter. The two pulse trains are similar but shifted in phase (typically 90°).

The primary purpose of the dual signal is to allow for **pulse integrity checking**. Added or missing pulses on either pulse train are detected and corrected for and simultaneous noise pulses are rejected.

The function provides detailed information on the raw, corrected and bad pulses for both channels and for both the forward and reverse flow direction.

The phase shifted pulse train signal also allows for automatic detection of flow direction. Each A pulse is followed by a B pulse within a time period ( $\Delta t$ ) in case the flow runs in the forward direction. In case the flow runs in the reverse direction, the opposite is the case, i.e. each B pulse is followed by an A pulse within the same time period  $\Delta t$ .

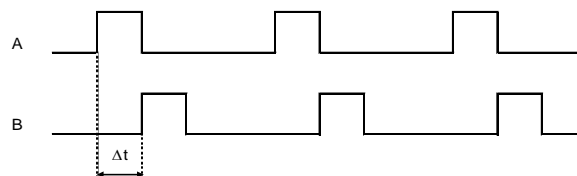

Channel B lags channel A

The function also provides the option to output the raw pulse signals, which is useful in case a separate flow computer is used for proving purposes. The proving flow computer takes the pulse output from the flow computer that processes the meter on prove to perform prove measurements including double chronometry if required. The prover output signal is generated at 20 MHz, the same frequency at which the raw pulse input signals are sampled.

### Compliance

ISO 6551:1982, Petroleum liquids and gases -- Fidelity and security of dynamic measurement -- Cabled transmission of electric and/or electronic pulsed data

Note: The Flow/X series of flow computers provides Level A pulse security as defined in ISO 6551, which means that bad pulses are not only detected (level B) but also corrected for.

### Function inputs

| Function inputs           | Remark  | EU | SW tag | Range     | Default             |
|---------------------------|---|----|--------|-----------|---------------------|
| Name                      | Optional tag name, tag description and tag group  |    |        |           |                     |
| Index                     | Index number. Always 1.   |    | INDEX  | 1..1      | 1                   |
| Channel A                 | Input channel number for pulse A<br>0 disables the entire function  |    | CHANA  | 0..16     | 0                   |
| Channel B                 | Input channel number for pulse B<br>Enter 0 in a case of single pulse input   |    | CHANB  | 0..16     | Input Channel A + 1 |
| Pulse fidelity threshold  | All pulse fidelity checking will be disabled when the corrected pulse frequency is below the 'Pulse fidelity threshold'<br>Enter a 0 to disable this functionality (the default value)<br>Note: In FPGA later than v13, pulse fidelity checking is always enabled | Hz | FRQTHD | 0..1e5    | 0                   |
| Error pulses limit        | When the total number of missing pulses, added and simultaneous pulses for either channel becomes larger than this value, the status becomes 'Error Pulses'<br>The value 0 disables the error pulses limit check.   |    | ERRLIM | 0..1e99   | 0                   |
| Missing pulses limit      | When the total number of missing pulses on channel A or B becomes larger than this value, the status becomes 'Missing Pulses Channel x' (with x either A or B)<br>The value 0 disables the missing pulses limit check.  | -  | MISLIM | 0..1e99   | 0                   |
| Added pulses limit        | When the total number of added pulses on channel A or B becomes larger than this value, the status becomes 'Added Pulses Channel x' (with x either A or B)<br>The value 0 disables the added pulses limit check.  | -  | ADDLIM | 0..1e99   | 0                   |
| Simultaneous pulses limit | When the total number of simultaneous pulses on both channels becomes larger than this value, the status becomes 'Simultaneous Pulses'<br>The value 0 disables the simultaneous pulses limit check.   | -  | SIMLIM | 0..1e99   | 0                   |
| Good pulse reset limit    | When the number of good pulses since the last 'bad' pulse has reached this value, all the bad pulse count and alarms will be reset automatically.<br>The value 0 disables the automatic reset function.   | -  | RSTLIM | 0..1e99   | 0                   |
| Bad pulse reset command   | When the value changes the bad pulse count and alarms are reset. Can be used reset the bad pulses manually or automatically e.g. at a every new batch.  | -  | RSTCMD | Any value | 0                   |
| Error rate limit          | When the difference in frequency between the two raw pulse trains is larger than this limit within the last calculation cycle, the status becomes 'Pulse Rate Error'<br>The value 0 disables the error rate limit check   | %  | ERRLIM | 0..100    | 0                   |

| Function inputs        | Remark  | EU | SW tag  | Range | Default |
|------------------------|---|----|---------|-------|---------|
| Pulse A output channel | Number of digital I/O channel that is used to output the raw A pulses.<br>0: Not used<br>1: Digital I/O channel 1<br>..<br>16: Digital I/O channel 16 | -  | POCHANA |       | 0       |
| Pulse B output channel | Number of digital I/O channel that is used to output the raw B pulses.<br>0: Not used<br>1: Digital I/O channel 1<br>..<br>16: Digital I/O channel 16 | -  | POCHANA |       | 0       |
| Pulse A output mode    | Used to switch the pulse A output on and off.<br>0: Pulse output A is disabled<br><> 0: Pulse output A is enabled                                     |    | POMODA  |       | 0       |
| Pulse B output mode    | Used to switch the pulse B output on and off.<br>0: Pulse output B is disabled<br><> 0: Pulse output B is enabled                                     |    | POMODA  |       | 0       |

### Function outputs

| Function outputs              | Remark   | EU | SW tag | Alarm   | Fallback |
|-------------------------------|--|----|--------|---|----------|
| Status                        | 0: Normal<br>1: Input argument out of range<br>2: No A pulses (while B pulses)<br>3: No B pulses (while A pulses)<br>4: Missing pulses channel A<br>5: Missing pulses channel B<br>6: Added pulses channel A<br>7: Added pulses channel B<br>8: Simultaneous pulses<br>9: Pulse rate error<br>10: Low frequency (above 0 and below cut-off)<br>11: Error pulses<br>Note: during normal operation status 'Low frequency' occurs for a relative short time whenever the flow starts or stops. In order to avoid unnecessary alarms the corresponding alarm delay time shall be defined accordingly (default 5 sec) | -  | STS    | FLOOR<br>NOPLSA<br>NOPLSB<br>MISPLSA<br>MISPLSB<br>ADDPLSA<br>ADDPLSB<br>SIMPLS<br>ERRRATE<br>LOFRQ<br>ERRPLS |          |
| Corrected pulse increment     | Number of good pulses within the last calculation cycle  | -  |        | CORINC  |          |
| Corrected frequency           | Frequency that corresponds to the last corrected pulse increment within the last calculation cycle   | Hz |        | CORFRQ  |          |
| Error pulse increment         | Number of bad pulses within the last calculation cycle   |    |        | ERRINC  |          |
| Error pulse frequency         | Frequency that corresponds to the last error pulse increment within the last calculation cycle   | Hz |        | ERRFRQ  |          |
| Flow direction                | 0: Forward<br>1: Reverse   | -  |        | FLOWDIR   |          |
| Raw pulse increment channel A | Number of raw pulses on channel A within the last calculation cycle  |    |        | RAWINCA   |          |
| Raw pulse increment channel B | Number of raw pulses on channel B within the last calculation cycle  |    |        | RAWINCB   |          |
| Missing pulse count channel A | Depends on FPGA version:<br>• FPGA v13 and earlier: Total missing pulse count channel A since the last reset<br>• FPGA following v13: Total number of B pulses while channel A was determined to be missing since the last reset   | -  |        | MISCNTA   |          |
| Missing pulse count channel B | Depends on FPGA version:<br>• FPGA v13 and earlier: Total missing pulse count channel B since the last reset<br>• FPGA following v13: Total number of A pulses while channel B was determined to be missing since the last reset   | -  |        | MISCNTB   |          |
| Added pulse count channel A   | Depends on FPGA version:<br>• FPGA v13 and earlier: Total added pulse count channel A since the last reset<br>• FPGA following v13: Total A pulses without preceding B pulse since the last reset, when missing channel is not determined  | -  |        | ADDCNTA   |          |
| Added pulse count channel B   | Depends on FPGA version:<br>• FPGA v13 and earlier: Total added pulse count channel B since the last reset<br>• FPGA following v13: Total B pulses without preceding A pulse since the last reset, when missing channel is not determined  | -  |        | ADDCNTB   |          |
| Simultaneous pulses           | Total simultaneous pulse count since the last reset  |    |        | SIMPLSF   |          |
| Phase difference              | Last measured phase difference between A and B pulse expressed as the ratio of the time delay between the last A and B and the time between two A pulses. A typical phase difference is 90° corresponding to a value of 0.25.  | -  |        | PHASEDIF  |          |



## fxResetPulseInputErrors

### Description

This function resets the error pulse counters (error, added, missing and simultaneous pulses) of the pulse input of one of the modules part of the same configuration.

It is required that the pulse input of the specified module is configured by function 'fxPulseInput'.

### Function inputs

| Function inputs | Remark  | EU | SW tag | Range | Default |
|-----------------|---|----|--------|-------|---------|
| Name            | Optional tag name, tag description and tag group  |    |        |       | <Empty> |
| Module          | Unused, set to 0  |    |        | 0..16 | 0       |
| Index           | Index number as defined in the corresponding fxPulseInput function<br>0 disables the function |    |        | 0..1  |         |
| Reset           | 0: No action<br><> 0 All error counters are reset to 0  |    |        |       |         |

### Function outputs

| Function outputs | Remark   | EU | SW tag | Alarm | Fallback |
|------------------|--|----|--------|-------|----------|
| Status           | 0: Normal<br>1: Input argument out of range or in conflict | -  | STS    |       | FLOOR    |

## xPulseOutput

### Description

This function is used to feed pulses to an electro-mechanical (E/M) counter. There are 4 pulse output units, to be selected by the index parameter. The function uses a reservoir to accumulate the pulses. On one hand the number of pulses that need to be added to the reservoir is calculated from inputs 'Increment' and 'Significance factor'. On the other hand pulses are taken from the reservoir and fed to the E/M counter at a rate that will not exceed the specified output rate.

This can also be used to configure a dual pulse situation, for this case you can configure a second channel and the delay it has on the primary channel.

### Function inputs

| Function inputs       | Remark   | EU | SW tag  | Range   | Default |
|-----------------------|--|----|---------|---------|---------|
| Name                  | Optional tag name, tag description and tag group   |    |         |         |         |
| Index                 | Index number 1..4.   |    | INDEX   | 1..4    | 1       |
| Channel               | Digital I/O channel number<br>0 disables the function  |    | CHAN    | 0..16   | 0       |
| Significance factor   | Factor that specifies the relation between the Increment value and the number of output pulses.<br>E.g. a value of 100 means that 1 pulse is generated whenever 100 increment units have been accumulated.   | -  | SIGFCT  | 0..1e99 | 1       |
| Pulse width           | Time that each output pulse remains active (high) in millisecond<br>Restriction (pulse duty cycle is 50%):<br>Pulse width $\leq 1000 / (2 * \text{max. output rate})$  | ms | PLSWID  | 0..1e6  | 20      |
| Max. output rate      | Maximum pulse output rate.<br>When output pulses are generated at a frequency higher than the maximum output rate, the superfluous pulses will be accumulated in the pulse reservoir.<br>Restriction when pulse duty cycle should not exceed 50%:<br>Max. output rate $\leq 1000 / (2 * \text{Pulse width})$ | Hz | MAXFREQ | 0..1e6  | 40      |
| Reservoir alarm limit | Alarm limit for the number of pulses in the reservoir buffer   | -  | RSVLIM  | 0..1e99 | 1e9     |
| Channel 2             | Digital I/O channel number<br>0 disables the function  |    | CHAN    | 0..16   | 0       |
| Delay                 | Delay between dual pulse channel A and B in milliseconds   | ms |         | 0..1e99 | 0       |

### Function outputs

| Function outputs       | Remark  | EU | SW tag | Alarm  | Fallback |
|------------------------|---|----|--------|--------|----------|
| Status                 | 0: Normal<br>1: Input argument out of range or in conflict  | -  | STS    | FLOOR  |          |
| Pulse reservoir        | Number of pulses that are accumulated in the reservoir.   | -  | RSVPLS |        | 0        |
| Reservoir alarm status | With respect to the 'Reservoir alarm limit' the number of pulses in the reservoir is:<br>0: Within limit<br>1: Out of limit | -  | RSVSTS |        | 0        |
|                        |   |    |        | RSVALM |          |

### Calculations

Every calculation cycle a number of pulses is added to the reservoir that is equal to input value 'Increment' divided by input value Significance factor.

## fxSetPulseOutput

Adds pulses to the reservoir, to be output on the next cycle.

Takes the 'significance factor' into account, see fxPulseOutput.

### Description

#### Function inputs

| Function inputs | Remark   | EU | SW tag | Range  | Default |
|-----------------|--|----|--------|--------|---------|
| Name            | Optional tag name, tag description and tag group     |    |        |        |         |
| module          | Not used, set to -1.                                 |    |        | -1..16 | -1      |
| index           | Index of the pulse output<br>0 disables the function |    |        | 0..4   |         |
| Increment       | Number of pulses to be added to the reservoir..      |    |        |        |         |
| Reset command   | 0 is normal, 1 is no hardware state changed          |    |        |        | 0       |

#### Function outputs

| Function outputs | Remark  | EU | SW tag | Alarm | Fallback |
|------------------|---|----|--------|-------|----------|
| Status           | 0: Normal                                     | -  | STS    |       |          |
|                  | 1: Input argument out of range or in conflict |    |        | FLOOR |          |

fxPT100Input

Description

Each flow module provides 2 inputs for **Pt-100** sensors.  
A Pt-100 sensor is a Platinum Resistance Thermometer (**PRT**) element with a resistance of 100 Ω at 0°C. 'Pt' is the symbol for platinum.  
Resistance thermometers as such are also referred to as Resistance Temperature Detectors (**RTD**).  
The resistance changes linearly with temperature. For Pt-100 elements the linearity coefficient is 0.385 Ohm/°C for European elements and 0.392 Ohm/°C for American elements

For each sample the temperature value is obtained from the measured Ohms by means of the standard RTD quadratic equation.  
The input signal is considered to be faulty when the input circuitry has an open or a short circuit or when the measured value is outside its range (as defined in table below).

Function inputs

| Function inputs | Remark  | EU   | Default |
|-----------------|---|------|---------|
| Name            | Optional tag name, tag description and tag group  |      |         |
| Channel number  |   | 1..2 | 1       |
| Input Type      | 1: European, 0.00385 Ω/ Ω /°C<br>As per DIN 43760, BS1905,IEC751<br>Range - 200..+850 °C<br>2: American, 0.00392 Ω/ Ω /°C<br>Range - 100..+457 °C |      | 1       |

Function outputs

| Function outputs | Remark   | EU | SW tag | Alarm                             | Fallback |
|------------------|--|----|--------|-----------------------------------|----------|
| Status           | Status output<br>0: Normal<br>1: Input argument out of range<br>2: Under range failure<br>3: Over range failure<br>4: Open circuit<br>5: Short circuit |    | STS    | FIOOR<br>(*)<br>(*)<br>(*)<br>(*) |          |
| Value            | Temperature in degrees Celsius   | °C | VAL    |                                   | 0        |

(\*) Note that no alarm is generated for this status output value. This is to avoid an unnecessary alarm in case the input is not used

fxRTDInput

Description

Reads the PT100 input as a ‘raw’ Ohm number. Use fxPT100Table to convert to degrees Celsius.

Function inputs

| Function inputs | Remark   | EU   | Default |
|-----------------|--|------|---------|
| Name            | Optional tag name, tag description and tag group |      |         |
| Channel number  |  | 1..2 |         |

Function outputs

| Function outputs | Remark                         | EU  | SW tag | Alarm | Fallback |
|------------------|--------------------------------|-----|--------|-------|----------|
| Status           | Status output                  |     | STS    |       |          |
|                  | 0: Normal                      |     |        |       |          |
|                  | 1: Input argument out of range |     |        | FLOOR |          |
|                  | 2: Under range failure         |     |        | (*)   |          |
|                  | 3: Over range failure          |     |        | (*)   |          |
|                  | 4: Open circuit                |     |        | (*)   |          |
|                  | 5: Short circuit               |     |        | (*)   |          |
| Value            |                                | Ohm |        |       | 0        |

fxPT100Table

Description

This function converts a resistance value (Ohm) into a temperature value (°C) according to the Pt-100 conversion tables. A Pt-100 sensor is a Platinum Resistance Thermometer (PRT) element with a resistance of 100 Ω at 0°C. 'Pt' is the symbol for platinum.

Resistance thermometers as such are also referred to as Resistance Temperature Detectors (RTD).

The resistance changes linearly with temperature. For Pt-100 elements the linearity coefficient is 0.385 Ohm/°C for European elements and 0.392 Ohm/°C for American elements

For each sample the temperature value is obtained from the measured Ohms by means of the standard RTD quadratic equation.

The input signal is considered to be faulty when the input circuitry has an open or a short circuit or when the measured value is outside its range (as defined in table below).

Function inputs

| Function inputs | Remark  | EU  | Default |
|-----------------|---|-----|---------|
| Name            | Optional tag name, tag description and tag group  |     |         |
| Ohm             | Measured temperature in Ohms  | Ohm |         |
| Input Type      | 1: European, 0.00385 Ω/ Ω /°C<br>As per DIN 43760, BS1905,IEC751<br>Range - 200..+850 °C<br>2: American, 0.00392 Ω/ Ω /°C<br>Range - 100..+457 °C |     | 1       |

Function outputs

| Function outputs | Remark | EU | SW tag | Alarm | Fallback |
|------------------|--------|----|--------|-------|----------|
| Value            |        | °C |        |       | 0        |

## fxTimePeriodInput

### Description

This function measures the time period between two pulses with a high resolution (100 nanoseconds) and is typically used for densitometer inputs. The measurement is performed continuously in the background and the function returns the average value since the previous calculation cycle.

The measured time period value can be linked to a subsequent densitometer-specific (Solartron, Sarasota, UGC) function that calculates the density at the densitometer conditions.

Abnormal measurements are filtered out and alarmed for.

### Function inputs

| Function inputs                | Remark   | EU | SW tag | Range    | Default |
|--------------------------------|--|----|--------|----------|---------|
| Name                           | Optional tag name, tag description and tag group   |    |        |          |         |
| Channel                        | Channel number for the signal  | -  | CHAN   | 1..16    | 0       |
| Time period differential limit | Maximum allowable difference in microseconds.<br>When the time period between two consecutive pulses differs more than this limit from the previous time period, the reading is considered to be abnormal.<br>Following an abnormal reading there must be 3 consecutive readings within the limit before the time period value is considered normal again.<br>When no 3 consecutive readings within the limit are available in the last 5 readings then the input signal is considered to be invalid.<br>Resolution of the limit value is 100 nanoseconds. | µs |        |          |         |
| Minimum stable time            | Minimum time for high- and low-times of a pulse to be considered valid.  | µs |        | 0..10000 | 30      |

### Function outputs

| Function outputs | Remark   | EU  | SW tag  | Alarm         | Fallback |
|------------------|--|-----|---------|---------------|----------|
| Status           | 0: Normal<br>1: Input argument out of range<br>Outputs will be set to fallback values<br>2: No valid measurement<br>Outputs will be set to fallback values |     | STS     | INPERR<br>(*) |          |
| Time period      | Average (arithmetic mean) in microseconds of the last calculation cycle  | µs  | TIME    |               | 0        |
| Frequency        | Average (arithmetic mean) of the last calculation cycle  | Hz  | FREQ    |               | 0        |
| Curcount         | Current counter value  |     | CURCNT  |               | 0        |
| Curtime          | Current time value   | sec | CURTIME |               | 0        |
| Oldcount         | Previous counter value   |     | PRVCNT  |               | 0        |
| Oldtime          | Previous time value  | sec | PRVTIME |               | 0        |

(\*) Note that no alarm is generated for this status output value. This is to avoid an unnecessary alarm in case the input is not used

## 5 Reference

### Unit Types

| Type of unit      | Description                                       | Unit                 | Convert to       | Excel constant | Multiply by                  | Conversion |
|-------------------|---|----------------------|------------------|----------------|------------------------------|------------|
| Acceleration      | meters per second squared                         | m/s <sup>2</sup>     |                  | xu_m_s2        |                              |            |
|                   | kilometers per second squared                     | km/s <sup>2</sup>    | m/s <sup>2</sup> | xu_km_s2       | 1.0 E+03                     | Exact      |
|                   | inch per second squared                           | in/s <sup>2</sup>    | m/s <sup>2</sup> | xu_in_s2       | 2.54 E-02                    | Exact      |
|                   | foot per second squared                           | ft/s <sup>2</sup>    | m/s <sup>2</sup> | xu_ft_s2       | 3.048 E-01                   | Exact      |
| Area              | square meter                                      | m <sup>2</sup>       |                  | xu_m2          |                              |            |
|                   | square millimeter                                 | mm <sup>2</sup>      | m <sup>2</sup>   | xu_mm2         | 1.0 E-06                     | Exact      |
|                   | square centimeter                                 | cm <sup>2</sup>      | m <sup>2</sup>   | xu_cm2         | 1.0 E-04                     | Exact      |
|                   | square kilometer                                  | km <sup>2</sup>      | m <sup>2</sup>   | xu_km2         | 1.0 E+06                     | Exact      |
|                   | square inch                                       | in <sup>2</sup>      | m <sup>2</sup>   | xu_in2         | 6.4516 E-04                  | Exact      |
|                   | square foot                                       | ft <sup>2</sup>      | m <sup>2</sup>   | xu_ft2         | 9.290304 E-02                | Exact      |
| Dynamic Viscosity | pascal second                                     | Pa.s                 |                  | xu_Pa.s        |                              |            |
|                   | poise   | poise                | Pa.s             | xu_poise       | 1.0 E-01                     | Exact      |
|                   | centipoise  | cP                   | Pa.s             | xu_cP          | 1.0 E-03                     | Exact      |
|                   | kilogram force second per square meter            | kgf.s/m <sup>2</sup> | Pa.s             | xu_kgf.s_m2    | 9.80665                      | Exact      |
|                   | pound-mass per foot second                        | lbm/ft.s             | Pa.s             | xu_lbm_ft.s    | 0.45359237 / 0.3048          | Exact      |
| Energy            | joules  | J                    |                  | xu_J           |                              |            |
|                   | kilojoules  | kJ                   | J                | xu_kJ          | 1.0 E+03                     | Exact      |
|                   | megajoules  | MJ                   | J                | xu_MJ          | 1.0 E+06                     | Exact      |
|                   | gigajoules  | GJ                   | J                | xu_GJ          | 1.0 E+09                     | Exact      |
|                   | terajoules  | TJ                   | J                | xu_TJ          | 1.0 E+12                     | Exact      |
|                   | watt hour   | W.h                  | J                |                | 3.6 E+03                     | Exact      |
|                   | kilowatt hour                                     | kW.h                 | J                |                | 3.6 E+06                     | Exact      |
|                   | watt second                                       | W.s                  | J                |                | 1                            | Exact      |
|                   | British thermal unit                              | Btu                  | J                |                | 1.05505585262 E+03           | Exact      |
|                   | kilo British thermal unit                         | kBtu                 | J                |                | 1.05505585262 E+06           | Exact      |
|                   | million British thermal unit                      | MMBtu                | J                |                | 1.05505585262 E+09           | Exact      |
|                   | calorie   | cal                  | J                |                | 4.1868                       | Exact      |
|                   | kilocalorie                                       | kcal                 | J                |                | 4.1868 E+03                  | Exact      |
|                   | megacalorie                                       | Mcal                 | J                |                | 4.1868 E+09                  | Exact      |
|                   | decatherm   | dT                   | J                |                | 1.05505585262 E+09           | Exact      |
| Energy per Mass   | joule per kilogram                                | J/kg                 |                  |                |                              |            |
|                   | kilojoule per kilogram                            | kJ/kg                | J/kg             |                | 1.0 E+03                     | Exact      |
|                   | megajoule per kilogram                            | MJ/kg                | J/kg             |                | 1.0 E+06                     | Exact      |
|                   | British thermal unit per pound (avoirdupois)      | Btu/lbm              | J/kg             |                | 2.32601 E+03                 | Exact      |
|                   | kilo British thermal unit per pound (avoirdupois) | kBtu/lbm             | J/kg             |                | 2.32601 E+06                 | Exact      |
|                   | calorie per kilogram                              | cal/kg               | J/kg             |                | 4.1868                       | Exact      |
|                   | kilocalorie per kilogram                          | kcal/kg              | J/kg             |                | 4.1868 E+03                  | Exact      |
|                   | million calorie per kilogram                      | MMcal/kg             | J/kg             |                | 4.1868 E+06                  | Exact      |
| Energy per Mole   | joules per mole                                   | J/mol                |                  |                |                              |            |
|                   | kilojoules per mole                               | kJ/mol               | J/mol            |                | 1.0 E+03                     | Exact      |
|                   | megajoules per mole                               | MJ/mol               | J/mol            |                | 1.0 E+06                     | Exact      |
|                   | kilojoules per kilomole                           | kJ/kmol              | J/mol            |                | 1                            | Exact      |
|                   | megajoules per kilomole                           | MJ/kmol              | J/mol            |                | 1.0 E+03                     | Exact      |
|                   | British thermal unit per pound mole               | Btu/lbmol            | J/mol            |                | 2.326 E+03                   | Exact      |
|                   | kilo British thermal unit per pound mole          | kBtu/lbmol           | J/mol            |                | 2.326 E+06                   | Exact      |
|                   | calorie per mole                                  | cal/mol              | J/mol            |                | 4.1868                       | Exact      |
|                   | kilocalorie per mole                              | kcal/mol             | J/mol            |                | 4.1868 E+03                  | Exact      |
|                   | megacalorie per mole                              | Mcal/mol             | J/mol            |                | 4.1868 E+06                  | Exact      |
| Energy per Time   | joules per second                                 | J/s                  |                  |                |                              |            |
|                   | megajoules per hour                               | MJ/hr                | J/s              |                | (1.0/3600) E+06              | Exact      |
|                   | gigajoules per hour                               | GJ/hr                | J/s              |                | (1.0/3600) E+09              | Exact      |
|                   | megajoules per day                                | MJ/day               | J/s              |                | (1.0/86400) E+06             | Exact      |
|                   | gigajoules per day                                | GJ/day               | J/s              |                | (1.0/86400) E+09             | Exact      |
|                   | kilo British thermal unit per hour                | kBtu/hr              | J/s              |                | (1.05505585262 / 3600) E+06  | Exact      |
|                   | million British thermal unit per hour             | MMBtu/hr             | J/s              |                | (1.05505585262 / 3600) E+09  | Exact      |
|                   | kilo British thermal unit per day                 | kBtu/d               | J/s              |                | (1.05505585262 / 86400) E+06 | Exact      |
|                   | million British thermal unit per day              | MMBtu/d              | J/s              |                | (1.05505585262 / 86400) E+09 | Exact      |
|                   | mega calorie per hour                             | Mcal/hr              | J/mol            |                | (4.1868/3600) E+06           | Exact      |
|                   | giga calorie per hour                             | Gcal/hr              | J/mol            |                | (4.1868/3600) E+09           | Exact      |



| Type of unit               | Description  | Unit         | Convert to | Excel constant | Multiply by                       | Conversion |
|----------------------------|--|--------------|------------|----------------|-----------------------------------|------------|
| Energy per Volume          | million calorie per day  | Mcal/d       | J/mol      |                | (4.1868/86400) E+06               | Exact      |
|                            | giga calorie per day   | Gcal/d       | J/mol      |                | (4.1868/86400) E+09               | Exact      |
|                            | joules per cubic meter   | J/m3         |            |                |                                   |            |
|                            | kilojoules per cubic meter   | kJ/m3        | J/m3       |                | 1.0 E+03                          | Exact      |
|                            | megajoules per cubic meter   | MJ/m3        | J/m3       |                | 1.0 E+06                          | Exact      |
|                            | British thermal unit per cubic foot                                | Btu/ft3      | J/m3       |                | (1.05505585262 / 0.02831685) E+03 | Exact      |
|                            | kilo British thermal unit per cubic foot                           | kBtu/ft3     | J/m3       |                | (1.05505585262 / 0.02831685) E+06 | Exact      |
|                            | calorie per cubic meter  | cal/m3       | J/mol      |                | 4.1868                            | Exact      |
|                            | kilocalorie per cubic meter  | kcal/m3      | J/mol      |                | 4.1868 E+03                       | Exact      |
|                            | joules per standard cubic meter                                    | J/sm3        |            |                |                                   |            |
| Energy per Standard Volume | kilojoules per standard cubic meter                                | kJ/sm3       | J/sm3      |                | 1.0 E+03                          | Exact      |
|                            | megajoules per standard cubic meter                                | MJ/sm3       | J/sm3      |                | 1.0 E+06                          | Exact      |
|                            | British thermal unit per standard cubic foot                       | Btu/scf      | J/sm3      |                | (1.05505585262 / 0.02831685) E+03 | Exact      |
|                            | kilo British thermal unit per standard cubic foot                  | kBtu/scf     | J/sm3      |                | (1.05505585262 / 0.02831685) E+06 | Exact      |
|                            | calorie per standard cubic meter                                   | cal/sm3      | J/sm3      |                | 4.1868                            | Exact      |
|                            | kilocalorie per standard cubic meter                               | kcal/sm3     | J/sm3      |                | 4.1868 E+03                       | Exact      |
|                            | joules per standard cubic meter                                    | J/m3(n)      |            |                |                                   |            |
| Energy per Normal Volume   | kilojoules per standard cubic meter                                | kJ/m3(n)     | J/m3(n)    | xu_J/m3n       | 1.0 E+03                          | Exact      |
|                            | megajoules per standard cubic meter                                | MJ/m3(n)     | J/m3(n)    |                | 1.0 E+06                          | Exact      |
|                            | calorie per standard cubic meter                                   | cal/m3(n)    | J/m3(n)    |                | 4.1868                            | Exact      |
|                            | kilocalorie per standard cubic meter                               | kcal/m3(n)   | J/m3(n)    |                | 4.1868 E+03                       | Exact      |
| Factor                     | scaling value  | Decimal      |            |                |                                   |            |
|                            | percent  | %            | Decimal    |                | 1.0 E-02                          | Exact      |
|                            | parts per million  | ppm          | Decimal    |                | 1.0 E-06                          | Exact      |
| Force                      | Newton   | N            |            |                |                                   |            |
|                            | kilogram-force   | kgf          | N          |                | 9.80665                           | Exact      |
|                            | pound-force  | lbf          | N          |                | 4.4482216152605                   | Exact      |
| Frequency                  | Hertz  | Hz           |            |                |                                   |            |
| Heat Capacity per Mass     | Joule per kilogram per degree Celsius                              | J/kg.°C      |            | xu_J_kg.degC   |                                   |            |
|                            | Joule per kilogram per degree Celsius                              | kJ/kg.°C     | J/kg.°C    |                | 1.0 E+03                          | Exact      |
|                            | British thermal unit per pound (avoirdupois) per degree Fahrenheit | Btu/lbm.°F   | J/kg. °C   |                | 4186.8                            | Exact      |
| Heat Capacity per Mole     | Joule per mole per degree Celsius                                  | J/mol.°C     |            |                |                                   |            |
|                            | kilo Joule per kilo mole per degree Celsius                        | kJ/kmol.°C   | J/mol.°C   |                | 1                                 | Exact      |
|                            | British thermal unit per mole per degree Fahrenheit                | Btu/lbmol.°F | J/mol.°C   |                | 2.326E+03 / 1.8                   | Exact      |
| Kinematic Viscosity        | square meter per second  | m2/s         |            |                |                                   |            |
|                            | square millimeter per second                                       | mm2/s        | m2/s       |                | 1.0 E-06                          | Exact      |
|                            | centistokes  | cSt          | m2/s       |                | 1.0 E-06                          | Exact      |
|                            | stokes   | St           | m2/s       |                | 1.0 E-04                          | Exact      |
| Length                     | meter  | m            |            |                |                                   |            |
|                            | centimeter   | cm           | m          |                | 1.0 E-02                          | Exact      |
|                            | millimeter   | mm           | m          |                | 1.0 E-03                          | Exact      |
|                            | kilometer  | km           | m          |                | 1.0 E+03                          | Exact      |
|                            | micron   | μ            | m          |                | 1.0 E-06                          | Exact      |
|                            | foot   | ft           | m          |                | 3.048 E-01                        | Exact      |
|                            | inch   | in           | m          |                | 2.54 E-02                         | Exact      |
| Length per Temperature     | meter per degree Celsius   | m/°C         |            |                |                                   |            |
|                            | meter per degree Fahrenheit  | m/°F         | m/°C       |                | 1.8                               | Exact      |
|                            | centimeter per degree Celsius                                      | cm/°C        | m/°C       |                | 1.0 E-02                          | Exact      |
|                            | centimeter per degree Fahrenheit                                   | cm/°F        | m/°C       |                | 1.8 E-02                          | Exact      |
|                            | millimeter per degree Celsius                                      | mm/°C        | m/°C       |                | 1.0 E-03                          | Exact      |
|                            | millimeter per degree Fahrenheit                                   | mm/°F        | m/°C       |                | 1.8 E-03                          | Exact      |
|                            |  |              |            |                |                                   |            |

| Type of unit             | Description  | Unit         | Convert to | Excel constant | Multiply by                                 | Conversion           |
|--------------------------|--|--------------|------------|----------------|---|----------------------|
|                          | feet per degree Celsius  | ft/°C        | m/°C       |                | 3.048 E-01                                  | Exact                |
|                          | feet per degree Fahrenheit   | ft/°F        | m/°C       |                | 5.4864 E-01                                 | Exact                |
|                          | inches per degree Celsius  | in/°C        | m/°C       |                | 2.54 E-02                                   | Exact                |
|                          | inches per degree Fahrenheit   | in/°F        | m/°C       |                | 4.572 E-02                                  | Exact                |
| Mass                     | kilogram   | kg           |            |                |   |                      |
|                          | gram   | g            | kg         |                | 1.0 E-03                                    | Exact                |
|                          | milligram  | mg           | kg         |                | 1.0 E-06                                    | Exact                |
|                          | pound mass (avoirdupois)   | lbm          | kg         |                | 4.5359237 E-01                              | Exact                |
|                          | kilopound mass (avoirdupois)   | klbm         | kg         |                | 4.5359237 E+02                              | Exact                |
|                          | Million pound mass (avoirdupois)   | Mlbm         | kg         |                | 4.5359237 E+05                              | Exact                |
|                          | metric ton   | tonne        | kg         |                | 1.0 E+03                                    | Exact                |
|                          | short ton (equals 2000 lb, also called tonUS)  | short ton    | kg         |                | 9.0718474 E+02                              | Exact                |
|                          | long ton (equals 2240 lb, also called tonUK)   | long ton     | kg         |                | 1.016046909 E+03                            | Exact                |
| Mass per Mass            | mass fraction  | mass/mass    |            |                |   |                      |
|                          | mass percentage  | %mass        | mass/mass  |                | 1.0 E-02                                    | Exact                |
| Mass per Mole            | kilograms per mole   | kg/mol       |            |                |   |                      |
|                          | kilograms per kilomole   | kg/kmol      | kg/mol     |                | 1.0 E-03                                    | Exact                |
|                          | grams per mole   | g/mol        | kg/mol     |                | 1.0 E-03                                    | Exact                |
|                          | pound per pound mole   | lbm/lbmol    | kg/mol     |                | 1.0 E-03                                    | Exact                |
|                          | kilopound per kilopound mole   | klbm/klbmol  | kg/mol     |                | 1.0 E-03                                    | Exact                |
| Mass per Pulse           | kilograms per pulse  | kg/pulse     |            |                |   |                      |
|                          | grams per pulse  | g/pulse      | kg/pulse   |                | 1.0 E-03                                    | Exact                |
|                          | pounds mass per pulse  | lbm/pulse    | kg/pulse   |                | 4.535924 E-01                               | Exact                |
| Mass per Time            | kilogram per second  | kg/s         |            |                |   |                      |
|                          | kilogram per hour  | kg/hr        | kg/s       |                | (1.0/3600)                                  | Exact                |
|                          | ton (metric) per hour  | tonne/hr     | kg/s       |                | (1.0/3600) E+03                             | Exact                |
|                          | ton (short) per hour   | short ton/hr | kg/s       |                | (9.071847/3600) E+02                        | Exact                |
|                          | ton (long) per hour  | long ton/hr  | kg/s       |                | (1.016046909/3600) E+03                     | Exact                |
|                          | pound mass (avoirdupois) per second  | lbm/s        | kg/s       |                | 4.535924 E-01                               | Exact                |
|                          | pound mass (avoirdupois) per hour  | lbm/hr       | kg/s       |                | (4.535924/3600) E-01                        | Exact                |
|                          | kilopound mass (avoirdupois) per hour  | klbm/hr      | kg/s       |                | (4.535924/3600) E+02                        | Exact                |
|                          | kilogram per day   | kg/d         | kg/s       |                | (1.0/86400)                                 | Exact                |
|                          | ton (metric) per day   | tonne/d      | kg/s       |                | (1.0/86400) E+03                            | Exact                |
|                          | ton (short) per day  | short ton/d  | kg/s       |                | (9.071847/86400) E+02                       | Exact                |
|                          | ton (long) per day   | long ton/d   | kg/s       |                | (1.016046909/86400) E+03                    | Exact                |
|                          | pound mass (avoirdupois) per day   | lbm/d        | kg/s       |                | (4.535924/86400) E-01                       | Exact                |
|                          | kilopound mass (avoirdupois) per day   | klbm/d       | kg/s       |                | (4.535924/86400) E+02                       | Exact                |
| Mass per Volume          | kilogram per cubic meter   | kg/m3        |            |                |   |                      |
|                          | gram per cubic centimeter  | g/cm3        | kg/m3      |                | 1.0 E03                                     | Exact                |
|                          | pound per cubic foot   | lbm/ft3      | kg/m3      |                | 1.601846337 E+01                            | Exact                |
|                          | API gravity <sup>(1)</sup>   | ° API        | kg/m3      |                | $\rho_{H2O,60°F} * 141.5 / (° API + 131.5)$ | Exact <sup>(3)</sup> |
|                          | Specific Gravity at 60 degrees Fahrenheit <sup>(1)</sup>   | SG @ 60°F    | kg/m3      |                | $\rho_{H2O,60°F}$ <sup>(2)</sup>            | Exact <sup>(3)</sup> |
|                          | Relative Density at 60 degrees Fahrenheit <sup>(1)</sup>   | RD @ 60°F    | kg/m3      |                | $\rho_{H2O,60°F}$ <sup>(2)</sup>            | Exact <sup>(3)</sup> |
|                          | <sup>(1)</sup> This conversion only applies when conversion is to /from the 'Mass per Volume' value at 60 °F<br><sup>(2)</sup> $\rho_{H2O,60°F}$ the density of water at 60 °F is a global setting with a default value of 999.012 kg/m3<br><sup>(3)</sup> The conversion is exact, however the resulting value is an approximation because of $\rho_{H2O,60°F}$ |              |            |                |   |                      |
| Mass per Standard Volume | kilogram per standard cubic meter  | kg/sm3       |            |                |   |                      |
|                          | gram per standard cubic centimeter   | g/scm3       | kg/sm3     |                | 1.0 E03                                     | Exact                |
|                          | pound per standard cubic foot  | lbm/scf      | kg/sm3     |                | 1.601846337 E+01                            | Exact                |
| Mass per Normal Volume   | kilogram per normal cubic meter  | kg/m3(n)     |            |                |   |                      |
|                          | gram per normal cubic  | g/cm3(n)     | kg/m3(n)   |                | 1.0 E-03                                    | Exact                |

| Type of unit            | Description  | Unit                        | Convert to         | Excel constant | Multiply by        | Conversion  |
|-------------------------|--|-----------------------------|--------------------|----------------|--------------------|-------------|
|                         | centimeter   |                             |                    |                |                    |             |
| Mole                    | mole   | mol                         |                    |                |                    |             |
|                         | A mole resembles $6.0251 \times 10^{23}$ molecules of a substance, a standard number of molecules known as Avogadro's number.  |                             |                    |                |                    |             |
|                         | kilomole   | kmol                        | mol                |                | 1.0 E+03           | Exact       |
|                         | pound mole   | lbmol                       | mol                |                | 4.5359237 E-01     | Exact       |
|                         | In English units, the pound-mass (lbm) is the standard unit of mass. In order to use the same molecular weights as those listed on the periodic chart, the pound-mol, (lbmol, sometimes lb-mol, lbm-mol, or lbm-mole) is defined |                             |                    |                |                    |             |
|                         | kilopound mole   | klbmol                      | mol                |                | 4.5359237 E+02     | Exact       |
| Mole per Mole           | mole fraction  | mole/mole                   |                    |                |                    |             |
|                         | mole percentage  | %mole                       | mole/mole          |                | 1.0 E-02           | Exact       |
| Mole per Volume         | mole per cubic meter   | mol/m <sup>3</sup>          |                    |                |                    |             |
|                         | mole per cubic centimeter  | mol/cm <sup>3</sup>         | mol/m <sup>3</sup> |                | 1.0 E+6            | Exact       |
|                         | mole per litre   | mol/l                       | mol/m <sup>3</sup> |                | 1.0 E+3            | Exact       |
|                         | kilomole per cubic meter   | kmol/m <sup>3</sup>         | mol/m <sup>3</sup> |                | 1.0 E+3            | Exact       |
|                         | kilomole per cubic centimeter  | kmol/cm <sup>3</sup>        | mol/m <sup>3</sup> |                | 1.0 E+9            | Exact       |
|                         | kilomole per litre   | kmol/l                      | mol/m <sup>3</sup> |                | 1.0 E+6            | Exact       |
|                         | kilomole per cubic feet  | kmol/ft <sup>3</sup>        | mol/m <sup>3</sup> |                | 1 / 28.31685 E -03 | Exact       |
| Power                   | watt   | W                           |                    |                |                    |             |
|                         | kilowatt   | kW                          | W                  |                | 1.0 E+03           | Exact       |
|                         | megawatt   | MW                          | W                  |                | 1.0 E+06           | Exact       |
|                         | gigawatt   | GW                          | W                  |                | 1.0 E+09           | Exact       |
| Pressure (differential) | pascal   | Pa                          |                    |                |                    |             |
|                         | kilo pascal  | kPa                         | Pa                 |                | 1.0 E+03           | Exact       |
|                         | kilogram-force per square meter  | kgf/m <sup>2</sup>          | Pa                 |                | 9.80665            | Exact       |
|                         | kilogram-force per square centimeter   | kgf/cm <sup>2</sup>         | Pa                 |                | 9.80665 E+04       | Exact       |
|                         | pound-force per square foot  | lbf/ft <sup>2</sup>         | Pa                 |                | 47.8803            | Exact       |
|                         | pound-force per square inch (psi)  | lbf/in <sup>2</sup>         | Pa                 |                | 6894.76            | Exact       |
|                         | pound-force per square inch (psi)  | psi                         | Pa                 |                | 6894.76            | Exact       |
|                         | bar  | bar                         | Pa                 |                | 1.0 E+05           | Exact       |
|                         | millibar   | mbar                        | Pa                 |                | 1.0 E+02           | Exact       |
|                         | millimeter of mercury, conventional  | mmHg                        | Pa                 |                | 133.322387415      | Exact       |
|                         | millimeter of water, conventional  | mmH <sub>2</sub> O          | Pa                 |                | 9.80665            | Exact       |
|                         | millimeter of water @ 60°F   | mmH <sub>2</sub> O @ 60°F   | Pa                 |                | 248.84/25.4        | Approximate |
|                         | inch of mercury, conventional  | inHg con                    | Pa                 |                | 3386.38864         | Exact       |
|                         | inch of mercury @ 32°F (0°C)   | inHg @ 32°F                 | Pa                 |                | 3386.38            | Approximate |
|                         | inch of mercury @ 60°F   | inHg @ 60°F                 | Pa                 |                | 3376.85            | Approximate |
|                         | inch of water, conventional  | inH <sub>2</sub> O con      | Pa                 |                | 249.08891          | Exact       |
|                         | inch of water @ 39.2°F (4°C)   | inH <sub>2</sub> O @ 39.2°F | Pa                 |                | 249.082            | Approximate |
|                         | inch of water @ 60°F   | inH <sub>2</sub> O @ 60°F   | Pa                 |                | 248.84             | Approximate |
|                         | inch of water @ 68°F   | inH <sub>2</sub> O @ 68°F   | Pa                 |                | 248.64108          | Approximate |
| Pressure (absolute)     | pascal absolute  | Pa(a)                       |                    |                |                    |             |
|                         | kilo pascal absolute   | kPa(a)                      | Pa(a)              |                | 1.0 E+03           | Exact       |
|                         | pound-force per square inch (psi) absolute   | psia                        | Pa(a)              |                | 6894.76            | Exact       |
|                         | bar absolute   | bar(a)                      | Pa(a)              |                | 1.0 E+05           | Exact       |
|                         | millibar absolute  | mbar(a)                     | Pa(a)              |                | 1.0 E+02           | Exact       |
|                         | millimeter of mercury, conventional absolute   | mmHga                       | Pa(a)              |                | 133.322387415      | Exact       |
|                         | millimeter of water, conventional absolute   | mmH <sub>2</sub> Oa         | Pa(a)              |                | 9.80665            | Exact       |
|                         | millimeter of water @ 60°F absolute  | mmH <sub>2</sub> Oa @ 60°F  | Pa(a)              |                | 248.84/25.4        | Approximate |
|                         | inch of mercury, conventional absolute   | inHga con                   | Pa(a)              |                | 3386.38864         | Exact       |
|                         | inch of mercury @ 32°F (0°C) absolute  | inHga @ 32°F                | Pa(a)              |                | 3386.38            | Approximate |
|                         | inch of mercury @ 60°F absolute  | inHga @ 60°F                | Pa(a)              |                | 3376.85            | Approximate |
|                         | inch of water, conventional absolute   | inH <sub>2</sub> Oa con     | Pa(a)              |                | 249.08891          | Exact       |

| Type of unit             | Description  | Unit            | Convert to | Excel constant | Multiply by                 | Conversion  |
|--------------------------|--|-----------------|------------|----------------|-----------------------------|-------------|
| Pressure (gauge)         | inch of water @ 39.2°F (4°C) absolute                  | inH2Oa @ 39.2°F | Pa(a)      |                | 249.082                     | Approximate |
|                          | inch of water @ 60°F absolute                          | inH2Oa @ 60°F   | Pa(a)      |                | 248.84                      | Approximate |
|                          | inch of water @ 68°F absolute                          | inH2Oa @ 68°F   | Pa(a)      |                | 248.64107                   | Approximate |
|                          | pascal gauge   | Pa(g)           |            |                |                             |             |
|                          | kilo pascal gauge                                      | kPa(g)          | Pa(g)      |                | 1.0 E+03                    | Exact       |
|                          | pound-force per square inch (psi) gauge                | psig            | Pa(g)      |                | 6894.76                     | Exact       |
|                          | bar gauge  | bar(g)          | Pa(g)      |                | 1.0 E+05                    | Exact       |
|                          | millibar gauge   | mbar(g)         | Pa(g)      |                | 1.0 E+02                    | Exact       |
|                          | millimeter of mercury, conventional gauge              | mmHg            | Pa(g)      |                | 133.322387415               | Exact       |
|                          | millimeter of water, conventional gauge                | mmH2Og          | Pa(g)      |                | 9.80665                     | Exact       |
|                          | millimeter of water @ 60°F gauge                       | mmH2Og @ 60°F   | Pa(g)      |                | 248.84/25.4                 | Approximate |
|                          | inch of mercury, conventional gauge                    | inHg con        | Pa(g)      |                | 3386.38864                  | Exact       |
|                          | inch of mercury @ 32°F (0°C) gauge                     | inHg @ 32°F     | Pa(g)      |                | 3386.38                     | Approximate |
|                          | inch of mercury @ 60°F gauge                           | inHg @ 60°F     | Pa(g)      |                | 3376.85                     | Approximate |
|                          | inch of water, conventional gauge                      | inH2Og con      | Pa(g)      |                | 249.08891                   | Exact       |
|                          | inch of water @ 39.2°F (4°C) gauge                     | inH2Og @ 39.2°F | Pa(g)      |                | 249.082                     | Approximate |
|                          | inch of water @ 60°F gauge                             | inH2Og @ 60°F   | Pa(g)      |                | 248.84                      | Approximate |
| Pressure inverse         | per pascal   | 1/Pa            |            |                |                             |             |
|                          | per kilo pascal  | 1/kPa           | 1/Pa       |                | 1.0 E-03                    | Exact       |
|                          | per Mega pascal  | 1/MPa           | 1/Pa       |                | 1.0 E-06                    |             |
|                          | per pound-force per square inch (psi)                  | 1/psi           | 1/Pa       |                | 1/6894.76                   | Exact       |
|                          | per bar  | 1/bar           | 1/Pa       |                | 1.0 E-05                    | Exact       |
| Pressure per Mass        | pascals per kilogram                                   | Pa/kg           |            |                |                             |             |
|                          | kilopascals per kilogram                               | kPa/kg          | Pa/kg      |                | 1.0 E+03                    | Exact       |
|                          | megapascals per kilogram                               | MPa/kg          | Pa/kg      |                | 1.0 E+06                    | Exact       |
|                          | pounds mass (avoirdupois) per square inch per kilogram | psi/kg          | Pa/kg      |                | 6894.76                     | Exact       |
|                          | bar per per kilogram                                   | bar/kg          | Pa/kg      |                | 1.0 E+05                    | Exact       |
| Pulses per Mass          | pulses per kilogram                                    | pulses/kg       |            |                |                             |             |
|                          | pulses per gram  | pulses/g        | pulses/kg  |                | 1.0 E+03                    | Exact       |
|                          | pulses per pound mass (avoirdupois)                    | pulses/lbm      | pulses/kg  |                | 1/0.4535924                 | Exact       |
| Pulses per Volume        | pulses per cubic meter                                 | pulses/m3       |            |                |                             |             |
|                          | pulses per cubic centimeter                            | pulses/cm3      | pulses/m3  |                | 1.0 E-06                    | Exact       |
|                          | pulses per litre                                       | pulses/lb       | pulses/m3  |                | 1.0 E-03                    | Exact       |
|                          | pulses per cubic inch                                  | pulses/in       | pulses/m3  |                | 1/0.0000163871              | Exact       |
|                          | pulses per cubic feet                                  | pulses/ft3      | pulses/m3  |                | 1/0.0283168                 | Exact       |
| Temperature              | Kelvin   | K               |            |                |                             |             |
|                          | degree Celsius   | °C              | K          |                | T[K] = t[°C] + 273.15       | Exact       |
|                          | degree Fahrenheit                                      | °F              | K          |                | T[K] = (t[°F] + 459.67)/1.8 | Exact       |
|                          | Rankine  | R               | K          |                | T[K] = T[R]/1.8             | Exact       |
| Temperature inverse      | per Kelvin   | 1/K             |            |                |                             |             |
|                          | per degree Celsius                                     | 1/°C            | 1/K        |                | 1.0                         | Exact       |
|                          | per degree Fahrenheit                                  | 1/°F            | 1/K        |                | 1.8                         | Exact       |
|                          | per Rankine  | 1/R             | 1/K        |                | 1.8                         | Exact       |
| Temperature per Pressure | degree Celsius per bar (Joule-Thomson coefficient)     | °C/bar          |            |                |                             |             |
|                          |  | °F/psi          | °C/bar     |                | 1.8/6894.76                 | Exact       |
| Time                     | second   | s               |            |                |                             |             |
|                          | milli second   | ms              | s          |                | 1.0 E-03                    | Exact       |
|                          | micro second   | µs              | s          |                | 1.0 E-06                    | Exact       |
|                          | nano second  | ns              | s          |                | 1.0 E-09                    | Exact       |
|                          | minute   | min             | s          |                | 6.0 E+01                    | Exact       |
|                          | hour   | H               | s          |                | 3.6 E+03                    | Exact       |
|                          | day  | D               | s          |                | 8.64 E+04                   | Exact       |
| Velocity                 | meters per second                                      | m/s             |            |                |                             |             |
|                          | kilometers per second                                  | km/s            | m/s        |                | 1.0 E+03                    | Exact       |
|                          | kilometers per hour                                    | km/hr           | m/s        |                | (1/3600) E+03               | Exact       |
|                          | foot per second  | ft/s            | m/s        |                | 3.048 E-01                  | Exact       |
| Volume                   | cubic meter  | m3              |            |                |                             |             |
|                          | cubic centimeter                                       | cm3             | m3         |                | 1.0 E-06                    | Exact       |
|                          | kilo cubic meter                                       | km3             | m3         |                | 1.0 E+03                    | Exact       |

| Type of unit             | Description                                 | Unit      | Convert to | Excel constant | Multiply by       | Conversion |
|--------------------------|---|-----------|------------|----------------|-------------------|------------|
|                          | mega cubic meter                            | Mm3       | m3         |                | 1.0 E+06          | Exact      |
|                          | liter                                       | L         | m3         |                | 1.0 E-03          | Exact      |
|                          | cubic inch                                  | in3       | m3         |                | 16.38706 E+06     | Exact      |
|                          | cubic foot                                  | ft3       | m3         |                | 28.31685 E -03    | Exact      |
|                          | kilo cubic foot                             | kft3      | m3         |                | 28.31685          | Exact      |
|                          | million cubic foot                          | MMft3     | m3         |                | 28.31685 E +03    | Exact      |
|                          | barrel (42 US liquid gallons exactly)       | bbl       | m3         |                | 0.158987295       | Exact      |
|                          | US liquid gallon (231 cubic inches exactly) | US.gal    | m3         |                | 3.785411784 E-03  | Exact      |
|                          | Imperial (U.K.) gallon                      | UK.gal    | m3         |                | 4.54609 E-03      | Exact      |
| Standard Volume          | standard cubic meter                        | sm3       |            |                |                   |            |
|                          | kilo standard cubic meter                   | ksm3      | sm3        |                | 1.0 E+03          | Exact      |
|                          | mega standard cubic meter                   | Msm3      | sm3        |                | 1.0 E+06          | Exact      |
|                          | standard cubic foot                         | scf       | sm3        |                | 28.31685 E -03    | Exact      |
|                          | kilo standard cubic foot                    | kscf      | sm3        |                | 28.31685          | Exact      |
|                          | million standard cubic foot                 | MMscf     | sm3        |                | 28.31685 E +03    | Exact      |
|                          | barrel (standard)                           | bbl (s)   | sm3        |                | 0.158987295       | Exact      |
| Normal Volume            | normal cubic meter                          | m3(n)     |            |                |                   |            |
|                          | kilo normal cubic meter                     | km3(n)    | m3(n)      |                | 1.0 E+03          | Exact      |
|                          | mega normal cubic meter                     | Mm3(n)    | m3(n)      |                | 1.0 E+06          | Exact      |
| Volume per Volume        | volume fraction                             | vol/vol   |            |                |                   |            |
|                          | volume percentage                           | %vol      | vol/vol    |                | 1.0 E-02          | Exact      |
| Volume per Pulse         | cubic meters per pulse                      | m3/pulse  |            |                |                   |            |
|                          | cubic centimeters per pulse                 | cm3/pulse | m3/pulse   |                | 1.0 E-06          | Exact      |
|                          | litres per pulse                            | l/pulse   | m3/pulse   |                | 1.0 E-03          | Exact      |
|                          | cubic inches per pulse                      | in3/pulse | m3/pulse   |                | 1.63871E-05       | Exact      |
|                          | cubic feet per pulse                        | ft3/pulse | m3/pulse   |                | 0.0283168         | Exact      |
| Volume per Time          | cubic meter per second                      | m3/s      |            |                |                   |            |
|                          | cubic meter per hour                        | m3/hr     | m3/s       |                | 1/3600            | Exact      |
|                          | cubic meter per day                         | m3/d      | m3/s       |                | 1/86400           | Exact      |
|                          | kilo cubic meter per second                 | km3/s     | m3/s       |                | 1.0 E+03          | Exact      |
|                          | kilo cubic meter per hour                   | km3/hr    | m3/s       |                | (1/3600) E+03     | Exact      |
|                          | kilo cubic meter per day                    | km3/d     | m3/s       |                | (1/86400) E+03    | Exact      |
|                          | mega cubic meter per hour                   | Mm3/hr    | m3/s       |                | (1/3600) E+06     | Exact      |
|                          | mega cubic meter per day                    | Mm3/d     | m3/s       |                | (1/86400) E+06    | Exact      |
|                          | cubic feet per hour                         | ft3/hr    | m3/s       |                | 0.02831685/3600   | Exact      |
|                          | cubic feet per day                          | ft3/d     | m3/s       |                | 0.02831685/86400  | Exact      |
|                          | kilo cubic feet per hour                    | kft3/hr   | m3/s       |                | 28.31685/3600     | Exact      |
|                          | kilo cubic feet per day                     | kft3/d    | m3/s       |                | 28.31685/86400    | Exact      |
|                          | million cubic feet per hour                 | Mft3/hr   | m3/s       |                | 28316.85/3600     | Exact      |
|                          | million cubic feet per day                  | Mft3/d    | m3/s       |                | 28316.85/86400    | Exact      |
|                          | barrels per hour                            | bbl/hr    | m3/s       |                | 0.158987295/3600  | Exact      |
|                          | barrels per day                             | bbl/d     | m3/s       |                | 0.158987295/86400 | Exact      |
| Standard Volume per Time | standard cubic meter per second             | sm3/s     |            |                |                   |            |
|                          | standard cubic meter per hour               | sm3/hr    | sm3/s      |                | 1/3600            | Exact      |
|                          | standard cubic meter per day                | sm3/d     | sm3/s      |                | 1/86400           | Exact      |
|                          | kilo standard cubic meter per second        | ksm3/s    | sm3/s      |                | 1.0 E+03          | Exact      |
|                          | kilo standard cubic meter per hour          | ksm3/hr   | sm3/s      |                | (1/3600) E+03     | Exact      |
|                          | kilo standard cubic meter per day           | ksm3/d    | sm3/s      |                | (1/86400) E+03    | Exact      |
|                          | mega standard cubic meter per hour          | Msm3/hr   | sm3/s      |                | (1/3600) E+06     | Exact      |
|                          | mega standard cubic meter per day           | Msm3/d    | sm3/s      |                | (1/86400) E+06    | Exact      |
|                          | standard cubic feet per hour                | scf/hr    | sm3/s      |                | 0.02831685/3600   | Exact      |
|                          | standard cubic feet per day                 | scf/d     | sm3/s      |                | 0.02831685/86400  | Exact      |
|                          | kilo standard cubic feet per hour           | kscf/hr   | sm3/s      |                | 28.31685/3600     | Exact      |
|                          | kilo standard cubic feet per day            | kscf/d    | sm3/s      |                | 28.31685/86400    | Exact      |
|                          | million standard cubic feet per hour        | MMscf/hr  | sm3/s      |                | 28316.85/3600     | Exact      |
|                          | million standard cubic feet per day         | MMscf/d   | sm3/s      |                | 28316.85/86400    | Exact      |
|                          | barrels per hour (standard)                 | bbl/hr    | sm3/s      |                | 0.158987295/3600  | Exact      |
|                          | barrels per day (standard)                  | bbl/d     | sm3/s      |                | 0.158987295/86400 | Exact      |
| Normal Volume per Time   | normal cubic meter per second               | m3(n)/s   |            |                |                   |            |
|                          | normal cubic meter per hour                 | m3(n)/hr  | m3(n)/s    |                | 1/3600            | Exact      |
|                          | normal cubic meter per day                  | m3(n)/d   | m3(n)/s    |                | 1/86400           | Exact      |

| Type of unit | Description                        | Unit      | Convert to | Excel constant | Multiply by    | Conversion |
|--------------|------------------------------------|-----------|------------|----------------|----------------|------------|
|              | kilo normal cubic meter per second | km3(n)/s  | m3(n)/s    |                | 1.0 E+03       | Exact      |
|              | kilo normal cubic meter per hour   | km3(n)/hr | m3(n)/s    |                | (1/3600) E+03  | Exact      |
|              | kilo normal cubic meter per day    | km3(n)/d  | m3(n)/s    |                | (1/86400) E+03 | Exact      |
|              | mega normal cubic meter per hour   | Mm3(n)/hr | m3(n)/s    |                | (1/3600) E+06  | Exact      |
|              | mega normal cubic meter per day    | Mm3(n)/d  | m3(n)/s    |                | (1/86400) E+06 | Exact      |

Terminology

| Term                     | Description   | Same as  |
|--------------------------|---|--|
| Heating Value            | Usually the same as Gross Heating Value   |  |
| Calorific Value          | Usually the same as Superior Calorific Value  |  |
| Superior Calorific Value | Heating value when assuming that water formed at the combustion stays in the gaseous state.<br>From ISO6976.                        | Gross Heating Value  |
| Inferior Calorific Value | Heating value when assuming that water formed at the combustion has totally condensed to the liquid state.<br>From ISO6976.         | Net Heating Value  |
| Gross Heating Value      | Heating value when assuming that water formed at the combustion stays in the gaseous state<br>Term used in GPA2172.                 | Superior Calorific Value   |
| Net Heating Value        | Heating value when assuming that water formed at the combustion has totally condensed to the liquid state.<br>Term used in GPA2172. | Inferior Calorific Value   |
| Molar Mass Ratio         | Ratio of molar mass of gas and molar mass of air at the base conditions   | Specific Gravity<br>Ideal Specific Gravity<br>Ideal Relative Density |
| Relative Density         | Ratio of real mass density of gas and real mass density of air at the base conditions   | Real Relative Density<br>Real Specific Gravity                       |
| Specific Gravity         | Ratio of real mass density of gas and real density of air at the base conditions  | Molar Mass Ratio<br>Ideal Specific Gravity<br>Ideal Relative Density |

## Standard composition

The Standard Composition is a standard array of mole fractional values that is used by all functions that require a (partial) compositional analysis.

The following table defines the sequence of the components and also defines which function uses which component.

| Component         | Used in<br>AGA8 / AGA10 | Used in<br>ISO6976 | Used in<br>GPA2172 | Used in<br>AGA5 | Used in GERG<br>2008 | Used in MR113 |
|-------------------|-------------------------|--------------------|--------------------|-----------------|----------------------|---------------|
| Methane           | √                       | √                  | √                  |                 | √                    | √             |
| Nitrogen          | √                       | √                  | √                  | √               | √                    | √             |
| Carbon Dioxide    | √                       | √                  | √                  | √               | √                    | √             |
| Ethane            | √                       | √                  | √                  |                 | √                    | √             |
| Propane           | √                       | √                  | √                  |                 | √                    | √             |
| Water             | √                       | √                  | 2)                 | √               | √                    | 3)            |
| Hydrogen Sulphide | √                       | √                  | √                  | √               | √                    | √             |
| Hydrogen          | √                       | √                  |                    | √               | √                    |               |
| Carbon Monoxide   | √                       | √                  |                    | √               | √                    |               |
| Oxygen            | √                       | √                  | √                  | √               | √                    | √             |
| i-Butane          | √                       | √                  | √                  |                 | √                    | √             |
| n-Butane          | √                       | √                  | √                  |                 | √                    | √             |
| i-Pentane         | √                       | √                  | √                  |                 | √                    | √             |
| n-Pentane         | √                       | √                  | √                  |                 | √                    | √             |
| n-Hexane          | √                       | √                  | √                  |                 | √                    | √             |
| n-Heptane         | √                       | √                  | √                  |                 | √                    | √             |
| n-Octane          | √                       | √                  | √                  |                 | √                    |               |
| n-Nonane          | √                       | √                  | √                  |                 | √                    |               |
| n-Decane          | √                       | √                  | √                  |                 | √                    |               |
| Helium            | √                       | √                  | √                  | √               | √                    |               |
| Argon             | √                       | √                  |                    |                 | √                    |               |
| Neo-Pentane       | (1)                     | √                  | (1)                |                 | (1)                  | (1)           |

1) Depending on function input 'Neo-Pentane mode' the value is added to i-Pentane or n-Pentane or it is neglected.

2) GPA2172 uses the specified water fraction for wet gas calculation only.

3) MR113 requires the input water fraction to be 0. The output water fraction is calculated from absolute humidity

## 6 Revisions

### Revision A

Date March 2017

- Initial, release
- Added IUPAC Ethylene and IAWS-IF97 functions
- Updated and corrected IO functions, moved to separate chapter.
- Updated incorrect page-header in TOC.
- Removed PPRV output from fxPeriodLatch(..) function.
- Added extended ISO6976 function that takes all 55 components of the standard
- Added GERG2004 and GERG2008 functions
- Minor editorial changes
- Added new natural gas viscosity calculation
- Added C11 – C21 components to the extended ISO6976 functions
- Added “Quarter circle” and “Conical entrance” orifice calculations
- Added GSSSD method MR 113-03 function
- Raised the pressure limit of API 2004 functions (tables 53, 54, 59, 60) from 150 to 250 bar.
- Removed duplicated functions.
- Added GOST30319 calculations.

### Revision B

Date November 2017

- Update to new ABB lay-out
- New document code: CM/FlowX/FR-EN
- Reintroduce revisions chapter

### Revision C

Date March 2018

- New calculations are added.
- Various existing functions are corrected.



---

**ABB B.V.****Measurement & Analytics**

Prof. Dr. Dorgelolaan 20  
5613 AM Eindhoven  
The Netherlands  
Phone: +31 40 236 9445  
Mail: [nl-spiritit-sales@abb.com](mailto:nl-spiritit-sales@abb.com)

**ABB Malaysia Sdn Bhd.****Measurement & Analytics**

Lot 608, Jalan SS 13/1K  
47500 Subang Jaya  
Selangor Darul Ehsan, Malaysia  
Phone: +60 3 5628 4888

[abb.com/midstream](http://abb.com/midstream)

**ABB Inc.****Measurement & Analytics**

7051 Industrial Boulevard  
Bartlesville OK 74006  
United States of America  
Phone: +1 800 442 3097

**ABB Limited****Measurement & Analytics**

Oldends Lane, Stonehouse  
Gloucestershire, GL10 3TA  
United Kingdom  
Phone: +44 7730 019 180



---

We reserve the right to make technical changes or modify the contents of this document without prior notice. With regard to purchase orders, the agreed particulars shall prevail. ABB AG does not accept any responsibility whatsoever for potential errors or possible lack of information in this document.

We reserve all rights in this document and in the subject matter and illustrations contained therein. Any reproduction, disclosure to third parties or utilization of its contents – in whole or in parts – is forbidden without prior written consent of ABB.

© ABB 2017